

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072716\
 Data File : BM006684.D
 Acq On : 27 Jul 2016 12:44
 Operator : UM/SJ
 Sample : PB92459BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK59

Quant Time: Jul 28 01:26:09 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 28 01:25:43 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	113162	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	489590	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	284099	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	651932	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	800437	20.00	ng/ul	0.00
83) Perylene-d12	23.42	264	848654	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	13937	4.79	ng/uL	0.00
5) Phenol-d5	6.79	99	334229	33.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	214878	35.17	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	262537	33.65	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	264913	33.96	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	129616	34.29	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	141250	34.59	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	238333	31.83	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	377776	49.67	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	842207	37.15	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	1001236	35.13	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	132573	33.99	ng/ul	0.00
57) Fluorene-d10	15.26	176	703037	35.75	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	109869	30.92	ng/ul	0.00
70) Anthracene-d10	17.11	188	1162020	38.20	ng/ul	0.00
76) Pyrene-d10	19.42	212	1343348	36.18	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.28	264	1489881	38.79	ng/ul	0.00


Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	8.32	70	7094	1.07 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072716\
Data File : BM006684.D
Acq On : 27 Jul 2016 12:44
Operator : UM/SJ
Sample : PB92459BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK59

Quant Time: Jul 28 01:26:09 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 28 01:25:43 2016
Response via : Initial Calibration

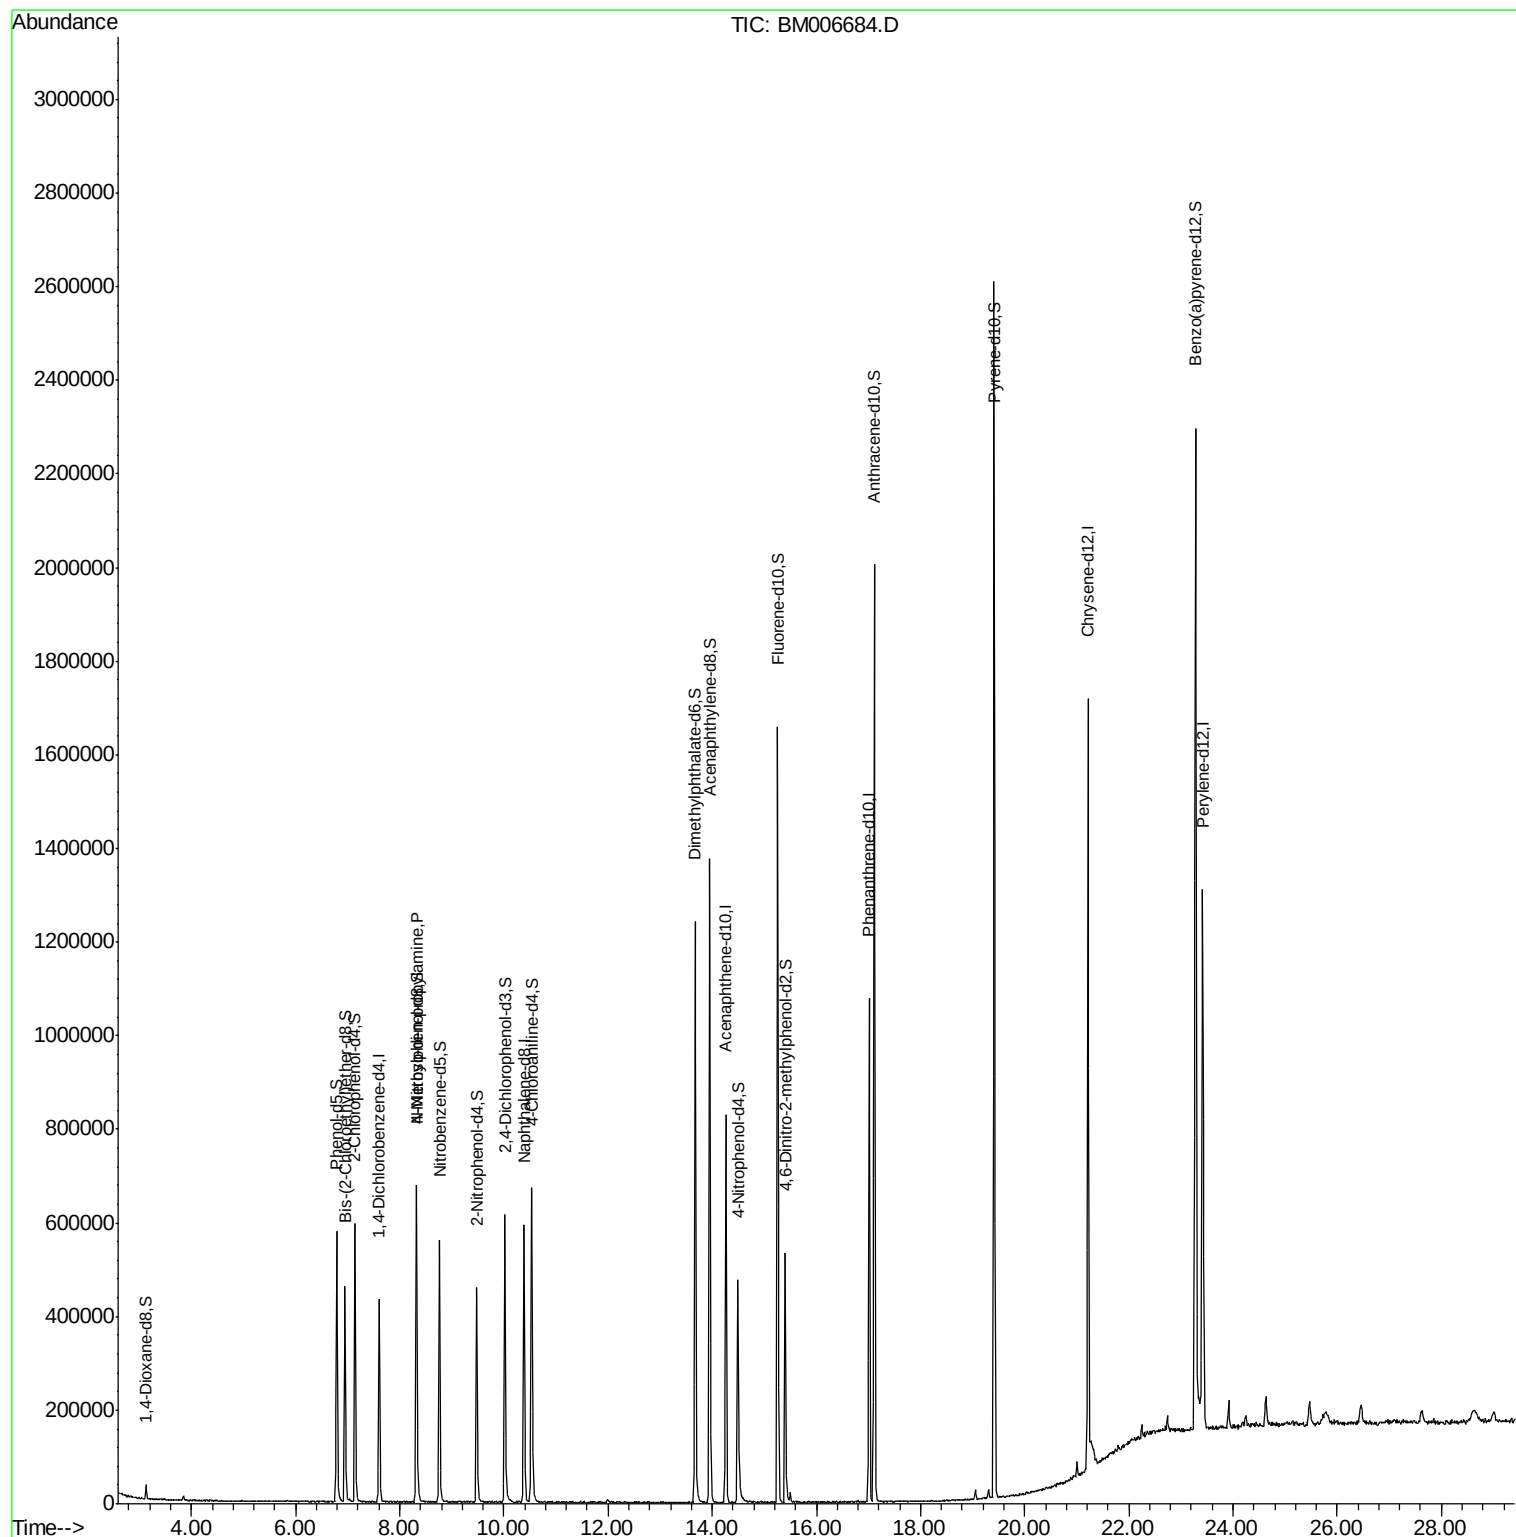

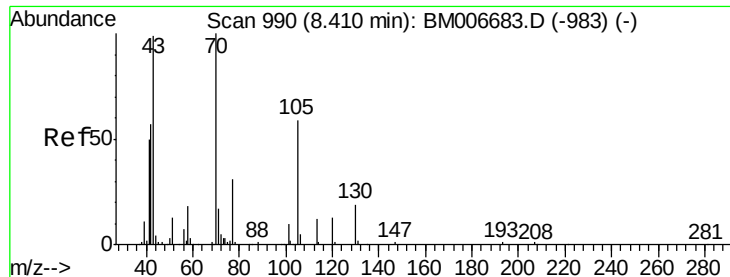

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.07 ng/ul
 RT: 8.32 min Scan# 975
 Delta R.T. -0.09 min
 Lab File: BM006684.D
 Acq: 27 Jul 2016 12:44

Instrument :
 BNA_M
 ClientSampleId :
 SBLK59

Tgt Ion:	70	Resp:	7094
Ion	Ratio	Lower	Upper
70	100		
42	354.9	50.6	75.8#
101	0.0	7.9	11.9#
130	0.0	15.8	23.6#

