

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072716\
 Data File : BM006685.D
 Acq On : 27 Jul 2016 13:20
 Operator : UM/SJ
 Sample : PB92315BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK15

Quant Time: Jul 28 01:26:17 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 28 01:25:43 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	120362	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	496906	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	283119	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	641233	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	793931	20.00	ng/ul	0.00
83) Perylene-d12	23.41	264	830109	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	13938	4.50	ng/uL	0.00
5) Phenol-d5	6.79	99	348162	32.90	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	223164	34.34	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	272103	32.79	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	267885	32.28	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	129496	33.76	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	142445	34.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	240292	31.62	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	353915	45.85	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	835708	36.99	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	985212	34.68	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	127838	32.89	ng/ul	0.00
57) Fluorene-d10	15.26	176	696311	35.53	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	107028	30.62	ng/ul	0.00
70) Anthracene-d10	17.11	188	1152016	38.50	ng/ul	0.00
76) Pyrene-d10	19.42	212	1318631	35.80	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.28	264	1454456	38.72	ng/ul	0.00


Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	8.32	70	7073	1.00 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072716\
Data File : BM006685.D
Acq On : 27 Jul 2016 13:20
Operator : UM/SJ
Sample : PB92315BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK15

Quant Time: Jul 28 01:26:17 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 28 01:25:43 2016
Response via : Initial Calibration

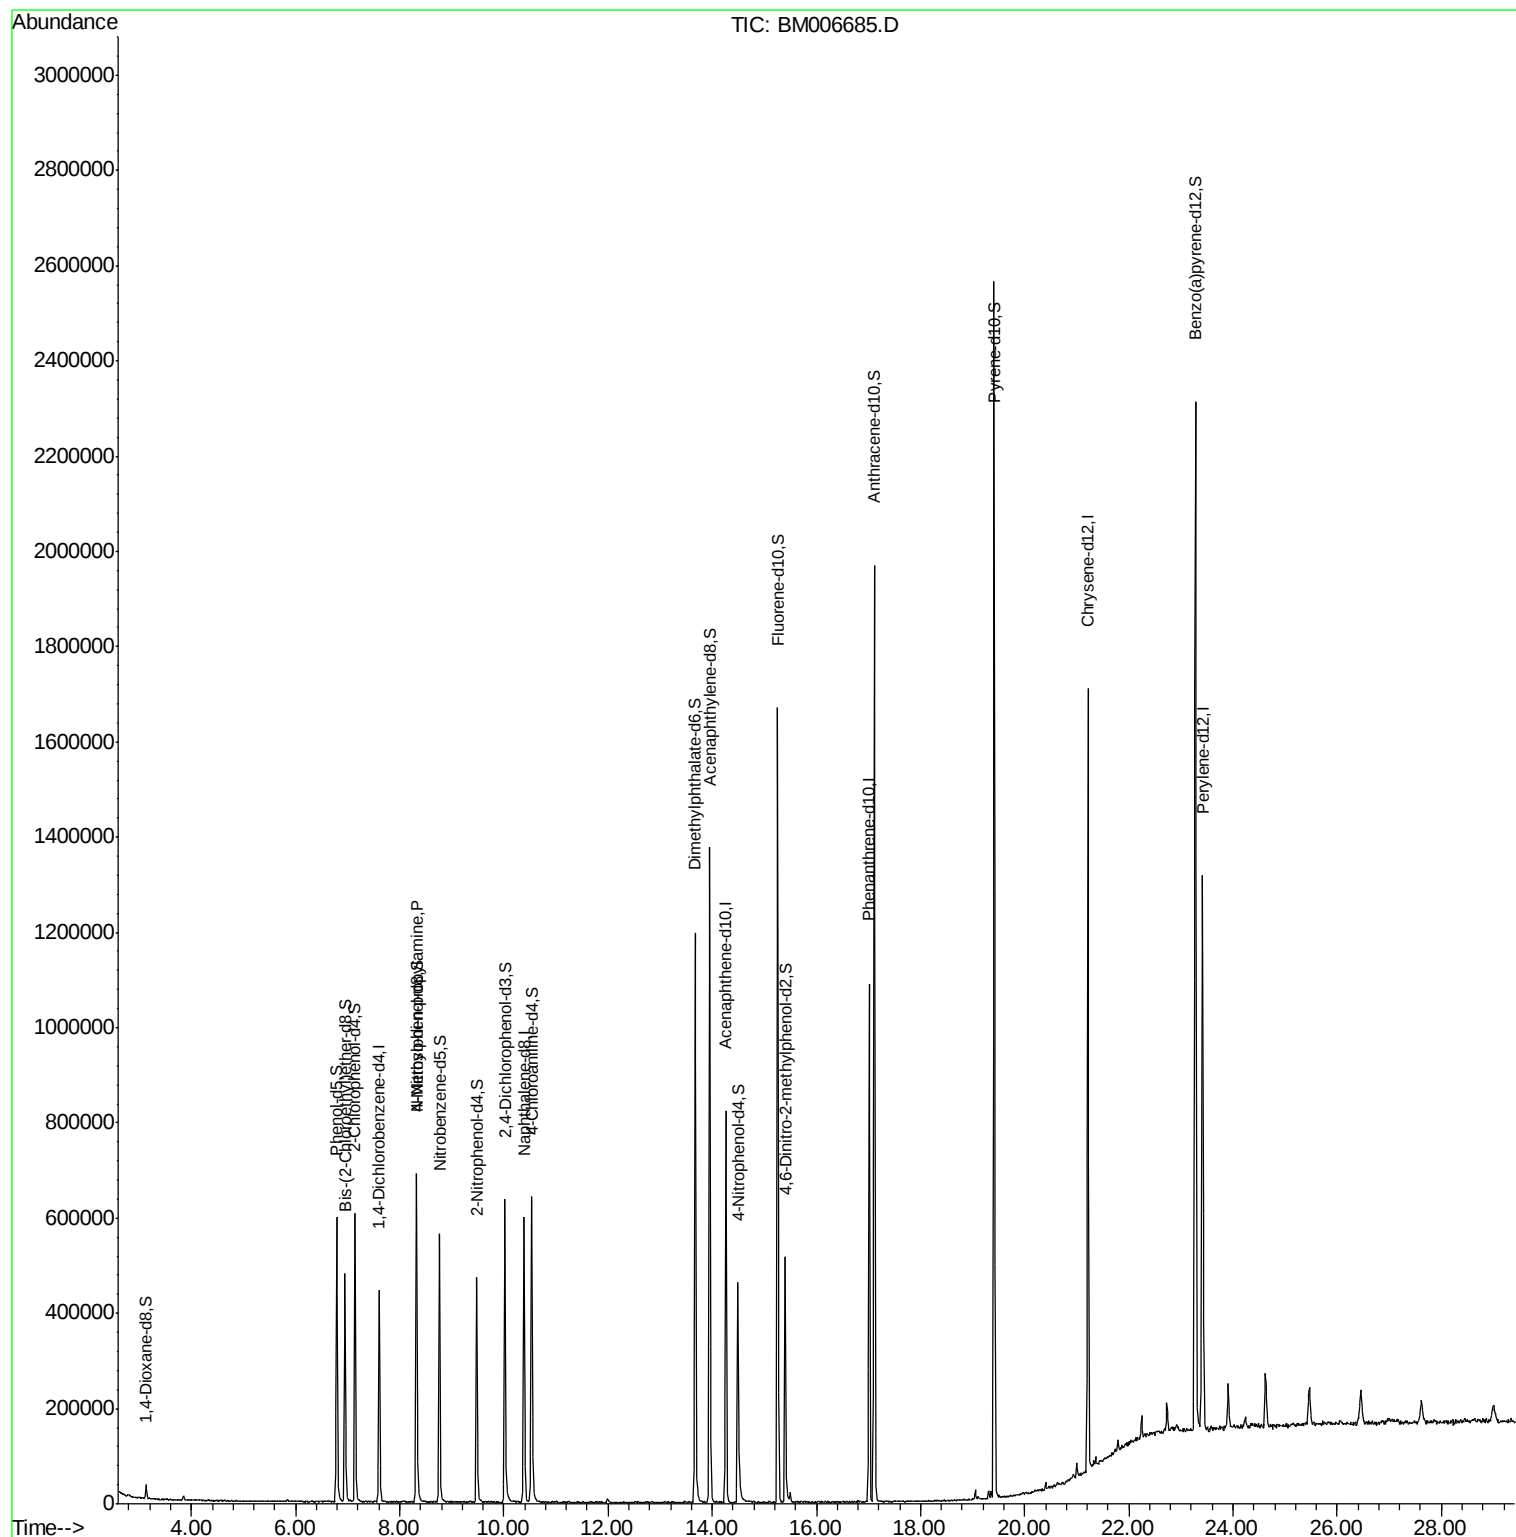

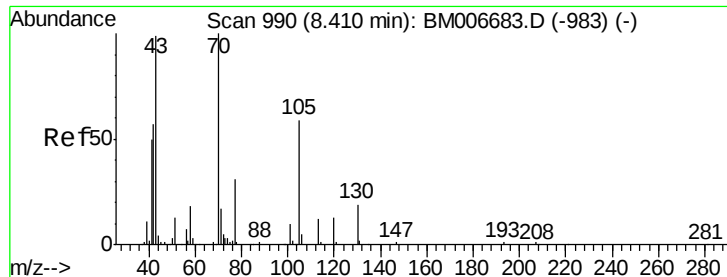

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.00 ng/ul
 RT: 8.32 min Scan# 974
 Delta R.T. -0.09 min
 Lab File: BM006685.D
 Acq: 27 Jul 2016 13:20

Instrument :
 BNA_M
 ClientSampleId :
 SBLK15

Tgt Ion: 70 Resp: 7073
 Ion Ratio Lower Upper
 70 100
 42 420.6 50.6 75.8#
 101 0.0 7.9 11.9#
 130 0.0 15.8 23.6#

