

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072716\
 Data File : BM006691.D
 Acq On : 27 Jul 2016 16:58
 Operator : UM/SJ
 Sample : H4094-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJE4

Quant Time: Jul 28 01:27:00 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 28 01:25:43 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	141499	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	617621	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	347142	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.01	188	798725	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	955217	20.00	ng/ul	0.00
83) Perylene-d12	23.42	264	991735	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	8553	2.35	ng/uL	0.00
5) Phenol-d5	6.79	99	330679	26.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	214820	28.12	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	255996	26.24	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	263036	26.96	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	125248	26.27	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	135744	26.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	236394	25.03	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	351812	36.67	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	768838	27.76	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	957869	27.50	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	92287	19.36	ng/ul	0.00
57) Fluorene-d10	15.26	176	672836	28.00	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	68317	15.69	ng/ul	0.00
70) Anthracene-d10	17.11	188	1060007	28.44	ng/ul	0.00
76) Pyrene-d10	19.42	212	1229149	27.74	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.27	264	1329381	29.62	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
6) Phenol	6.82	94	15445	1.17	ng/ul#	81
44) Dimethylphthalate	13.72	163	427605	15.43	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072716\
Data File : BM006691.D
Acq On : 27 Jul 2016 16:58
Operator : UM/SJ
Sample : H4094-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJE4

Quant Time: Jul 28 01:27:00 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 28 01:25:43 2016
Response via : Initial Calibration

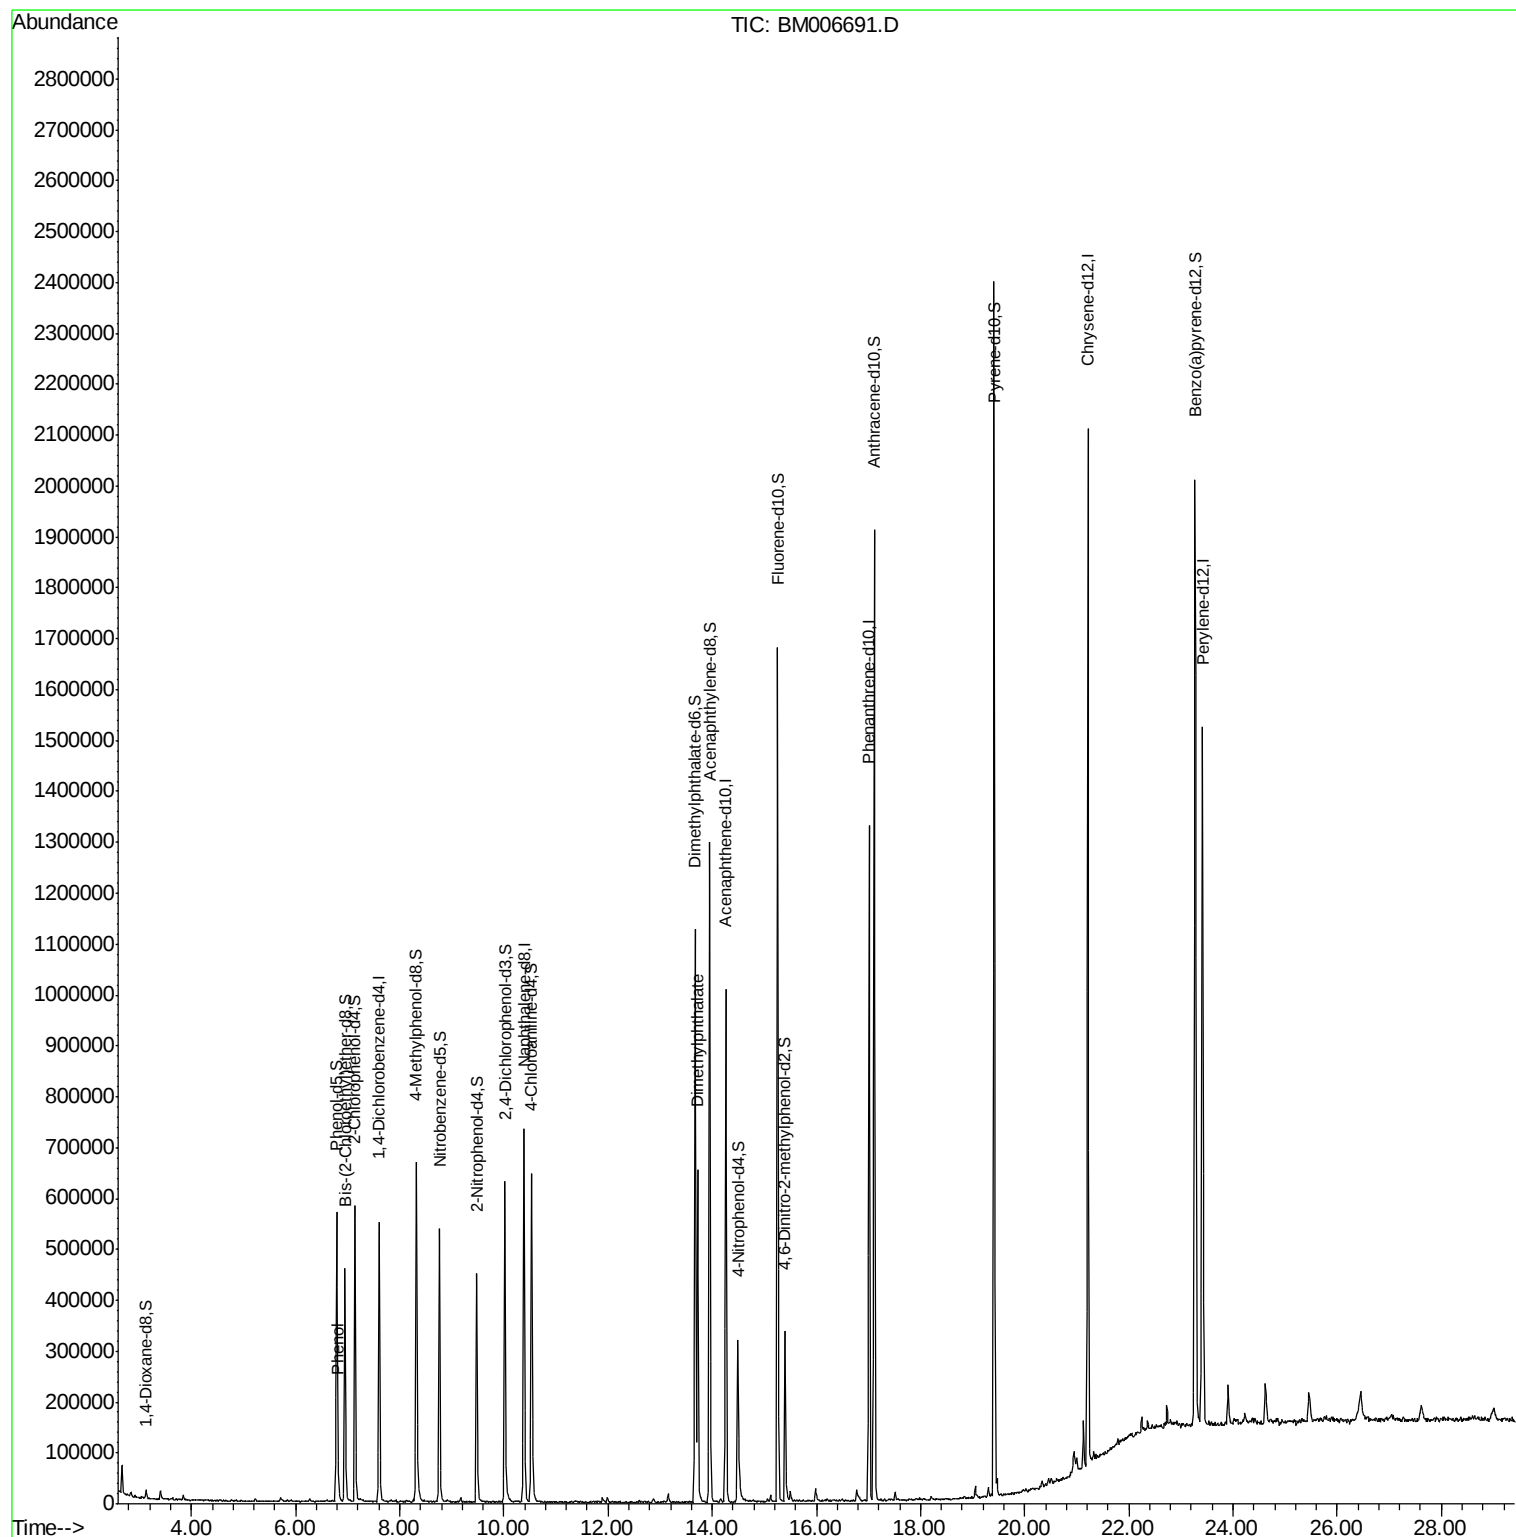

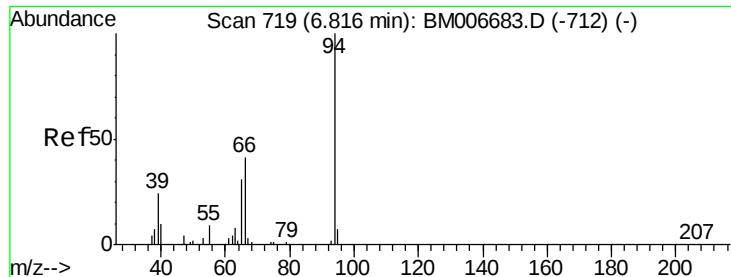

#6

Phenol

Concen: 1.17 ng/ul

RT: 6.82 min Scan# 719

Delta R.T. 0.00 min

Lab File: BM006691.D

Acq: 27 Jul 2016 16:58

Instrument :

BNA_M

ClientSampleId :

BDJE4


Tgt Ion: 94 Resp: 15445

Ion Ratio Lower Upper

94 100

65 41.2 25.8 38.8#




66 58.1 35.7 53.5#

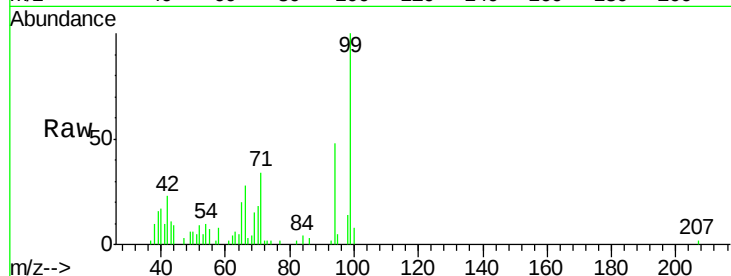

Abundance Ion 94.00 (93.70 to 94.70): BM006683.D (-712) (-)

Ion 65.00 (64.70 to 65.70): BM006683.D (-712) (-)

Ion 66.00 (65.70 to 66.70): BM006683.D (-712) (-)

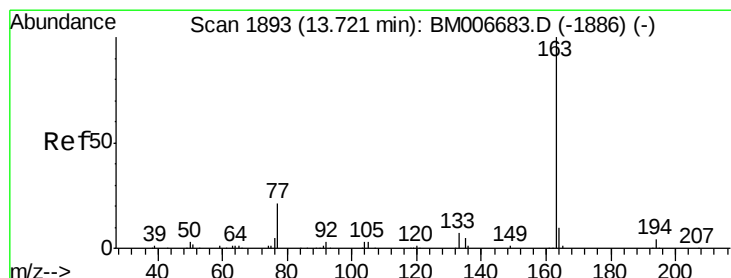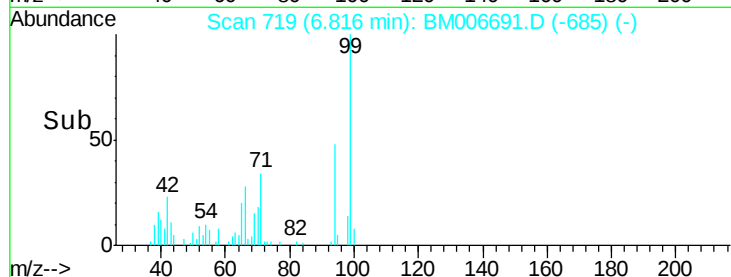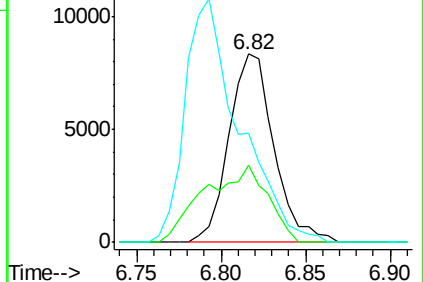

#44

Dimethylphthalate

Concen: 15.43 ng/ul

RT: 13.72 min Scan# 1893

Delta R.T. 0.00 min

Lab File: BM006691.D

Acq: 27 Jul 2016 16:58


Tgt Ion: 163 Resp: 427605

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.0

164 9.8 7.8 11.8

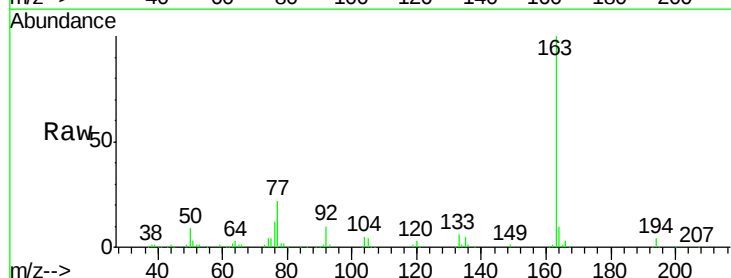

Abundance Ion 163.00 (162.70 to 163.70): BM006683.D (-1886) (-)

Ion 194.00 (193.70 to 194.70): BM006683.D (-1886) (-)

Ion 164.00 (163.70 to 164.70): BM006683.D (-1886) (-)

