

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072716\
 Data File : BM006693.D
 Acq On : 27 Jul 2016 18:10
 Operator : UM/SJ
 Sample : PB92425BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK25

Quant Time: Jul 28 01:27:35 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 28 01:25:43 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	128894	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	544539	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	314193	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	724417	20.00	ng/ul	0.00
75) Chrysene-d12	21.21	240	873980	20.00	ng/ul	0.00
83) Perylene-d12	23.41	264	901695	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	15283	4.61	ng/uL	0.00
5) Phenol-d5	6.79	99	375658	33.15	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	241675	34.73	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	301689	33.95	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	294597	33.15	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	143406	34.11	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	157753	34.73	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	271019	32.55	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	379707	44.89	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	934456	37.27	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	1106844	35.11	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	149464	34.65	ng/ul	0.00
57) Fluorene-d10	15.26	176	779685	35.85	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	126223	31.97	ng/ul	0.00
70) Anthracene-d10	17.11	188	1292413	38.23	ng/ul	0.00
76) Pyrene-d10	19.42	212	1473438	36.34	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.28	264	1594943	39.09	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
15) N-Nitroso-di-n-propylamine	8.32	70	7681	1.01	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072716\
Data File : BM006693.D
Acq On : 27 Jul 2016 18:10
Operator : UM/SJ
Sample : PB92425BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK25

Quant Time: Jul 28 01:27:35 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 28 01:25:43 2016
Response via : Initial Calibration

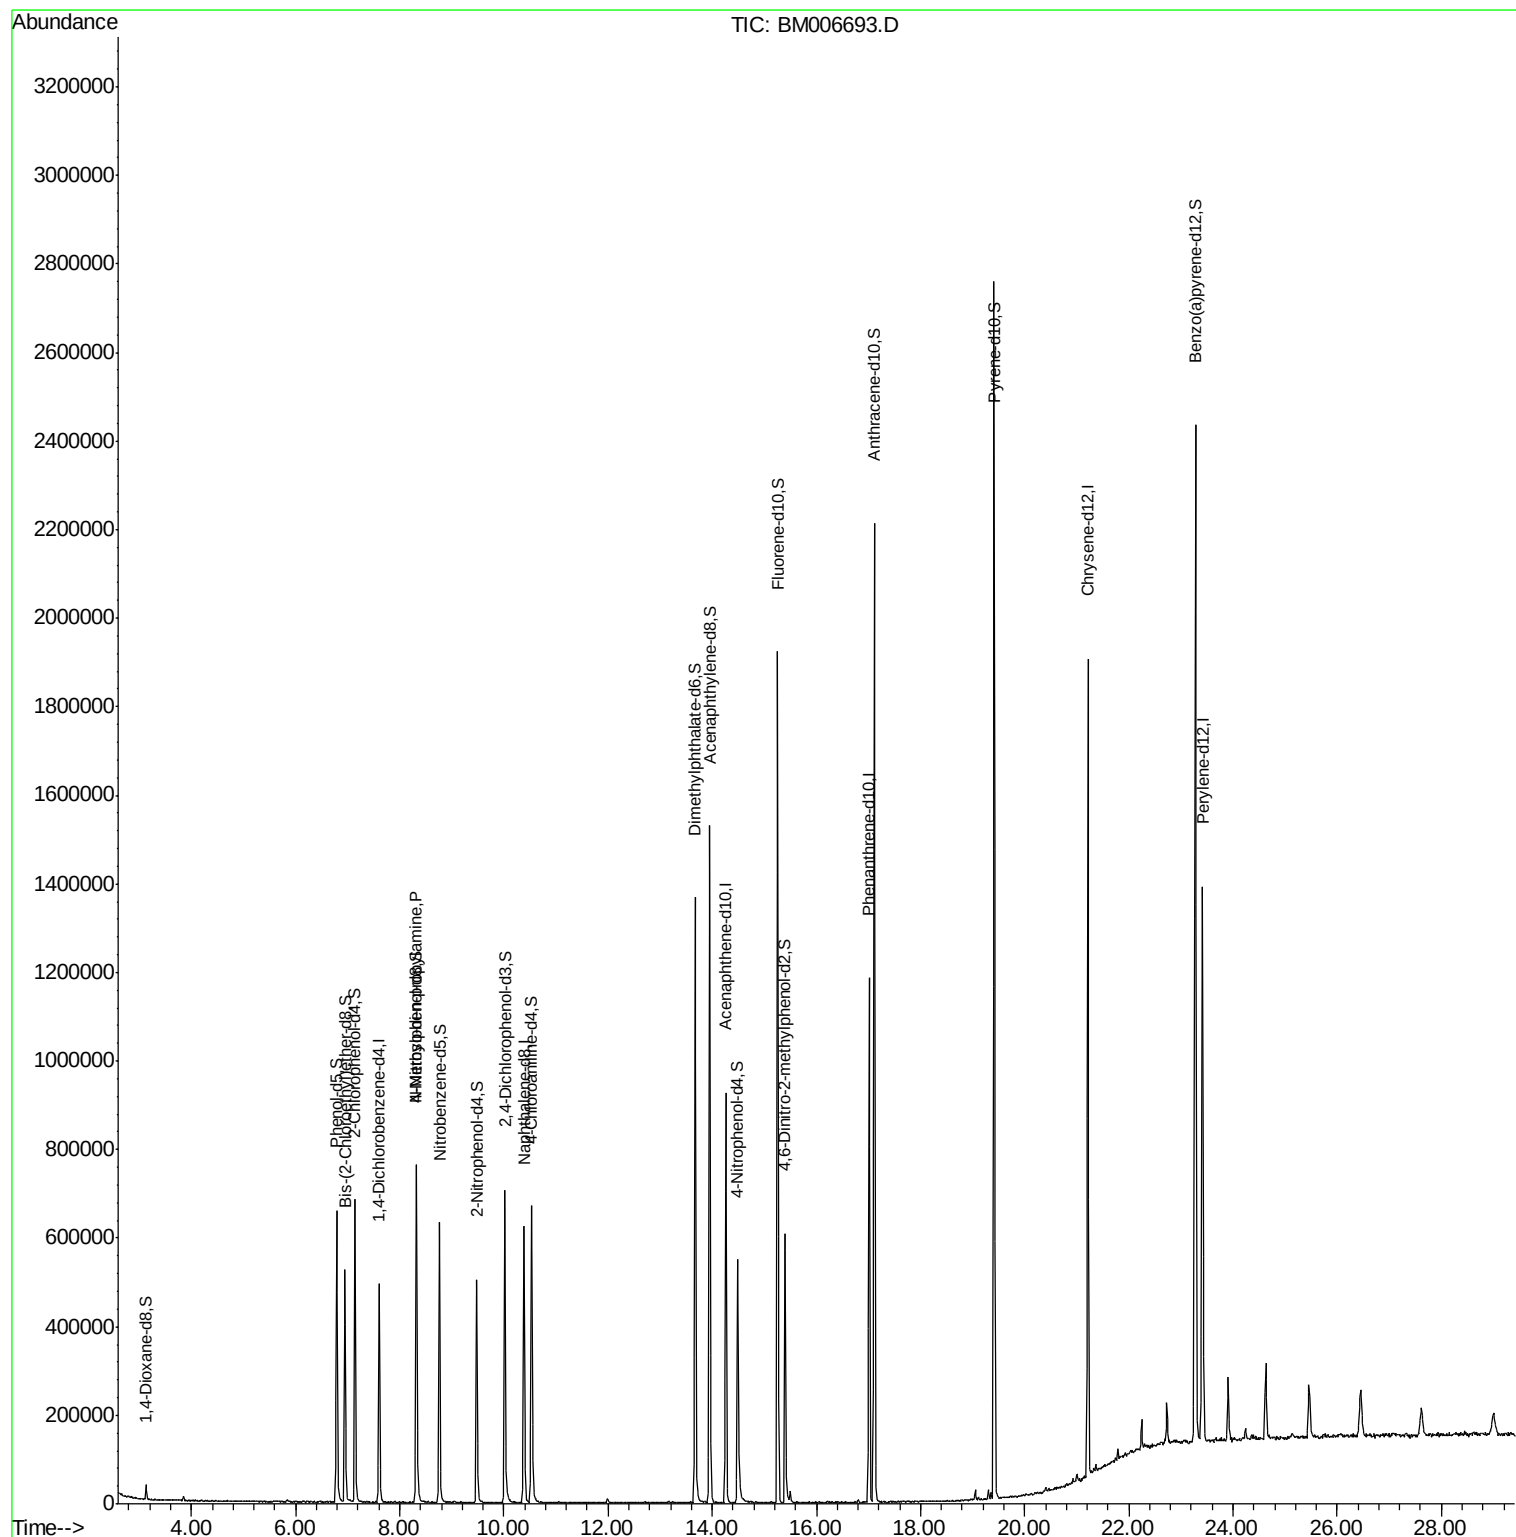

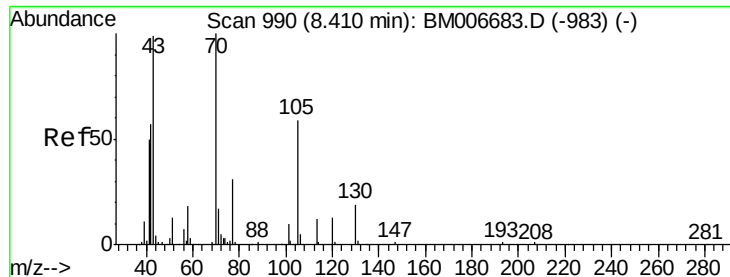

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.01 ng/ul
 RT: 8.32 min Scan# 974
 Delta R.T. -0.09 min
 Lab File: BM006693.D
 Acq: 27 Jul 2016 18:10

Instrument :
 BNA_M
 ClientSampleId :
 SBLK25

Tgt Ion:	70	Resp:	7681
Ion	Ratio	Lower	Upper
70	100		
42	394.8	50.6	75.8#
101	0.0	7.9	11.9#
130	0.0	15.8	23.6#

