

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072716\
 Data File : BM006698.D
 Acq On : 27 Jul 2016 21:12
 Operator : UM/SJ
 Sample : H4094-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJE9

Quant Time: Jul 28 01:28:12 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 28 01:25:43 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	161699	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	707554	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	412499	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.01	188	945199	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	1110928	20.00	ng/ul	0.00
83) Perylene-d12	23.41	264	1165079	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	8259	1.98	ng/uL	0.00
5) Phenol-d5	6.79	99	330744	23.27	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	213265	24.43	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	262173	23.52	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	263520	23.64	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	128832	23.59	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	139854	23.70	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	243926	22.54	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	368192	33.50	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	824270	25.04	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	1020994	24.67	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	82246	14.52	ng/ul	0.00
57) Fluorene-d10	15.26	176	720713	25.24	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	68607	13.32	ng/ul	0.00
70) Anthracene-d10	17.11	188	1129878	25.62	ng/ul	0.00
76) Pyrene-d10	19.42	212	1303266	25.29	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.28	264	1403325	26.62	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.72	163	452077	13.73	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072716\
Data File : BM006698.D
Acq On : 27 Jul 2016 21:12
Operator : UM/SJ
Sample : H4094-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJE9

Quant Time: Jul 28 01:28:12 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 28 01:25:43 2016
Response via : Initial Calibration

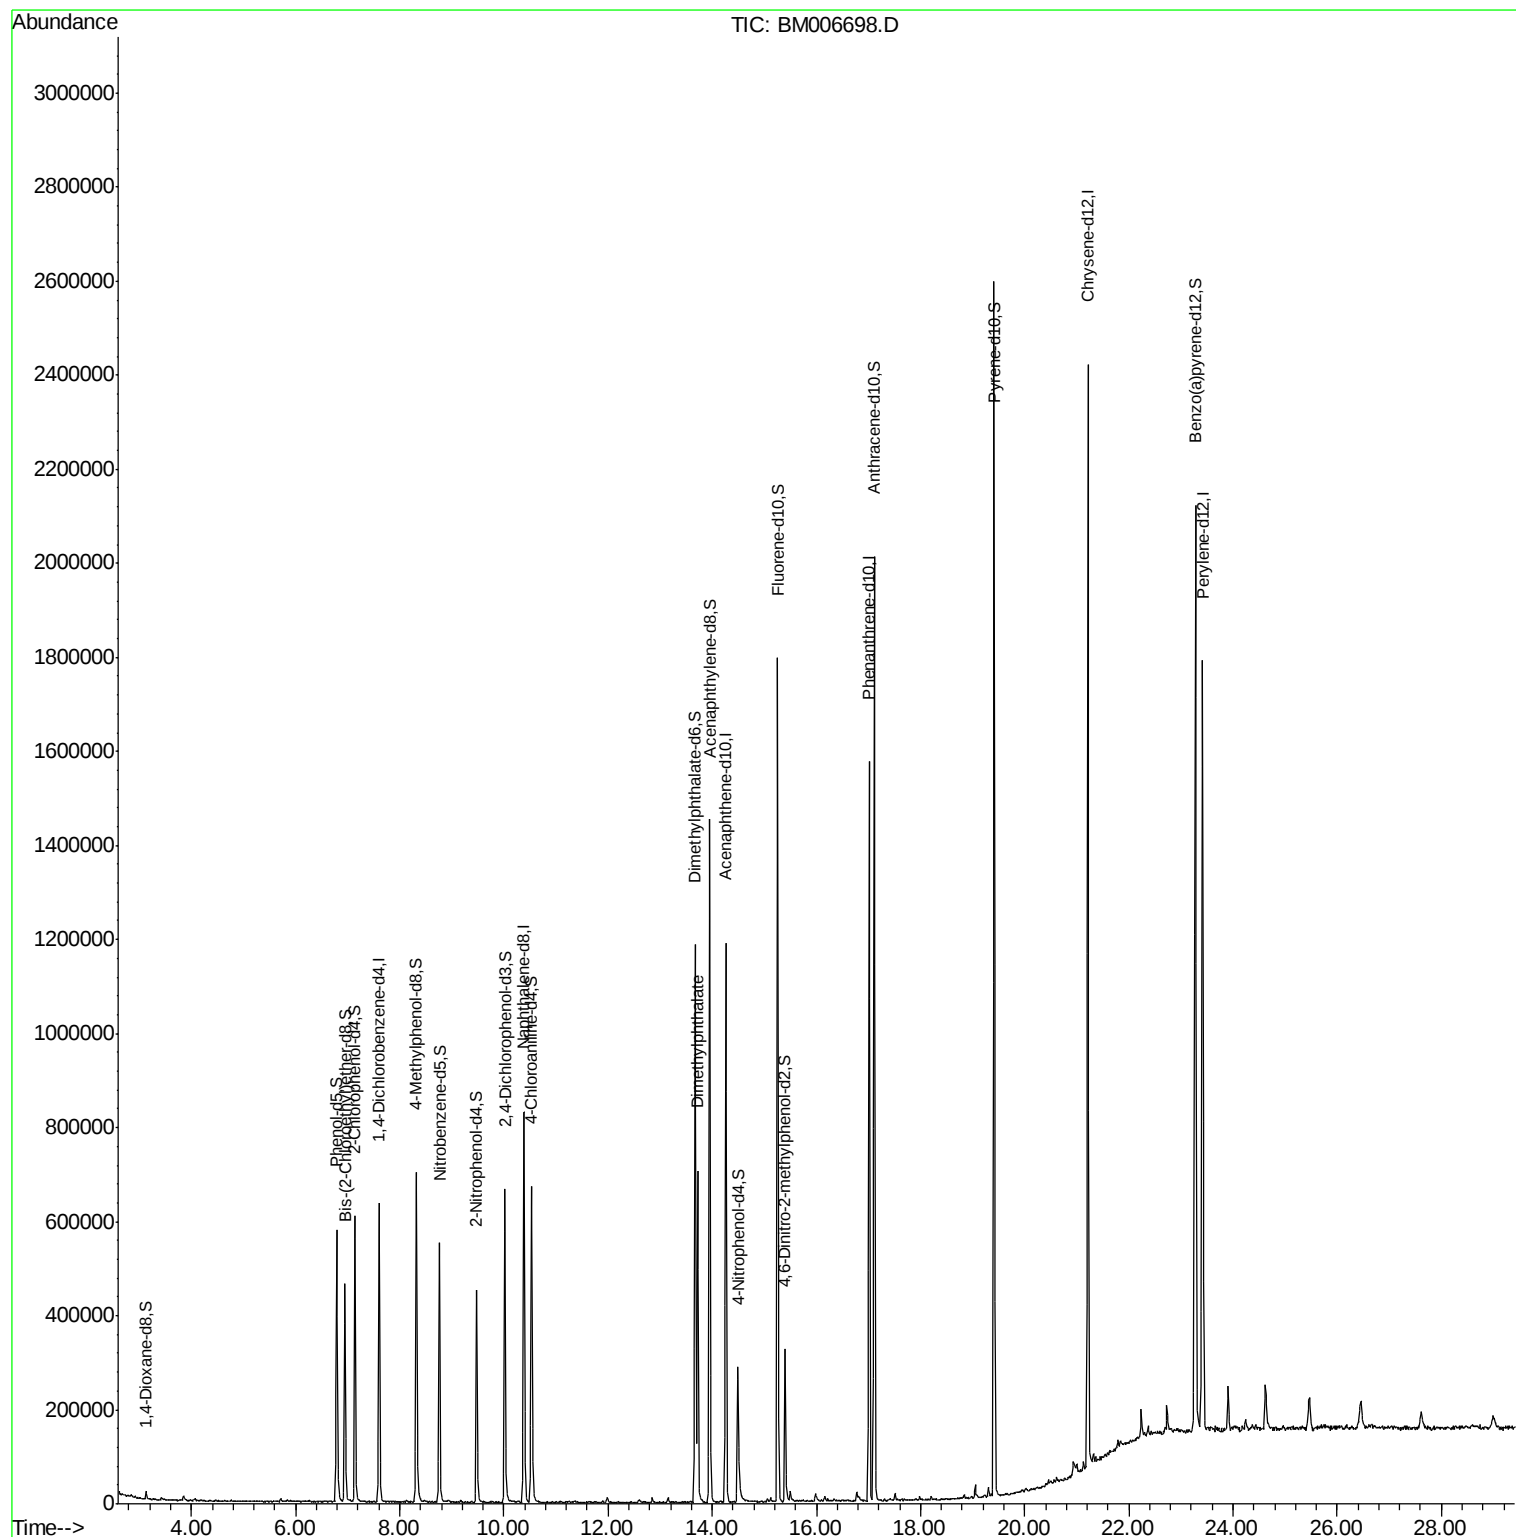

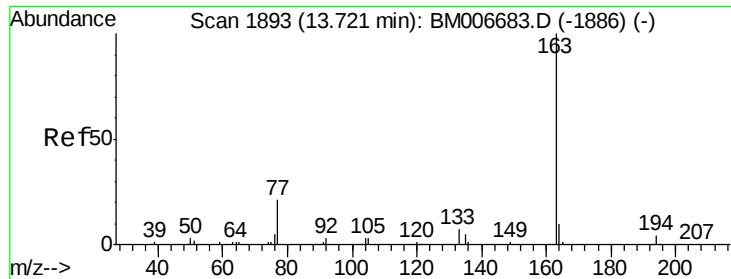

#44

Dimethylphthalate

Concen: 13.73 ng/ul

RT: 13.72 min Scan# 1893

Delta R.T. -0.00 min

Lab File: BM006698.D


Acq: 27 Jul 2016 21:12

Instrument :

BNA_M

ClientSampleId :

BDJE9

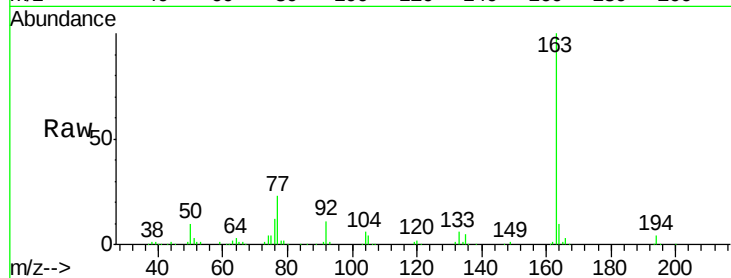

Tgt Ion:163 Resp: 452077

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.0

164 10.0 7.8 11.8

