

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072716\
 Data File : BM006699.D
 Acq On : 27 Jul 2016 21:48
 Operator : UM/SJ
 Sample : H4094-15
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJF0

Quant Time: Jul 28 01:28:19 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 28 01:25:43 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	177182	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	775900	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	439592	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.01	188	1003418	20.00	ng/ul	0.00
75) Chrysene-d12	21.21	240	1170951	20.00	ng/ul	0.00
83) Perylene-d12	23.41	264	1227437	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	8787	1.93	ng/uL	0.00
5) Phenol-d5	6.79	99	360928	23.17	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	235491	24.62	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	286831	23.48	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	293776	24.05	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	138810	23.17	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	150925	23.32	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	267322	22.53	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	391440	32.48	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	887040	25.29	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	1071411	24.29	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	134889	22.35	ng/ul	0.00
57) Fluorene-d10	15.26	176	766318	25.19	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	99106	18.12	ng/ul	0.00
70) Anthracene-d10	17.11	188	1222301	26.10	ng/ul	0.00
76) Pyrene-d10	19.42	212	1365764	25.14	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.27	264	1466958	26.41	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	13.72	163	458173	13.06 ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072716\
Data File : BM006699.D
Acq On : 27 Jul 2016 21:48
Operator : UM/SJ
Sample : H4094-15
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJF0

Quant Time: Jul 28 01:28:19 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 28 01:25:43 2016
Response via : Initial Calibration

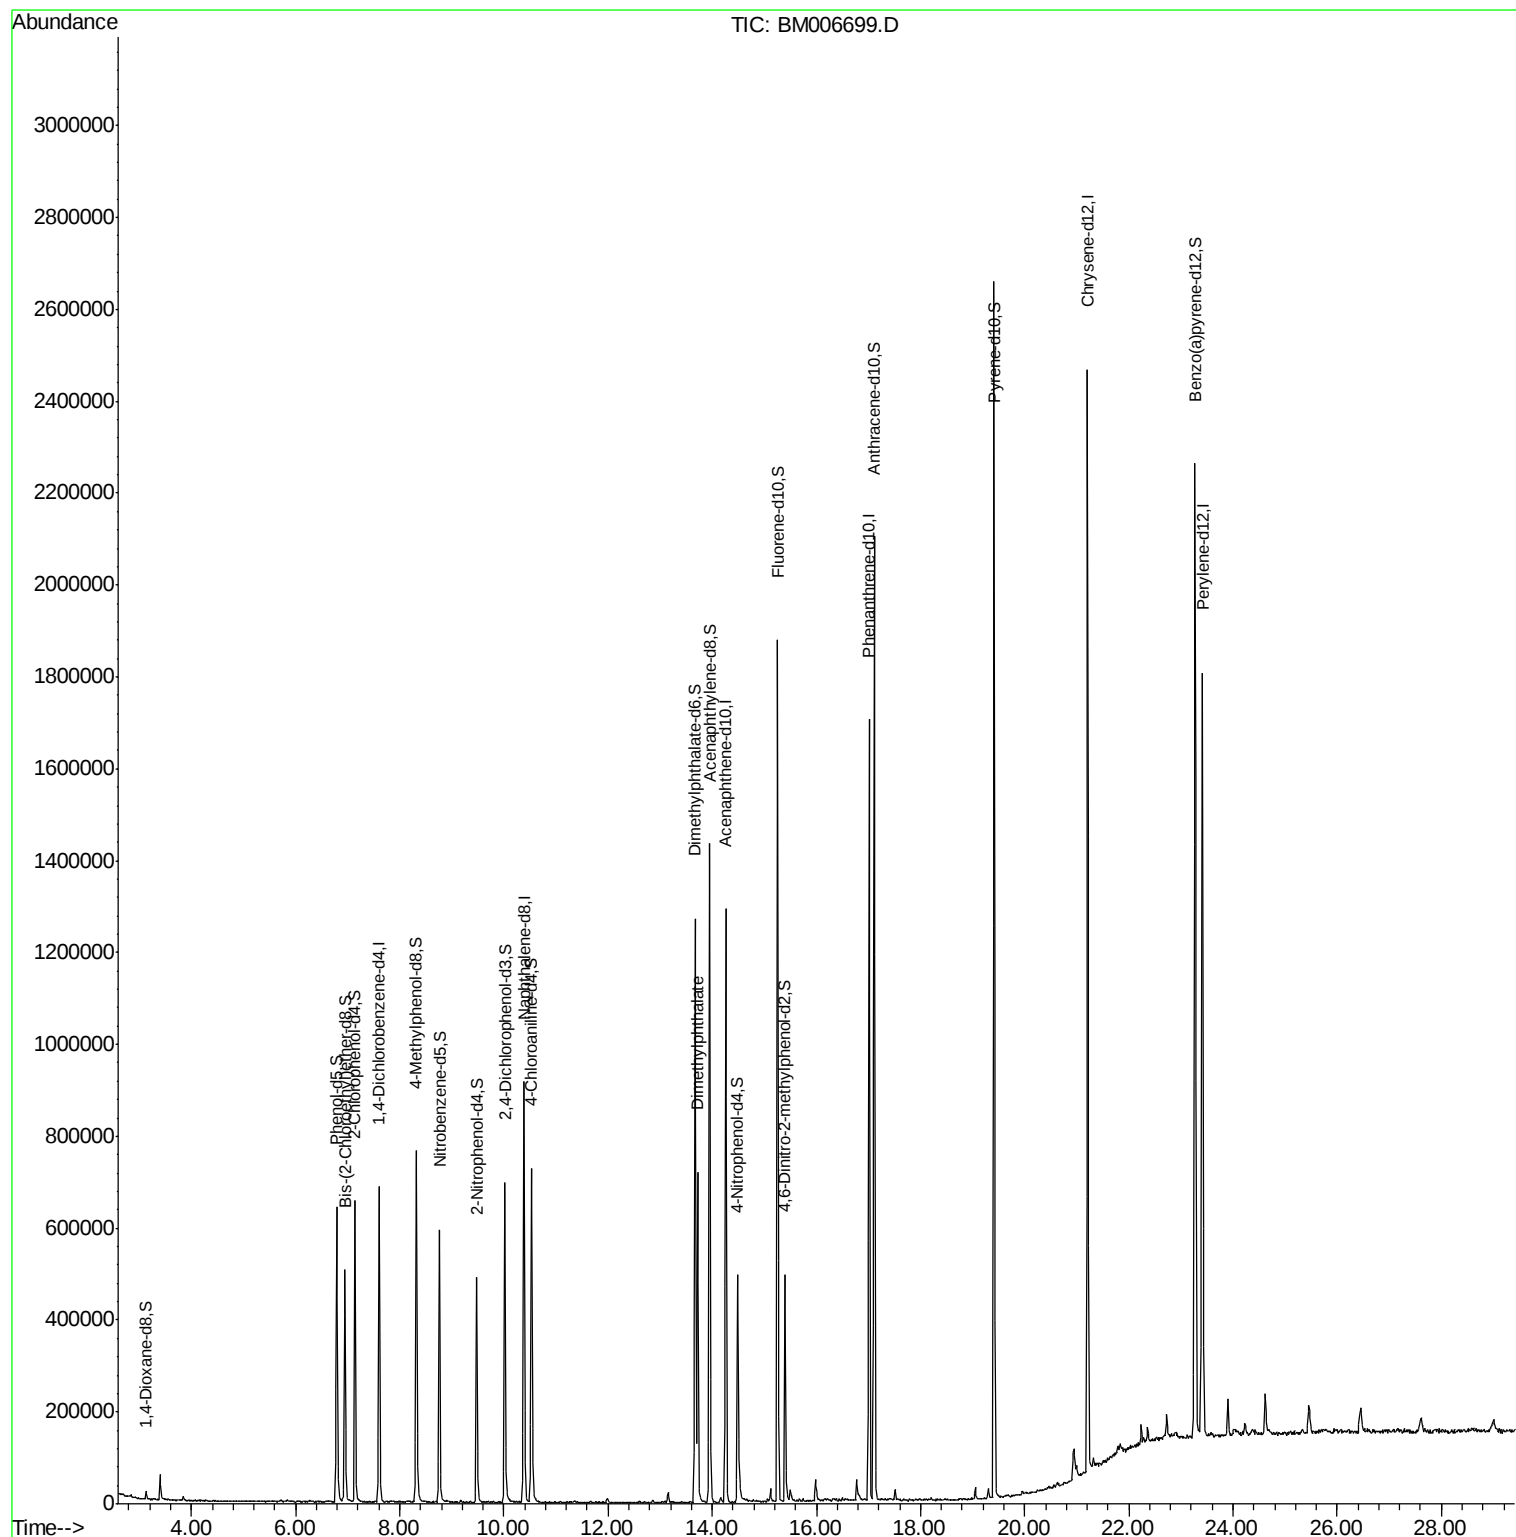

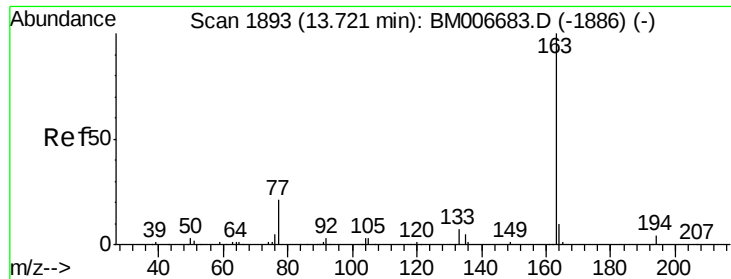

#44

Dimethylphthalate

Concen: 13.06 ng/ul

RT: 13.72 min Scan# 1893

Delta R.T. 0.00 min

Lab File: BM006699.D

Acq: 27 Jul 2016 21:48

Instrument :

BNA_M

ClientSampleId :

BDJF0


Tgt Ion:163 Resp: 458173

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.0

164 10.0 7.8 11.8

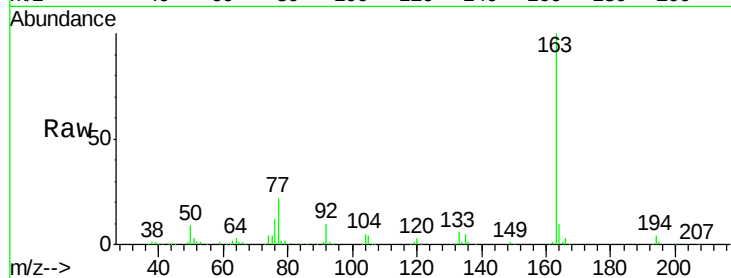

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

