

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072716\
 Data File : BM006696.D
 Acq On : 27 Jul 2016 19:59
 Operator : UM/SJ
 Sample : H4094-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJE6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.786	708	714	732	rBV	500676	881559	26.43%	2.486%
2	6.945	735	741	754	rVB	387627	616447	18.48%	1.738%
3	7.139	768	774	787	rBV	512044	839129	25.15%	2.366%
4	7.604	845	853	865	rBV	552338	926086	27.76%	2.611%
5	8.316	968	974	990	rBV	592288	1035397	31.04%	2.920%
6	8.763	1043	1050	1066	rBV	453072	804591	24.12%	2.269%
7	9.480	1165	1172	1186	rVB	387676	678945	20.35%	1.915%
8	10.016	1257	1263	1283	rBV	551757	1003485	30.08%	2.830%
9	10.386	1318	1326	1340	rBV	767583	1348010	40.41%	3.801%
10	10.527	1343	1350	1374	rVB	549818	1066032	31.95%	3.006%
11	13.674	1878	1885	1889	rBV	1039602	1534456	46.00%	4.327%
12	13.721	1889	1893	1902	rVB	547583	829414	24.86%	2.339%
13	13.951	1925	1932	1944	rBV	1175653	1827488	54.78%	5.153%
14	14.262	1978	1985	1998	rVB2	1083158	1754300	52.59%	4.947%
15	14.492	2018	2024	2043	rBV	274435	582916	17.47%	1.644%
16	15.257	2148	2154	2164	rBV	1602202	2306176	69.13%	6.503%
17	15.398	2173	2178	2192	rBV	323071	512697	15.37%	1.446%
18	15.980	2272	2277	2286	rBV2	28445	55953	1.68%	0.158%
19	16.774	2408	2412	2416	rBV2	23504	34217	1.03%	0.096%
20	17.015	2446	2453	2463	rBV2	1402048	2141228	64.18%	6.038%
21	17.109	2463	2469	2482	rVB2	1732442	2563435	76.84%	7.229%
22	19.415	2855	2861	2874	rBV2	2192546	3125366	93.68%	8.813%
23	20.950	3117	3122	3127	rBV5	31680	72832	2.18%	0.205%
24	21.215	3161	3167	3176	rBV	2086847	2809638	84.22%	7.923%
25	23.274	3510	3517	3532	rVV2	1765475	3336069	100.00%	9.407%
26	23.415	3534	3541	3551	rVB	1463572	2776738	83.23%	7.830%


Sum of corrected areas: 35462604

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072716\
Data File : BM006696.D
Acq On : 27 Jul 2016 19:59
Operator : UM/SJ
Sample : H4094-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJE6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

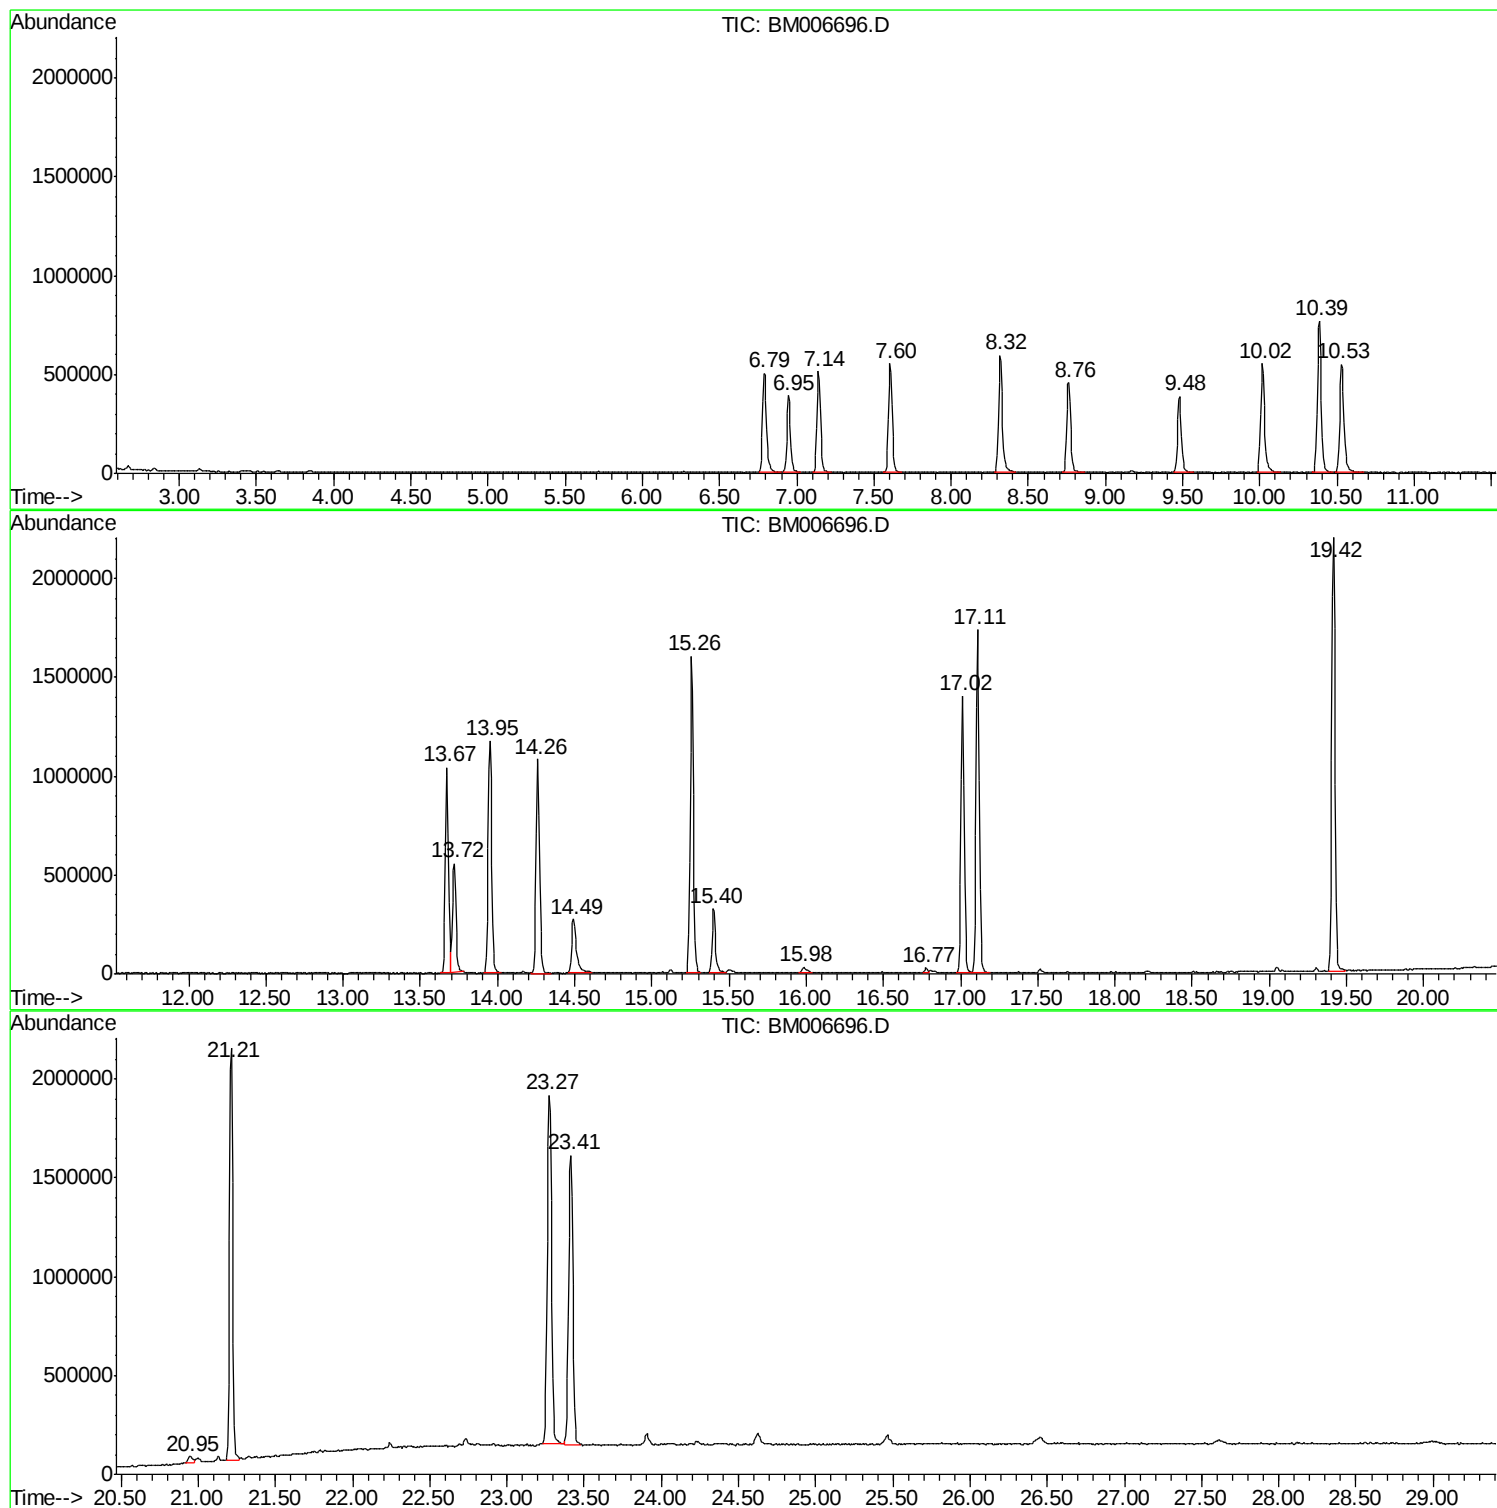

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072716\
Data File : BM006696.D
Acq On : 27 Jul 2016 19:59
Operator : UM/SJ
Sample : H4094-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJE6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072716\
Data File : BM006696.D
Acq On : 27 Jul 2016 19:59
Operator : UM/SJ
Sample : H4094-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJE6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc