

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072716\
 Data File : BM006700.D
 Acq On : 27 Jul 2016 22:24
 Operator : UM/SJ
 Sample : H4094-16
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJF1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.787	708	714	731	rBV	661784	1125174	26.56%	2.506%
2	6.945	731	741	754	rBV	523685	830214	19.60%	1.849%
3	7.139	768	774	795	rVB	681804	1119908	26.44%	2.494%
4	7.604	845	853	862	rBV	664850	1089738	25.73%	2.427%
5	8.316	968	974	983	rBV	799053	1356593	32.03%	3.021%
6	8.757	1042	1049	1064	rBV	617136	1078713	25.47%	2.402%
7	9.475	1164	1171	1190	rVB	507233	910826	21.50%	2.028%
8	10.016	1256	1263	1276	rBV	742622	1335078	31.52%	2.973%
9	10.386	1317	1326	1343	rBV	895800	1594623	37.65%	3.551%
10	10.527	1343	1350	1370	rVB	750107	1437984	33.95%	3.202%
11	13.674	1878	1885	1889	rBV	1366754	2058017	48.59%	4.583%
12	13.721	1889	1893	1901	rVB	748922	1108948	26.18%	2.469%
13	13.951	1923	1932	1948	rBV	1573911	2428216	57.33%	5.407%
14	14.262	1977	1985	1995	rBV2	1239683	2047116	48.33%	4.559%
15	14.492	2017	2024	2042	rBV	413871	822244	19.41%	1.831%
16	15.257	2147	2154	2164	rBV	2039162	3038103	71.73%	6.765%
17	15.398	2172	2178	2190	rBV	442709	686095	16.20%	1.528%
18	15.498	2190	2195	2204	rVB3	25702	44326	1.05%	0.099%
19	17.009	2446	2452	2463	rBV2	1636341	2498407	58.98%	5.564%
20	17.109	2463	2469	2483	rVB2	2258014	3379785	79.79%	7.526%
21	19.415	2855	2861	2869	rBV2	2770253	4005703	94.57%	8.920%
22	21.215	3161	3167	3177	rBV	2377132	3188636	75.28%	7.101%
23	23.274	3510	3517	3529	rVB2	2253350	4235673	100.00%	9.432%
24	23.415	3534	3541	3554	rVB	1658982	3170336	74.85%	7.060%
25	23.909	3620	3625	3634	rVB3	77905	158371	3.74%	0.353%
26	24.627	3743	3747	3754	rVB2	79731	157036	3.71%	0.350%


Sum of corrected areas: 44905863

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072716\
Data File : BM006700.D
Acq On : 27 Jul 2016 22:24
Operator : UM/SJ
Sample : H4094-16
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJF1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

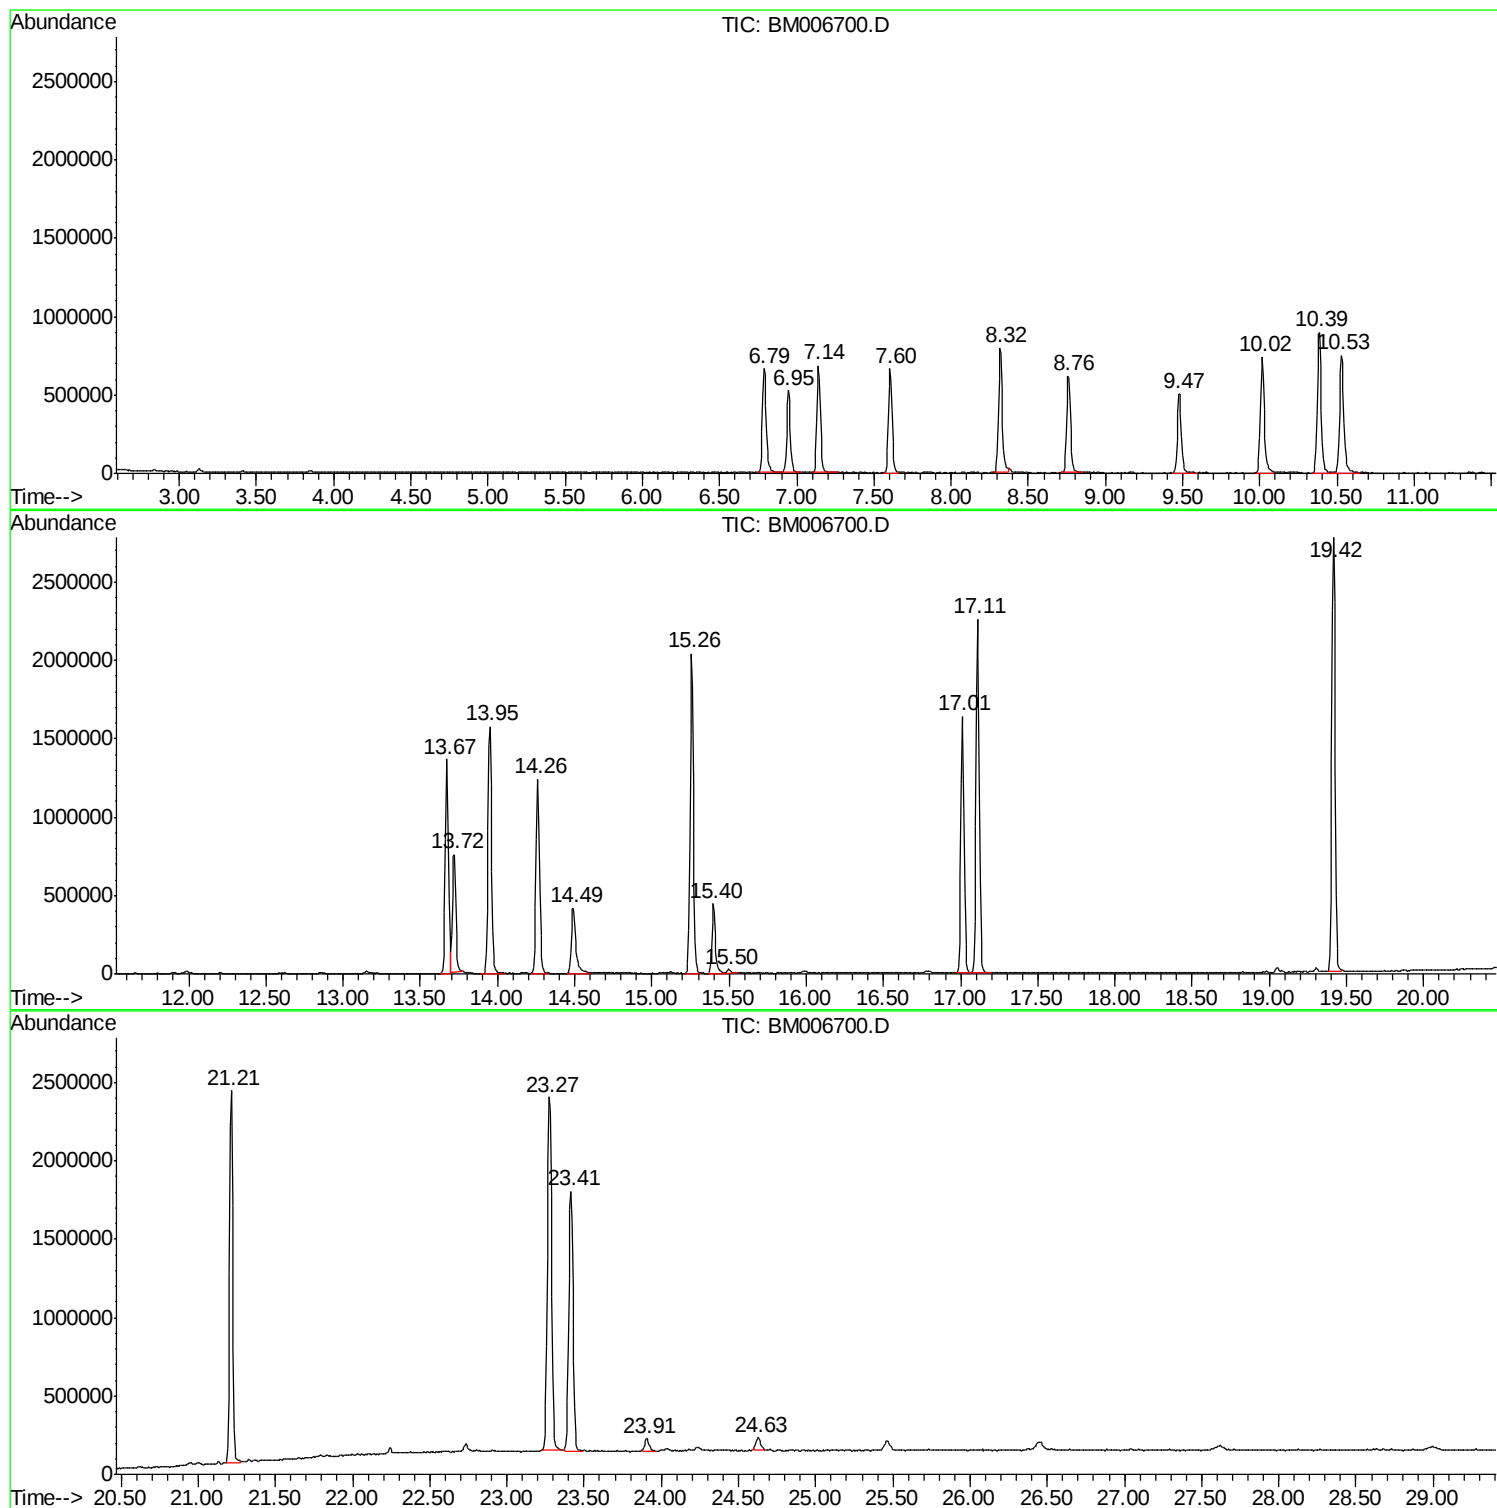

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072716\
Data File : BM006700.D
Acq On : 27 Jul 2016 22:24
Operator : UM/SJ
Sample : H4094-16
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJF1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072716\
Data File : BM006700.D
Acq On : 27 Jul 2016 22:24
Operator : UM/SJ
Sample : H4094-16
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJF1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc