
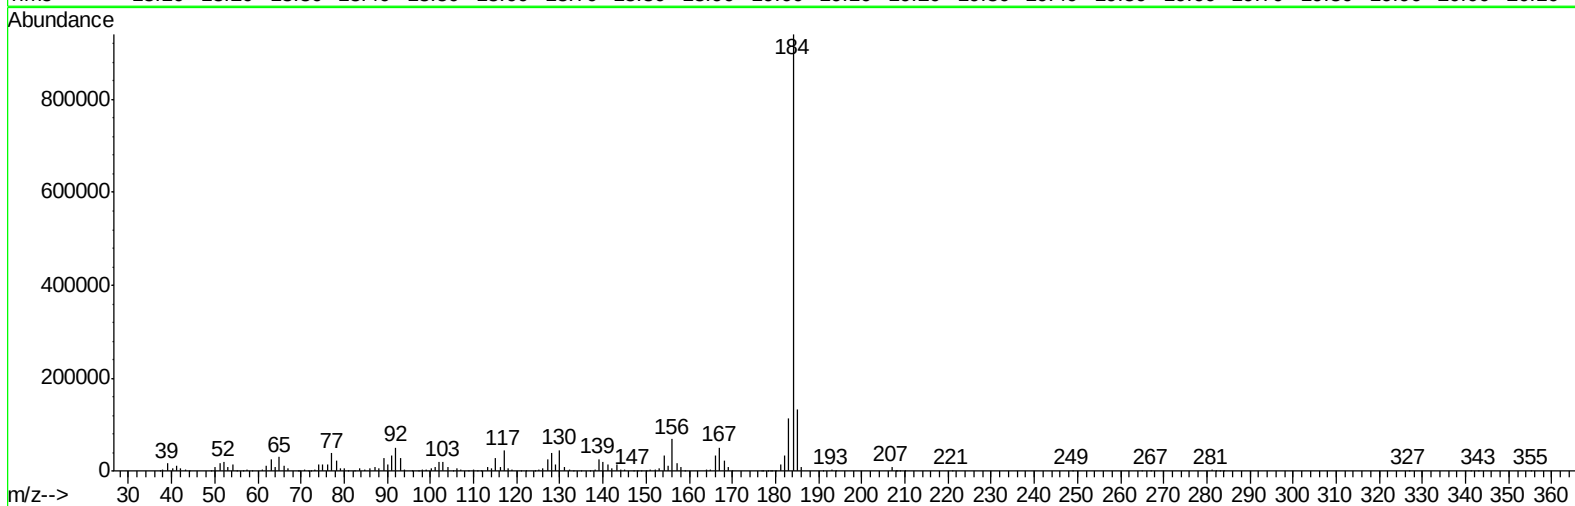


Data Path : Z:\HPCHEM1\BNA M\DATA\BM072717\
Data File : BM011020.D
Acq On : 27 Jul 2017 20:47
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 28 04:56:22 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 17:29:06 2017
Response via : Initial Calibration

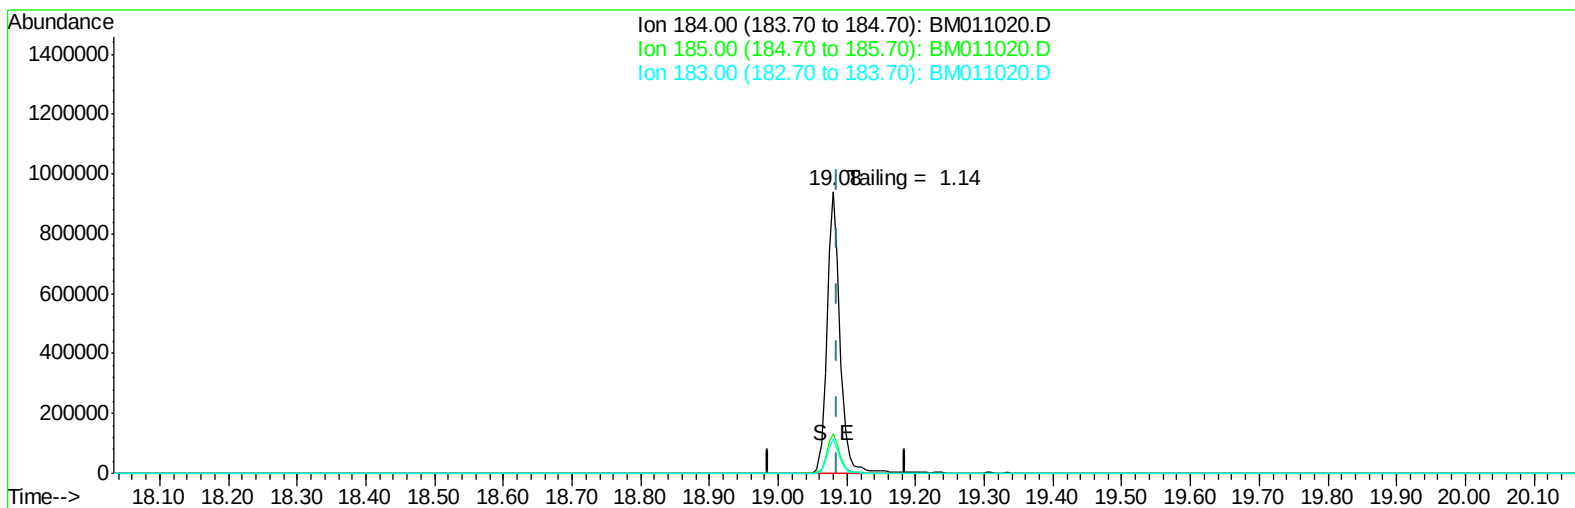

TIC: BM011020.D

(76) Benzidine

19.080min (-0.006) 53517.57ng

response 1241880

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.14
183.00	11.10	12.13
0.00	0.00	0.00