

Data Path : Z:\HPCHEM1\BNA M\DATA\BM072717\
 Data File : BM011015.D
 Acq On : 27 Jul 2017 17:47
 Operator : SJ/JU
 Sample : I4432-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 28 01:05:50 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 26 17:29:06 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	159935	20.00	ng	0.00
21) Naphthalene-d8	10.15	136	600010	20.00	ng	0.00
38) Acenaphthene-d10	14.05	164	391590	20.00	ng	0.00
63) Phenanthrene-d10	16.80	188	936648	20.00	ng	0.00
75) Chrysene-d12	21.02	240	1054677	20.00	ng	0.00
86) Perylene-d12	23.13	264	1043571	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.03	112	515299	54.46	ng	0.00
7) Phenol-d6	6.58	99	443142	32.97	ng	-0.01
23) Nitrobenzene-d5	8.53	82	1471680	92.06	ng	0.00
41) 2,4,6-Tribromophenol	15.55	330	797792	127.11	ng	0.00
44) 2-Fluorobiphenyl	12.66	172	2820357	90.33	ng	0.00
78) Terphenyl-d14	19.47	244	4369798	82.07	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM072717\
Data File : BM011015.D
Acq On : 27 Jul 2017 17:47
Operator : SJ/JU
Sample : I4432-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jul 28 01:05:50 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 17:29:06 2017
Response via : Initial Calibration

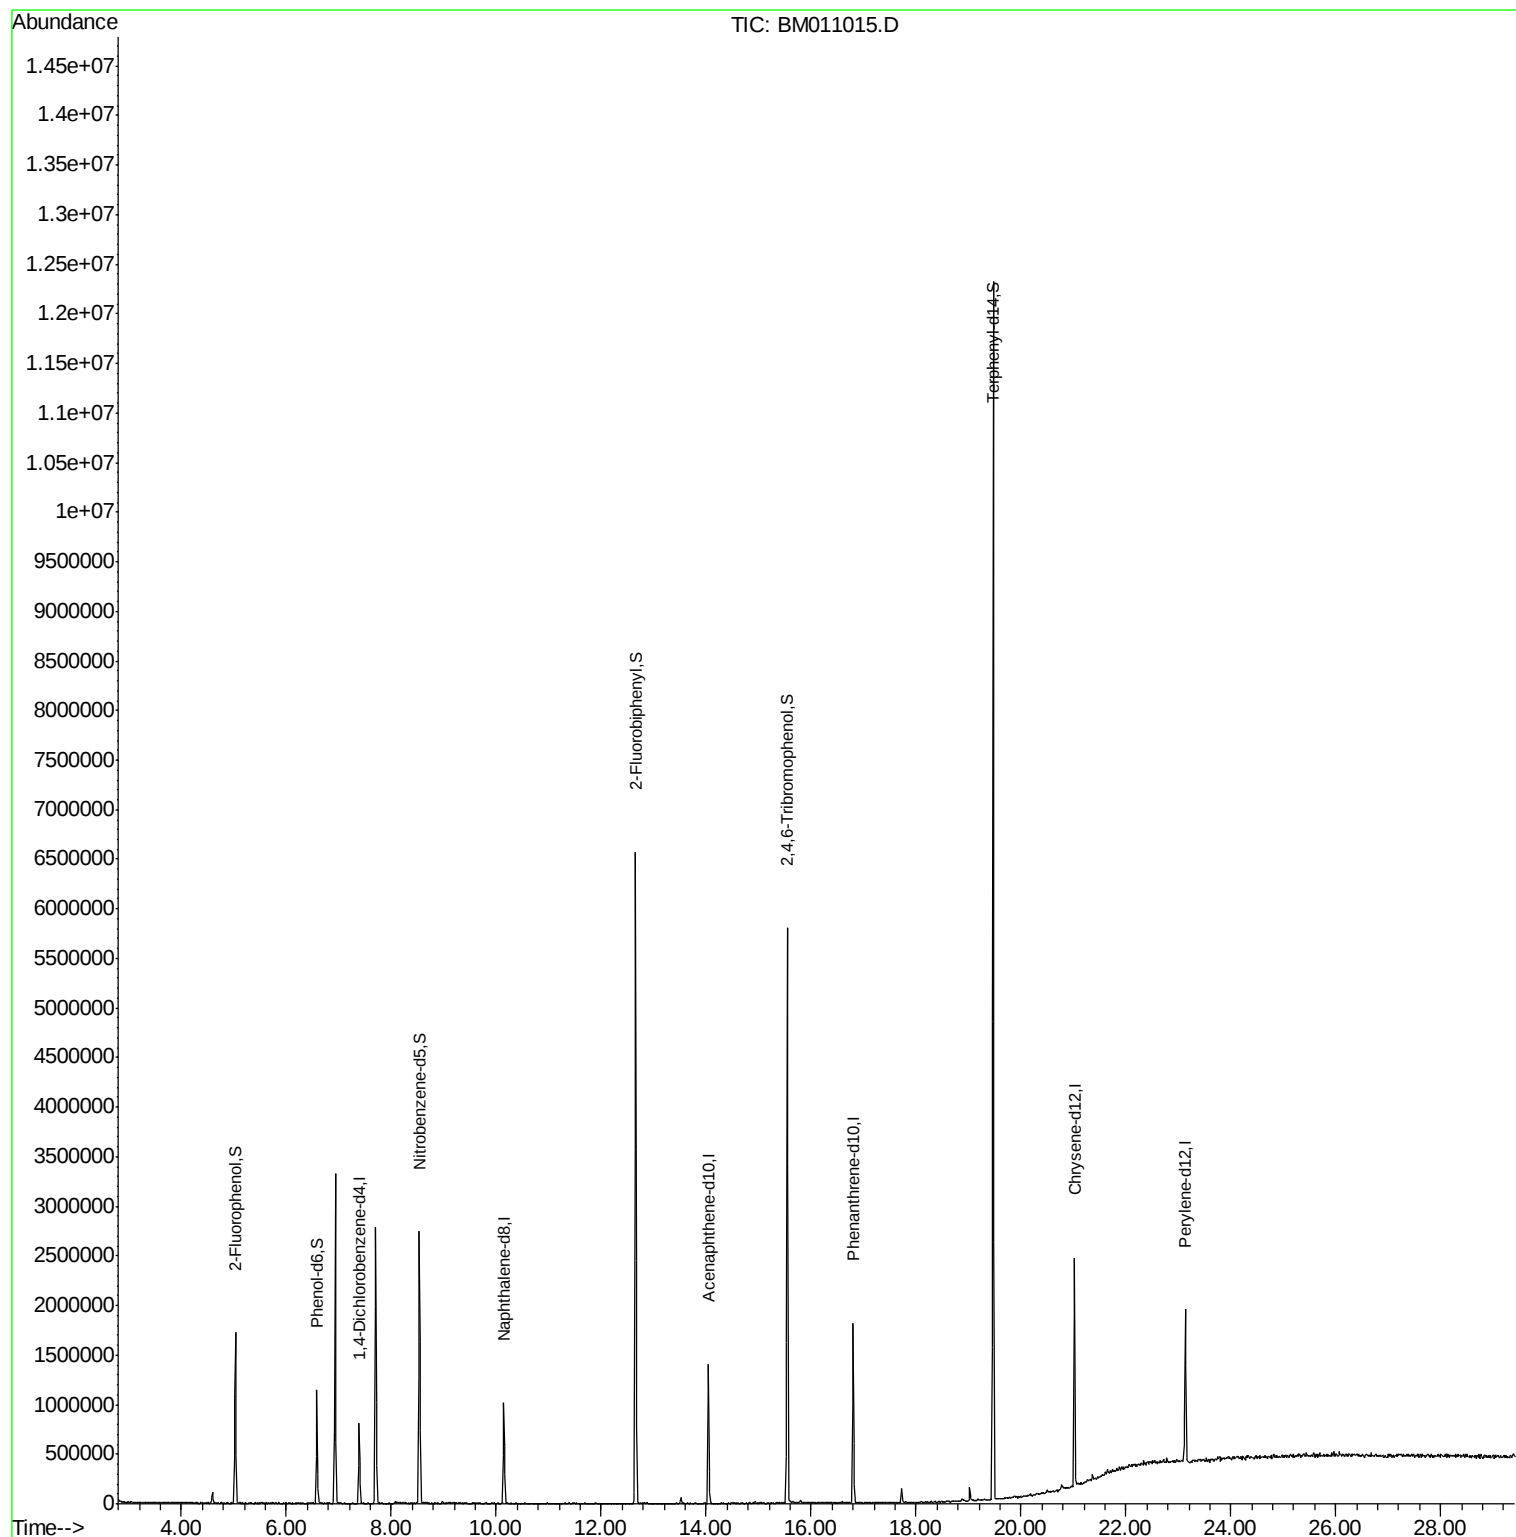

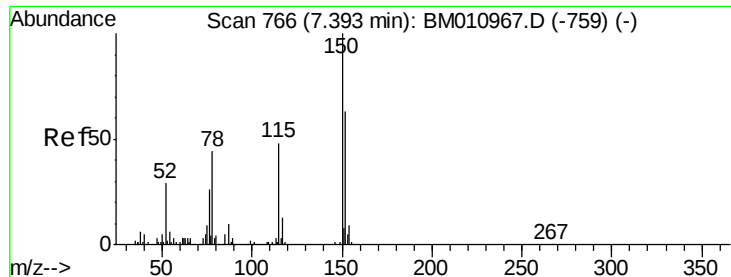


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.39 min Scan# 782
Delta R.T. -0.01 min
Lab File: BM011015.D
Acq: 27 Jul 2017 17:47

Instrument :
BNA_M
ClientSampleId :

Tot Ion:152 Resp: 159935
Ion Ratio Lower Upper
152 100
150 148.1 119.5 179.3
115 67.6 43.0 64.4#

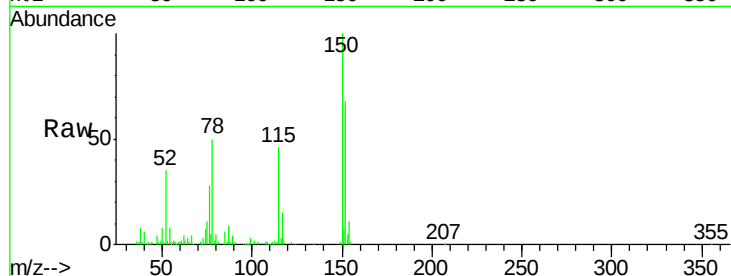


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

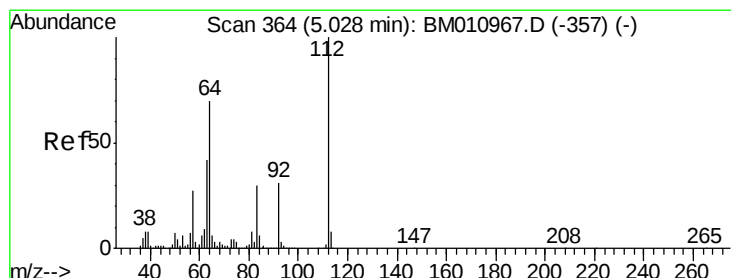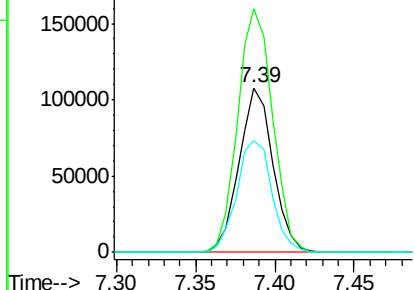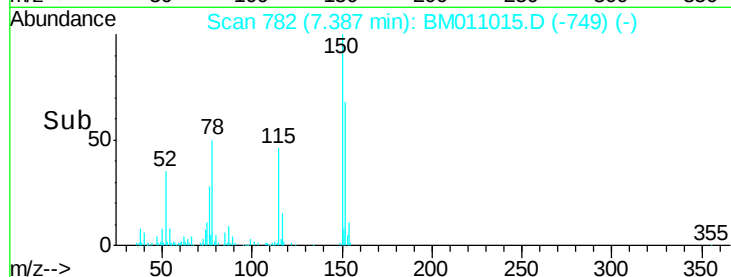



#5


2-Fluorophenol
Concen: 54.46 ng
RT: 5.03 min Scan# 381
Delta R.T. 0.00 min
Lab File: BM011015.D
Acq: 27 Jul 2017 17:47

Tgt Ion:112 Resp: 515299
Ion Ratio Lower Upper
112 100
64 71.6 38.6 57.8#
63 45.9 19.3 28.9#

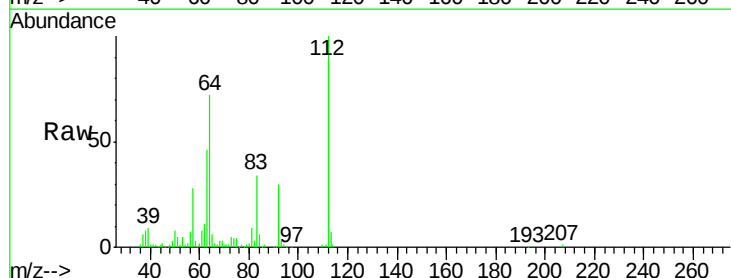

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

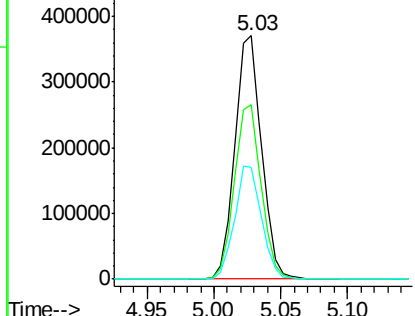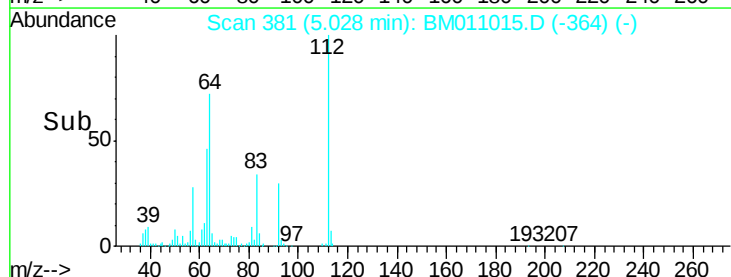

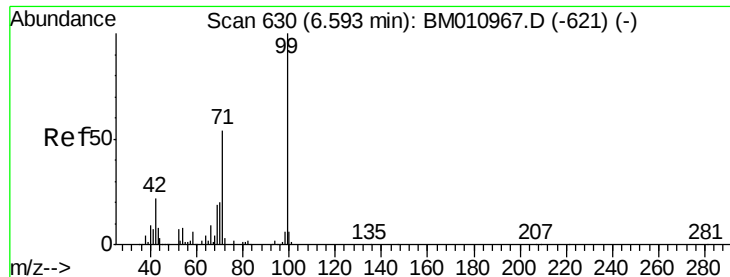

#7

Phenol-d6

Concen: 32.97 ng

RT: 6.58 min Scan# 645

Delta R.T. -0.01 min

Lab File: BM011015.D

Acq: 27 Jul 2017 17:47

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 99 Resp: 443142

Ion Ratio Lower Upper

99 100

42 25.4 11.0 16.4#




71 67.2 23.4 35.2#

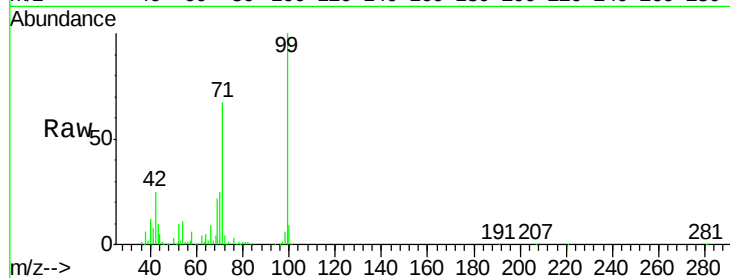

Abundance Ion 99.00 (98.70 to 99.70): BM011015.D (-630) (-)

Ion 42.00 (41.70 to 42.70): BM011015.D (-630) (-)

Ion 71.00 (70.70 to 71.70): BM011015.D (-630) (-)

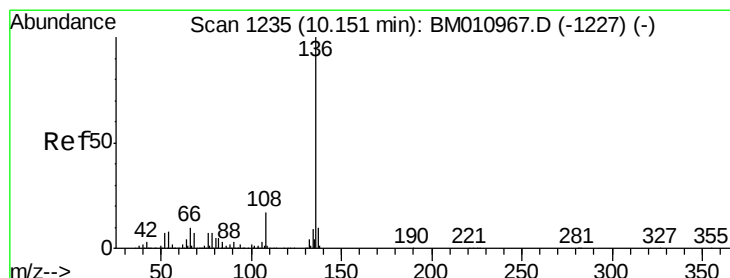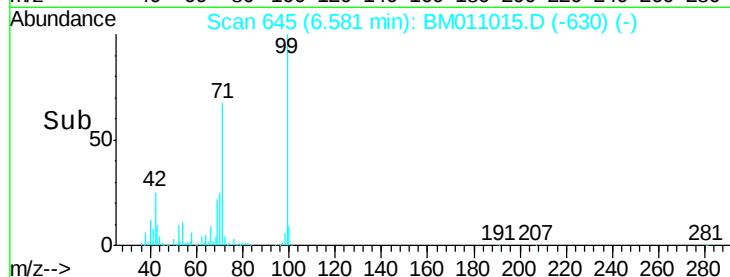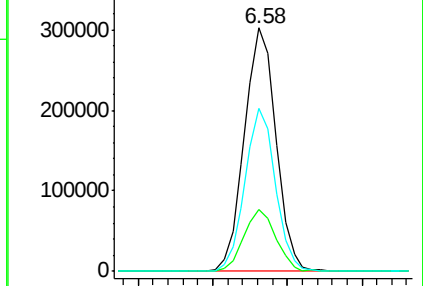

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.15 min Scan# 1251

Delta R.T. -0.01 min

Lab File: BM011015.D

Acq: 27 Jul 2017 17:47

Tgt Ion: 136 Resp: 600010


Ion Ratio Lower Upper

136 100

137 9.7 8.7 13.1

54 10.5 4.6 6.8#

68 7.1 3.7 5.5#


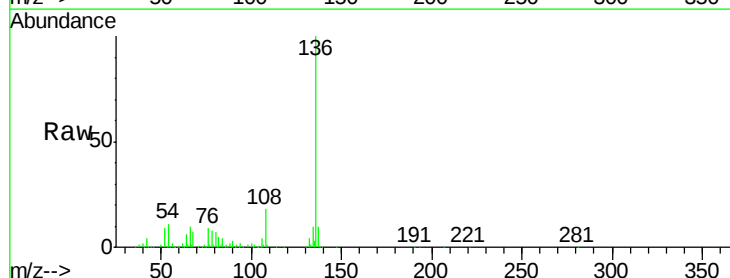



Abundance Ion 136.00 (135.70 to 136.70): BM011015.D (-1235) (-)

Ion 137.00 (136.70 to 137.70): BM011015.D (-1235) (-)

Ion 54.00 (53.70 to 54.70): BM011015.D (-1235) (-)

Ion 68.00 (67.70 to 68.70): BM011015.D (-1235) (-)



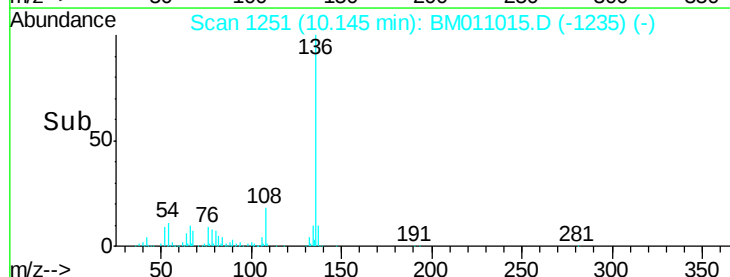
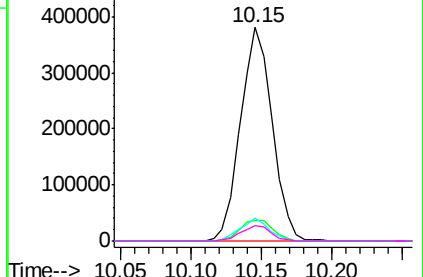


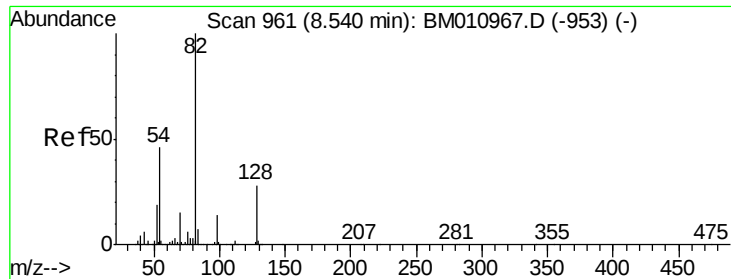

#23
 Nitrobenzene-d5
 Concen: 92.06 ng
 RT: 8.53 min Scan# 977
 Delta R.T. -0.01 min
 Lab File: BM011015.D
 Acq: 27 Jul 2017 17:47




Instrument :
 BNA_M
 ClientSampleId :


Tot Ion: 82 Resp: 1471680
 Ion Ratio Lower Upper
 82 100
 128 27.8 32.8 49.2#
 54 50.2 40.6 60.8

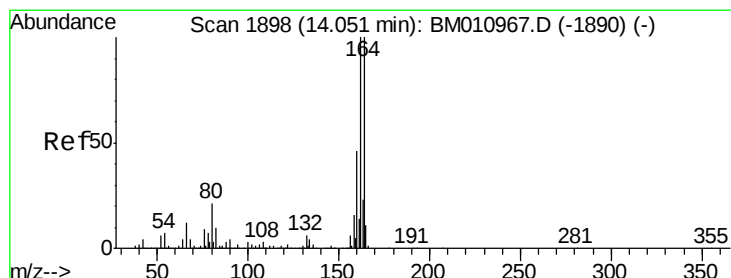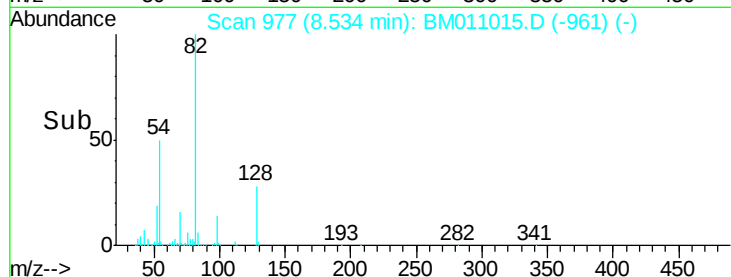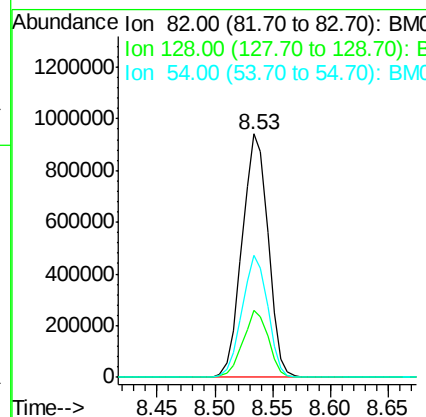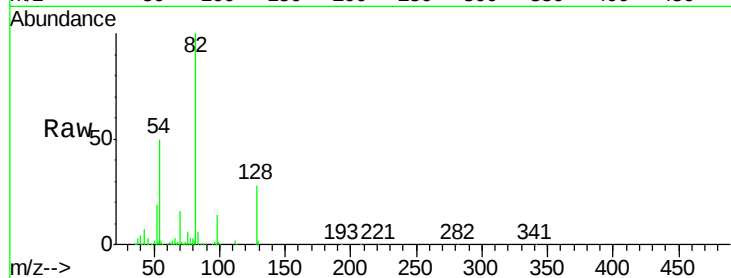

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.05 min Scan# 1914
 Delta R.T. -0.01 min
 Lab File: BM011015.D
 Acq: 27 Jul 2017 17:47

Tgt Ion: 164 Resp: 391590
 Ion Ratio Lower Upper
 164 100
 162 98.2 82.4 123.6
 160 45.6 35.8 53.6


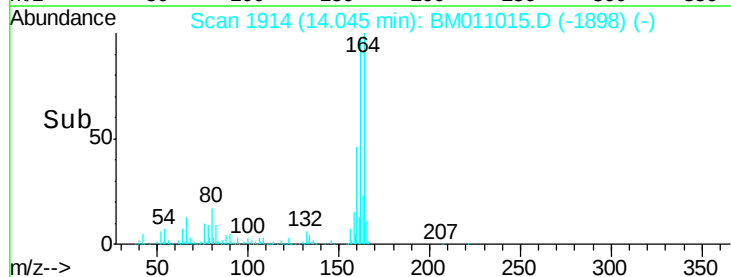
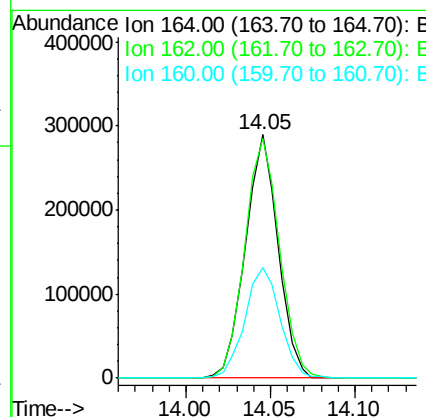
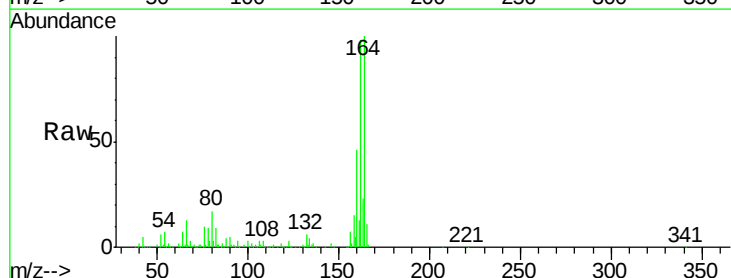


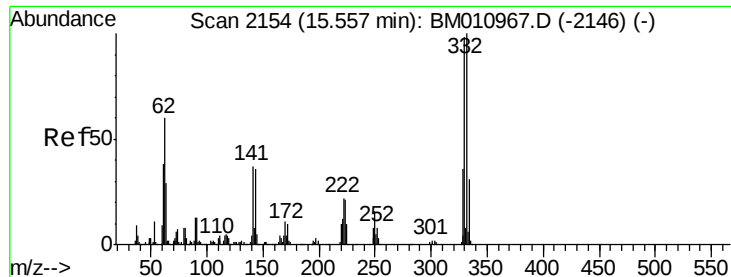

#41
 2,4,6-Tribromophenol
 Concen: 127.11 ng
 RT: 15.55 min Scan# 2170
 Delta R.T. -0.01 min
 Lab File: BM011015.D
 Acq: 27 Jul 2017 17:47




Instrument :
 BNA_M
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
330	100		
332	95.5	0.0	0.0#
141	45.5	0.0	0.0#

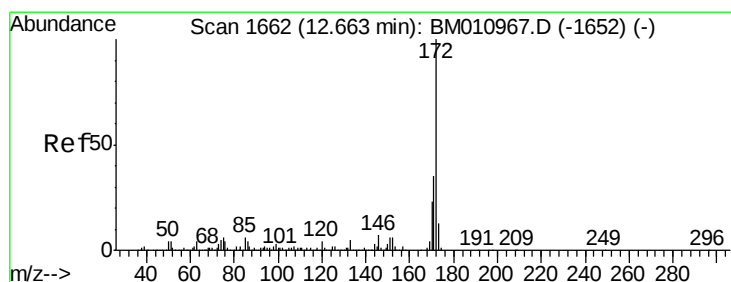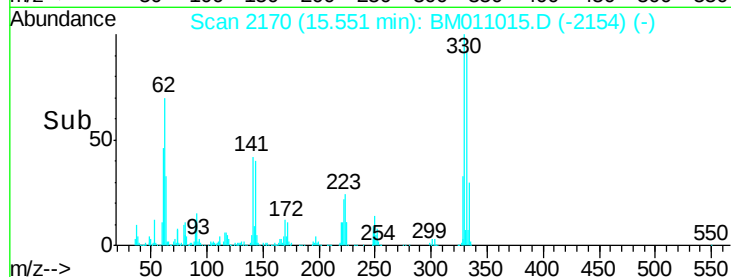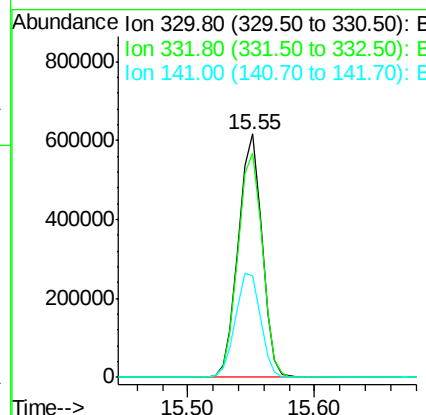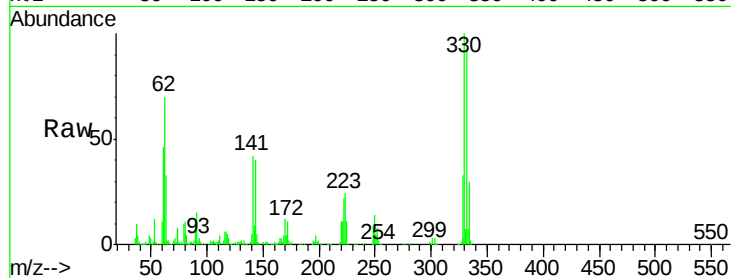

#44
 2-Fluorobiphenyl
 Concen: 90.33 ng
 RT: 12.66 min Scan# 1678
 Delta R.T. -0.01 min
 Lab File: BM011015.D
 Acq: 27 Jul 2017 17:47

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.1	28.5	42.7
170	22.7	18.8	28.2


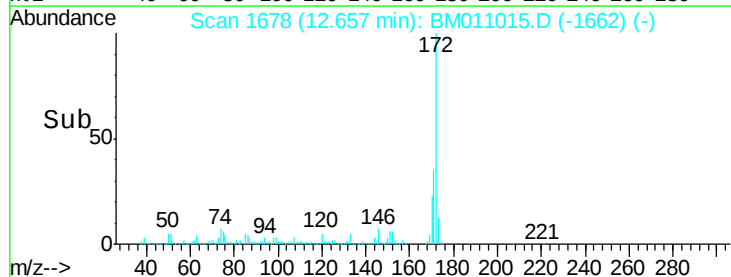
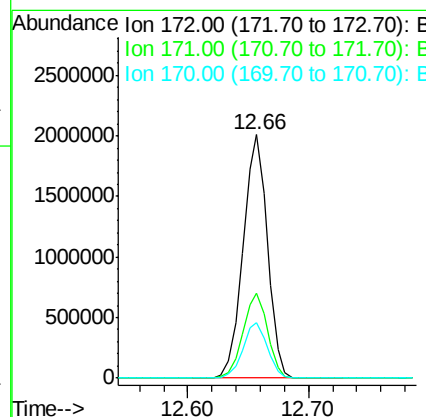
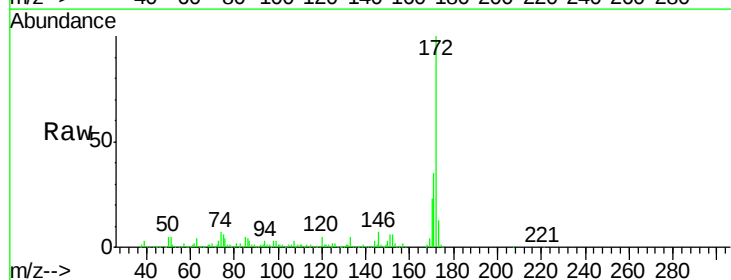


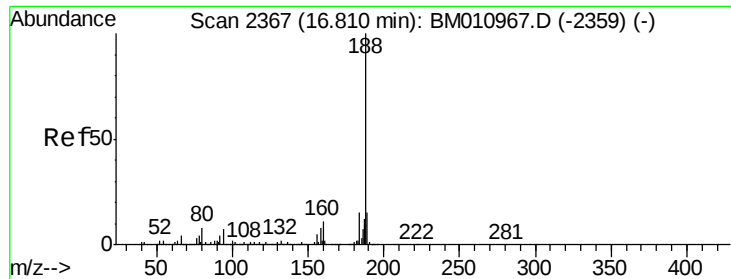

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 16.80 min Scan# 2383
Delta R.T. -0.01 min
Lab File: BM011015.D
Acq: 27 Jul 2017 17:47




Instrument :
BNA_M
ClientSampleId :


Tot Ion:188 Resp: 936648
Ion Ratio Lower Upper
188 100
94 5.7 8.7 13.1#
80 7.5 9.3 13.9#

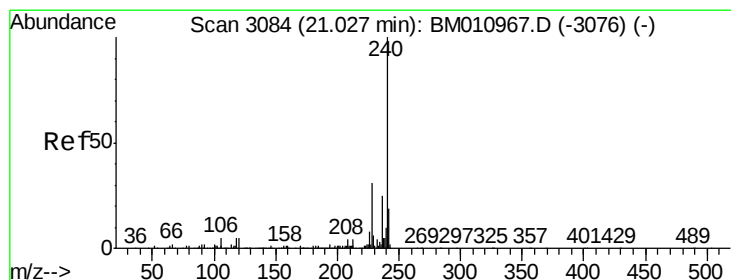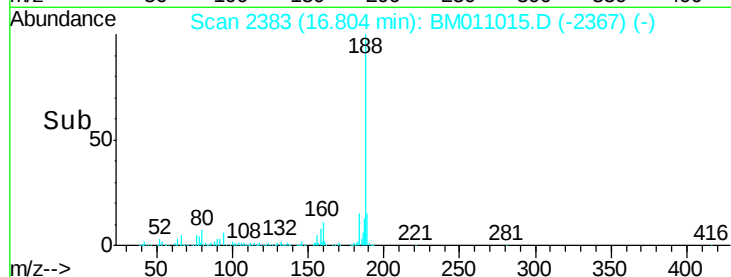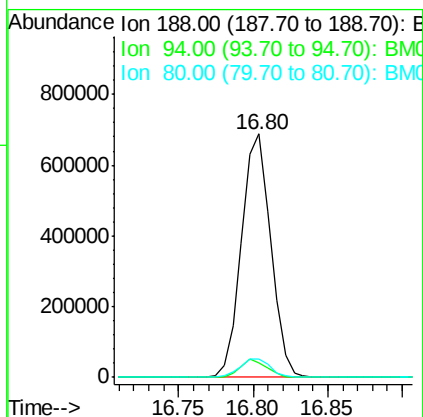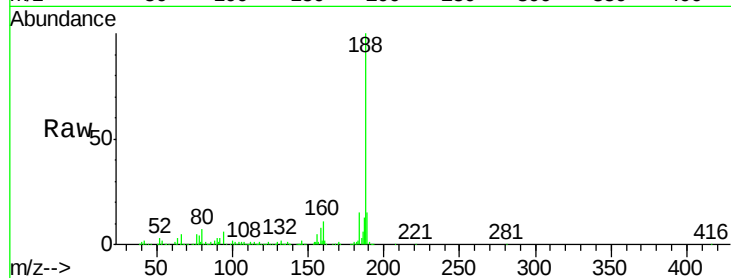

#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.02 min Scan# 3100
Delta R.T. -0.01 min
Lab File: BM011015.D
Acq: 27 Jul 2017 17:47

Tgt Ion:240 Resp: 1054677
Ion Ratio Lower Upper
240 100
120 4.9 8.2 12.2#
236 22.8 20.0 30.0

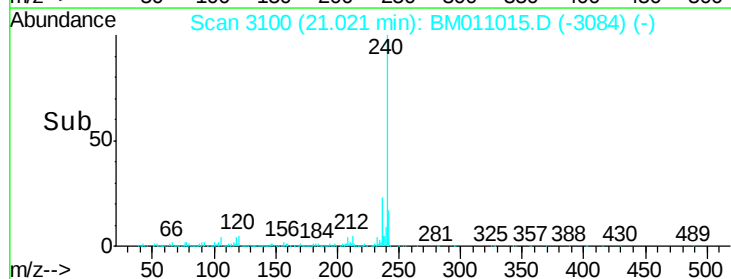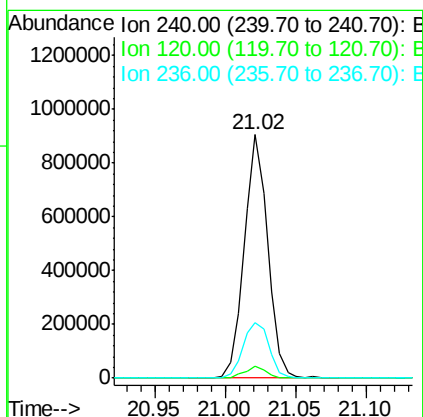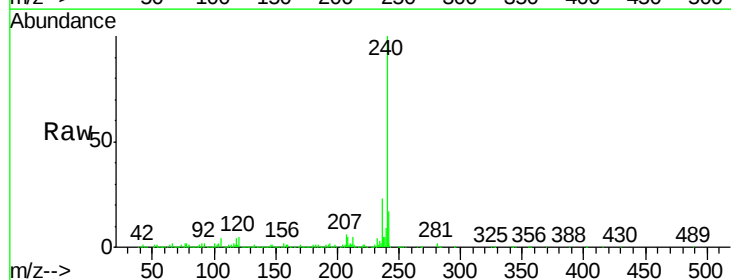

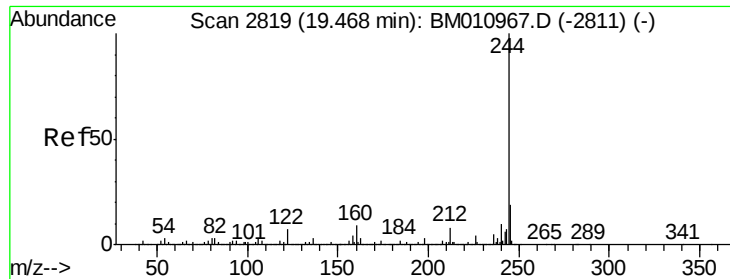

#78

Terphenyl-d14

Concen: 82.07 ng

RT: 19.47 min Scan# 2836

Delta R.T. 0.00 min

Lab File: BM011015.D

Acq: 27 Jul 2017 17:47

Instrument :

BNA_M

ClientSampleId :


Tot Ion:244 Resp: 4369798

Ion Ratio Lower Upper

244 100

212 8.7 4.9 7.3#




122 6.3 6.2 9.4

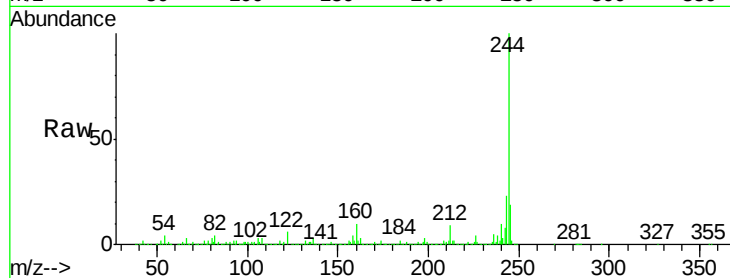

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

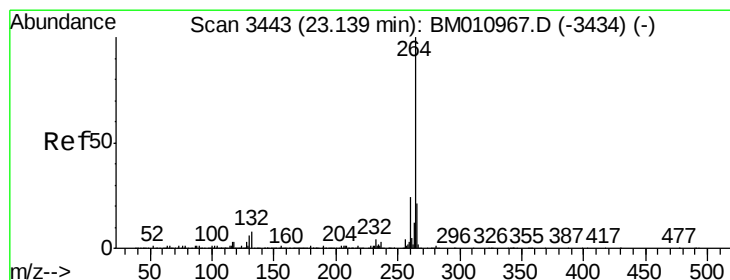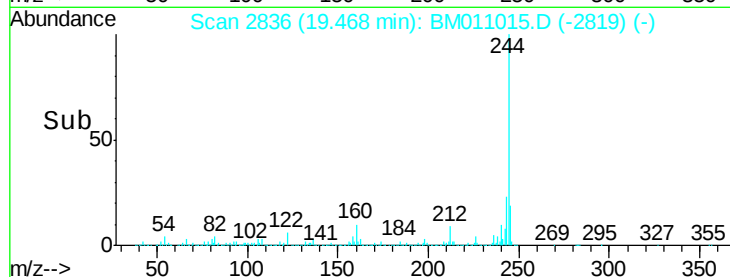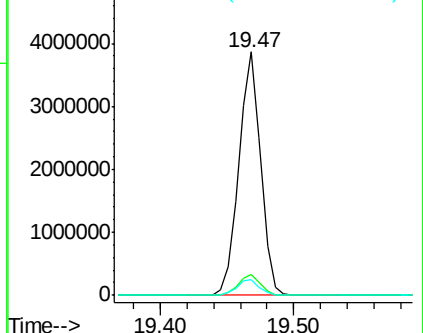

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.13 min Scan# 3459

Delta R.T. -0.01 min

Lab File: BM011015.D

Acq: 27 Jul 2017 17:47


Tgt Ion:264 Resp: 1043571

Ion Ratio Lower Upper

264 100

260 23.3 18.6 27.8

265 20.7 17.3 25.9

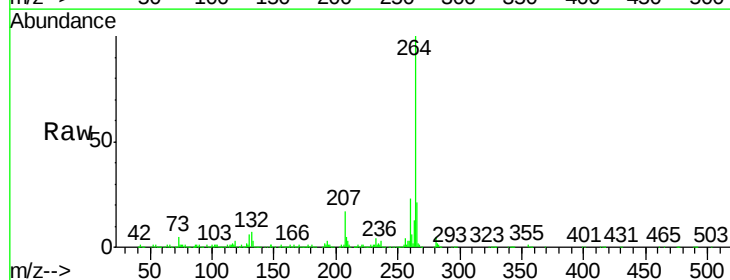

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

