

Data Path : Z:\HPCHEM1\BNA M\DATA\BM072717\
 Data File : BM011027.D
 Acq On : 28 Jul 2017 00:59
 Operator : SJ/JU
 Sample : I4446-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 28 02:02:02 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 26 17:29:06 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	154936	20.00	ng	0.00
21) Naphthalene-d8	10.15	136	552642	20.00	ng	0.00
38) Acenaphthene-d10	14.05	164	231275	20.00	ng	0.00
63) Phenanthrene-d10	16.80	188	700248	20.00	ng	-0.01
75) Chrysene-d12	21.02	240	414460	20.00	ng	0.00
86) Perylene-d12	23.13	264	29016	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.03	112	1320922	144.12	ng	0.00
7) Phenol-d6	6.59	99	1470553	112.92	ng	0.00
23) Nitrobenzene-d5	8.53	82	1502328	102.03	ng	0.00
41) 2,4,6-Tribromophenol	15.54	330	733168	197.79	ng	-0.01
44) 2-Fluorobiphenyl	12.66	172	2649707	143.69	ng	0.00
78) Terphenyl-d14	19.47	244	3184659	152.21	ng	0.00
Target Compounds						
15) Benzyl Alcohol	7.70	79	26825	2.15	ng	Qvalue # 35


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM072717\
Data File : BM011027.D
Acq On : 28 Jul 2017 00:59
Operator : SJ/JU
Sample : I4446-03
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jul 28 02:02:02 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 17:29:06 2017
Response via : Initial Calibration

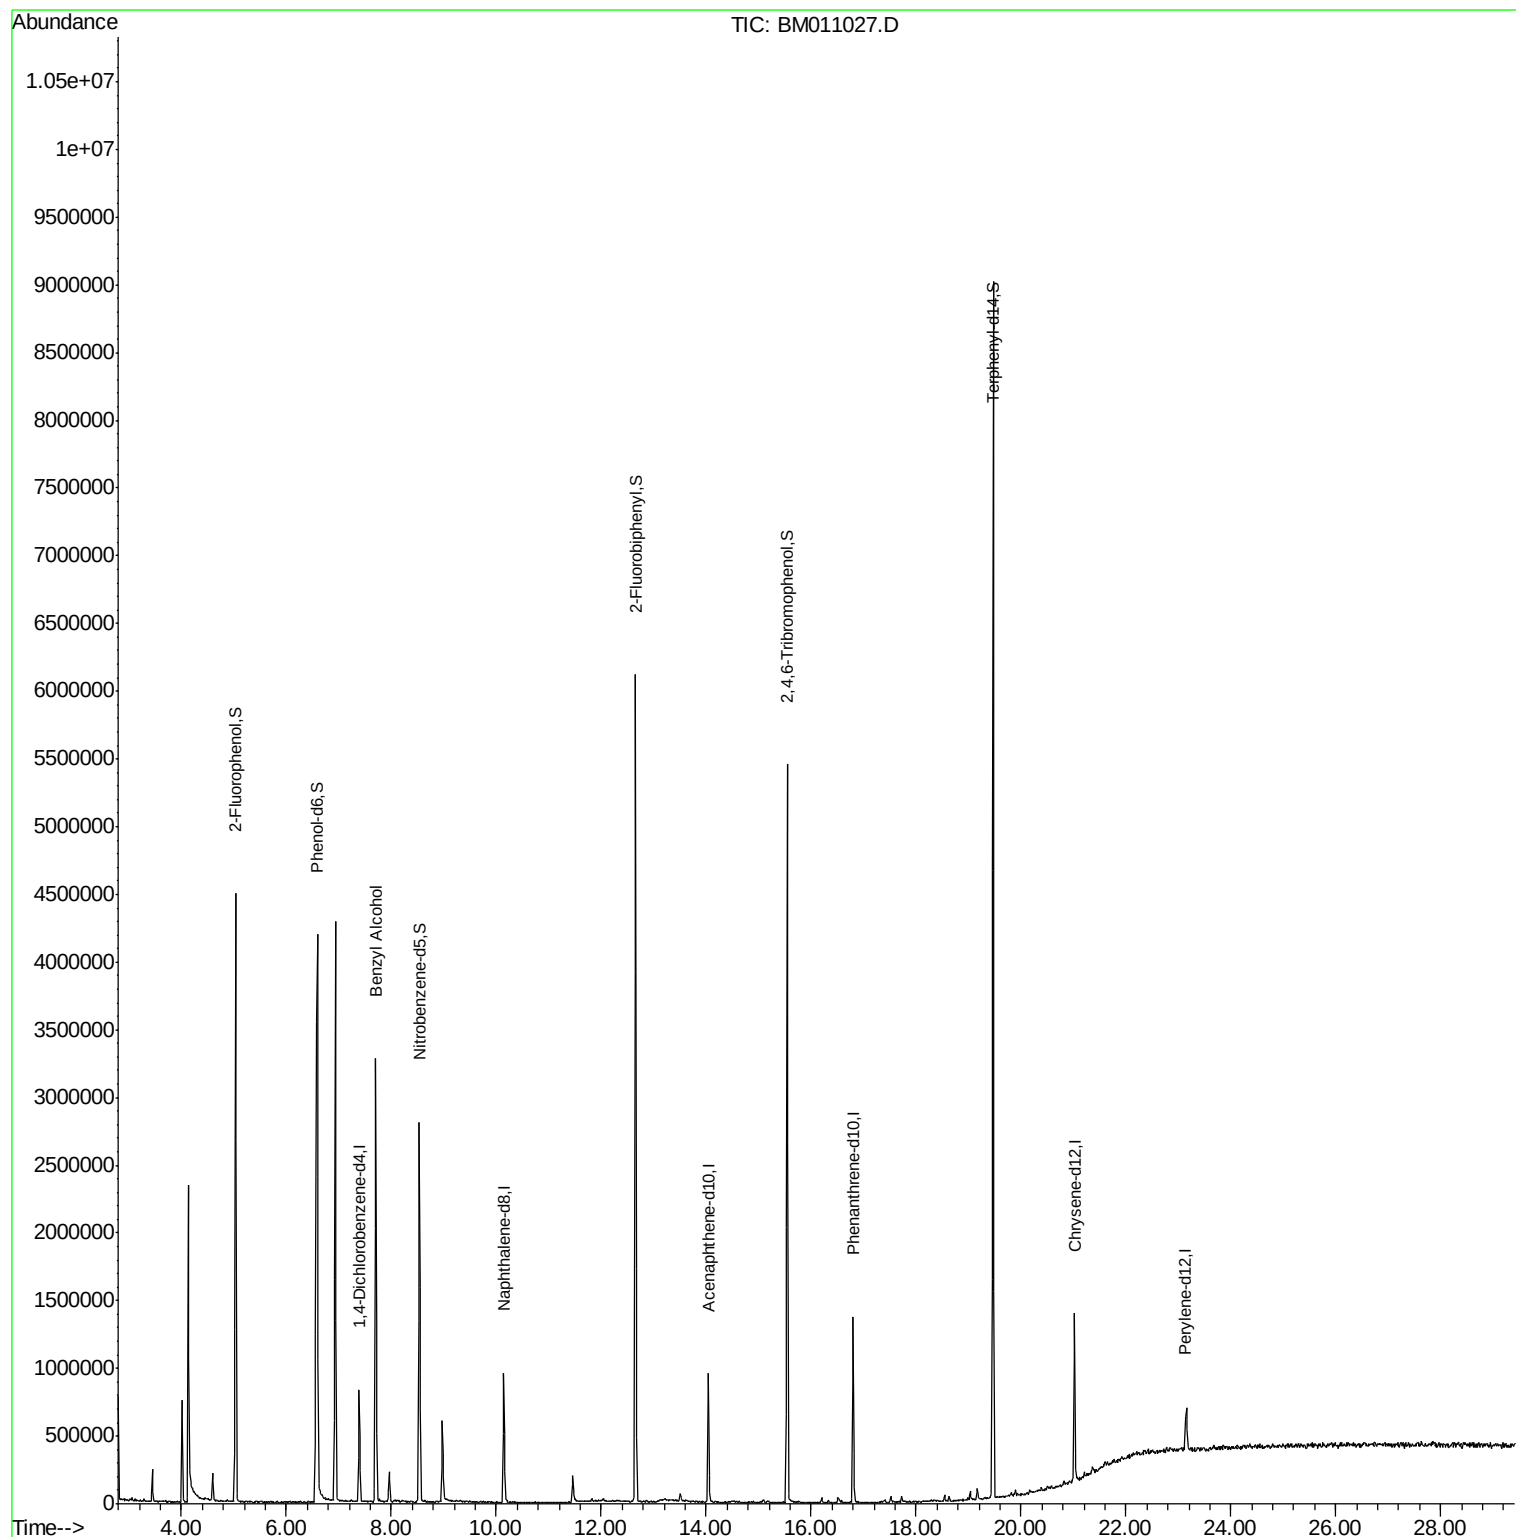

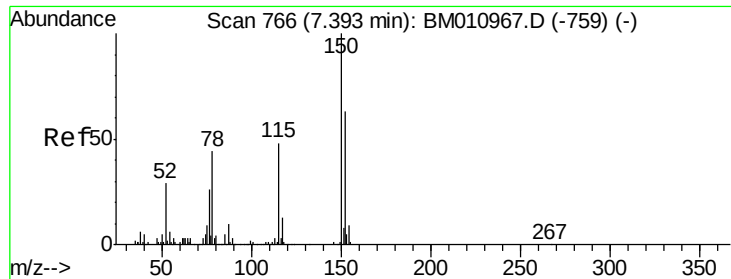


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.39 min Scan# 782
Delta R.T. -0.01 min
Lab File: BM011027.D
Acq: 28 Jul 2017 00:59

Instrument :
BNA_M
ClientSampled :

Tot Ion:152 Resp: 154936
Ion Ratio Lower Upper
152 100
150 154.8 119.5 179.3
115 69.8 43.0 64.4#

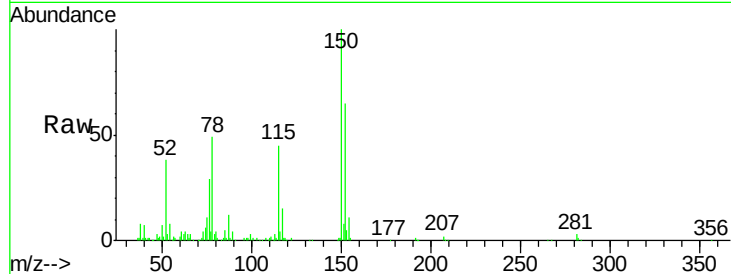


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

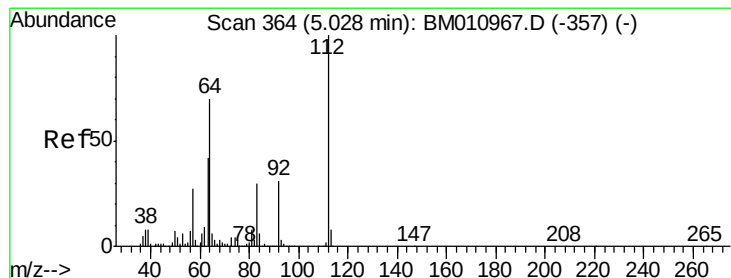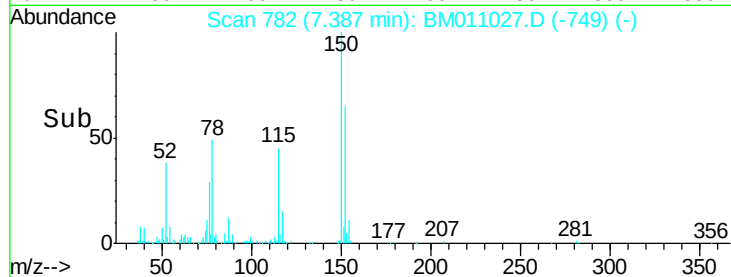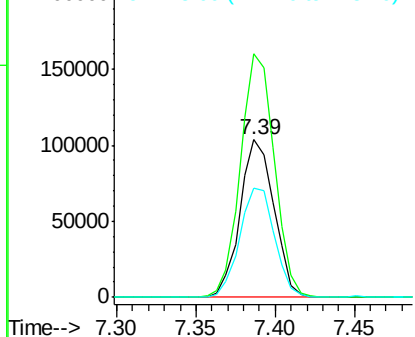



#5


2-Fluorophenol
Concen: 144.12 ng
RT: 5.03 min Scan# 381
Delta R.T. 0.00 min
Lab File: BM011027.D
Acq: 28 Jul 2017 00:59

Tgt Ion:112 Resp: 1320922
Ion Ratio Lower Upper
112 100
64 72.9 38.6 57.8#
63 47.7 19.3 28.9#

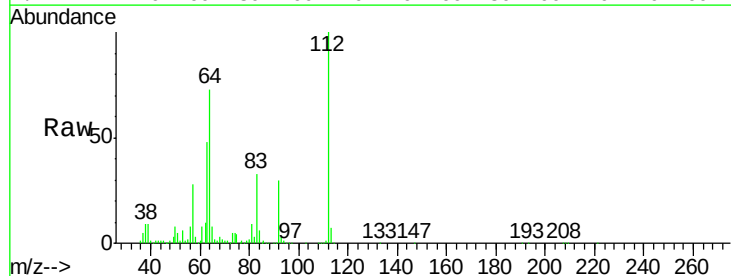

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

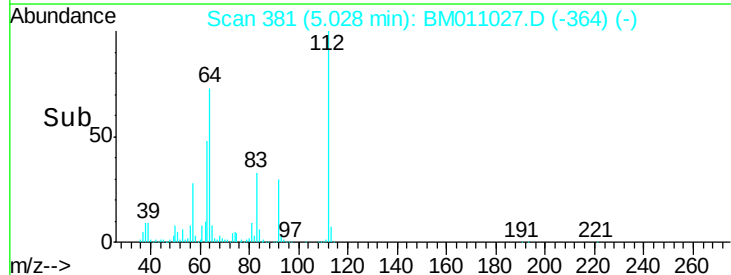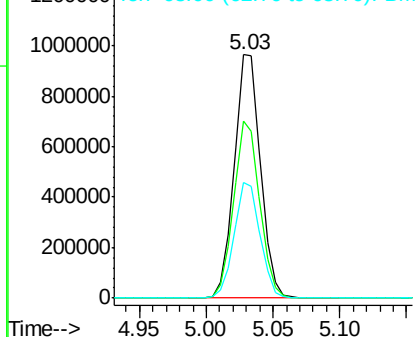

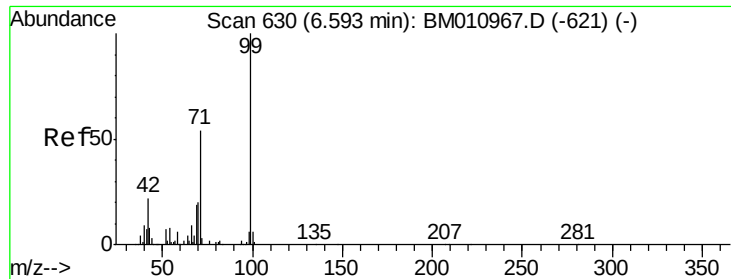

#7

Phenol-d6

Concen: 112.92 ng

RT: 6.59 min Scan# 646

Delta R.T. -0.01 min

Lab File: BM011027.D

Acq: 28 Jul 2017 00:59

Instrument :

BNA_M

ClientSampled :


Tot Ion: 99 Resp: 1470553

Ion Ratio Lower Upper

99 100

42 26.2 11.0 16.4#




71 63.4 23.4 35.2#

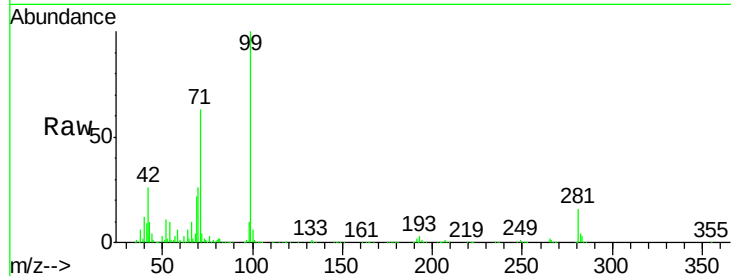

Abundance Ion 99.00 (98.70 to 99.70): BM011027.D (-630) (-)

Ion 42.00 (41.70 to 42.70): BM011027.D (-630) (-)

Ion 71.00 (70.70 to 71.70): BM011027.D (-630) (-)

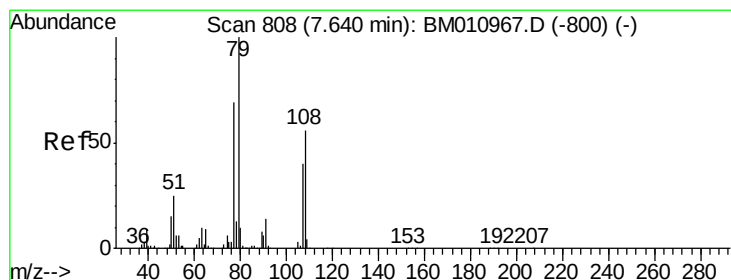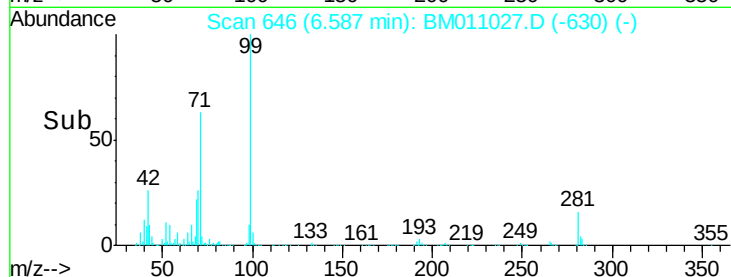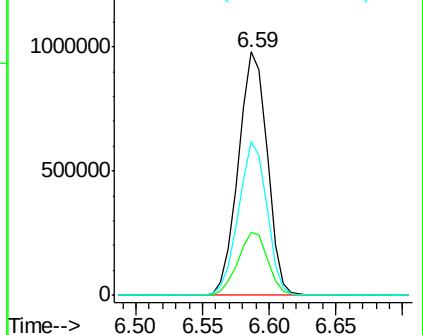

#15

Benzyl Alcohol

Concen: 2.15 ng

RT: 7.70 min Scan# 836

Delta R.T. 0.06 min

Lab File: BM011027.D

Acq: 28 Jul 2017 00:59


Tgt Ion: 79 Resp: 26825

Ion Ratio Lower Upper

79 100

108 57.6 65.0 97.4#



77 156.1 53.0 79.6#

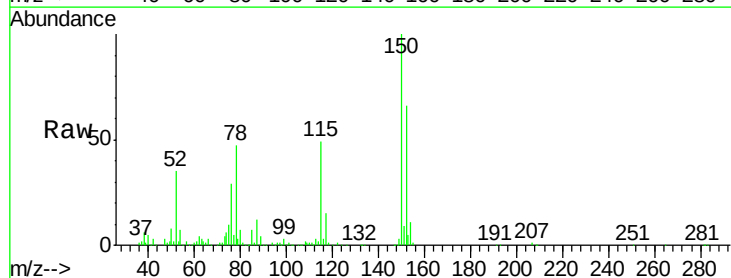


Abundance Ion 79.00 (78.70 to 79.70): BM011027.D (-808) (-)

Ion 108.00 (107.70 to 108.70): BM011027.D (-808) (-)

Ion 77.00 (76.70 to 77.70): BM011027.D (-808) (-)



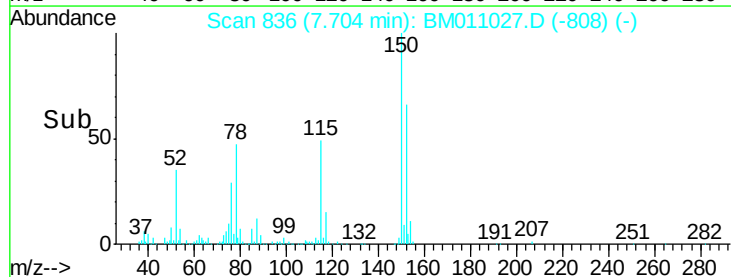
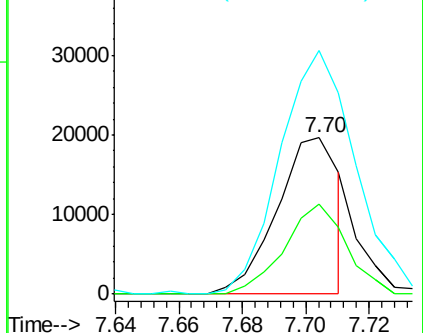


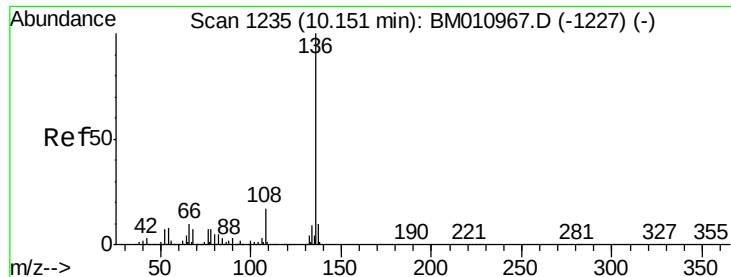

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.15 min Scan# 1251
Delta R.T. -0.01 min
Lab File: BM011027.D
Acq: 28 Jul 2017 00:59




Instrument :
BNA_M
ClientSampleId :


Tot Ion:	136	Resp:	552642
Ion	Ratio	Lower	Upper
136	100		
137	12.0	8.7	13.1
54	8.7	4.6	6.8#
68	5.4	3.7	5.5

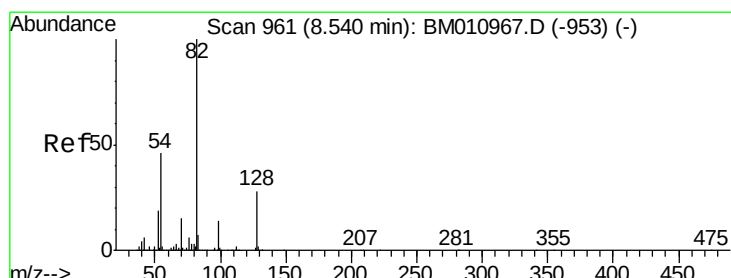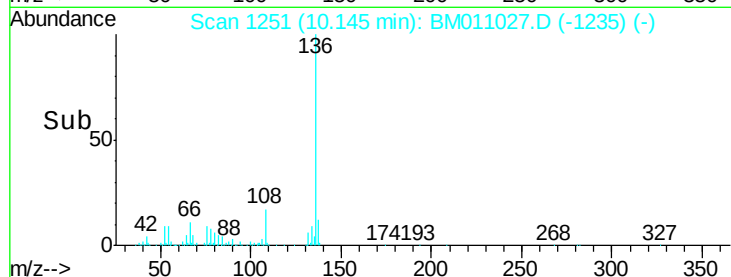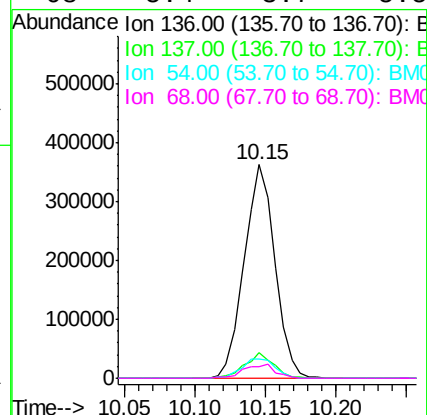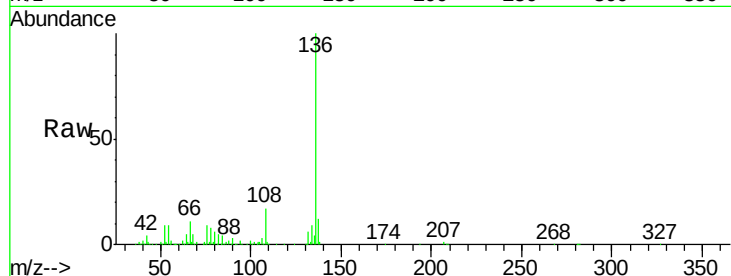

#23
Nitrobenzene-d5
Concen: 102.03 ng
RT: 8.53 min Scan# 977
Delta R.T. -0.01 min
Lab File: BM011027.D
Acq: 28 Jul 2017 00:59

Tgt Ion:	82	Resp:	1502328
Ion	Ratio	Lower	Upper
82	100		
128	26.5	32.8	49.2#
54	50.1	40.6	60.8


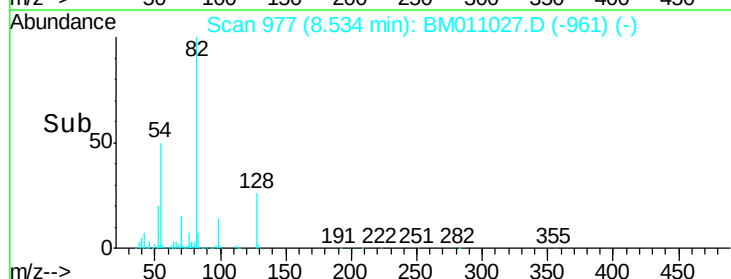
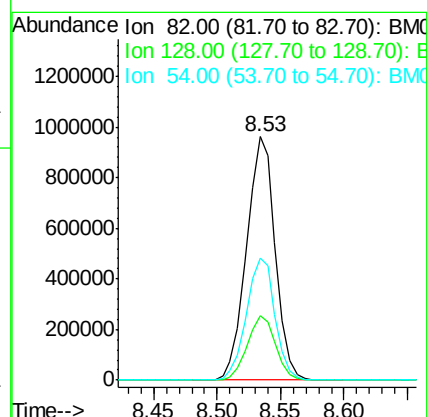
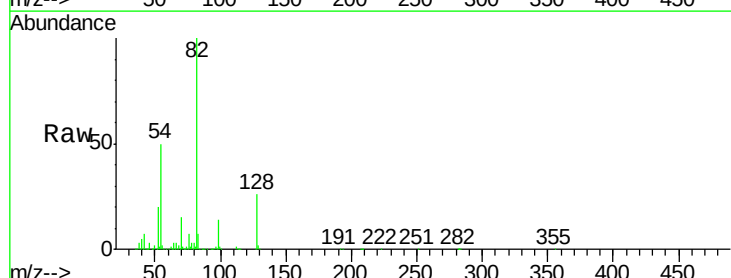


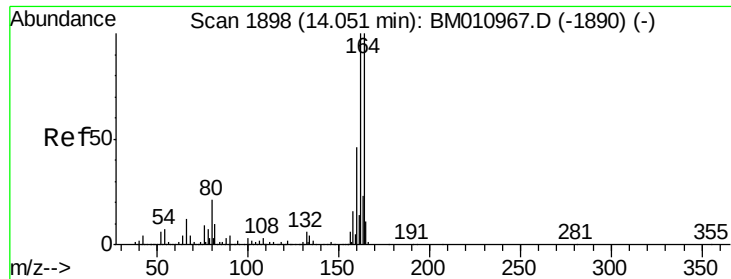

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.05 min Scan# 1914
Delta R.T. -0.01 min
Lab File: BM011027.D
Acq: 28 Jul 2017 00:59




Instrument :
BNA_M
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
164	100		
162	108.0	82.4	123.6
160	54.0	35.8	53.6

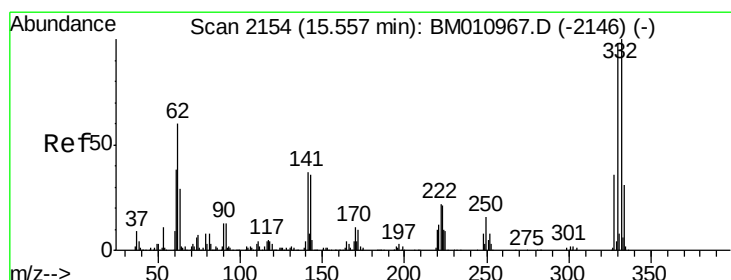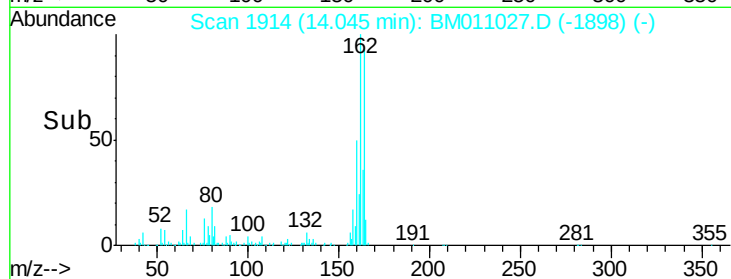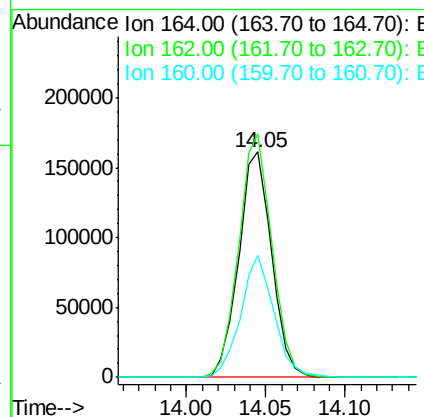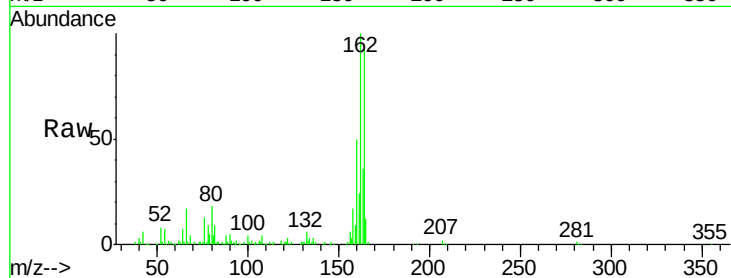

#41
2,4,6-Tribromophenol
Concen: 197.79 ng
RT: 15.54 min Scan# 2169
Delta R.T. -0.01 min
Lab File: BM011027.D
Acq: 28 Jul 2017 00:59

Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.5	0.0	0.0#
141	46.5	0.0	0.0#

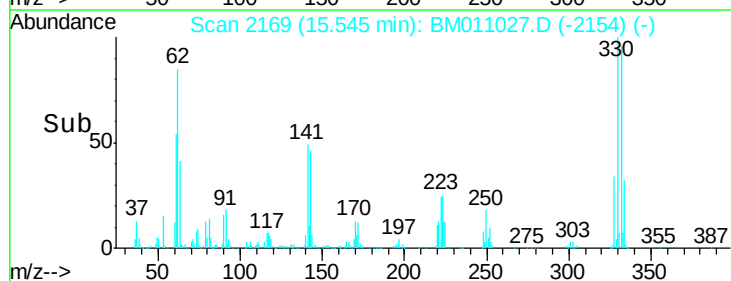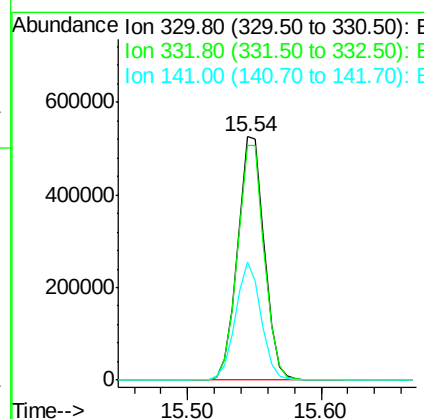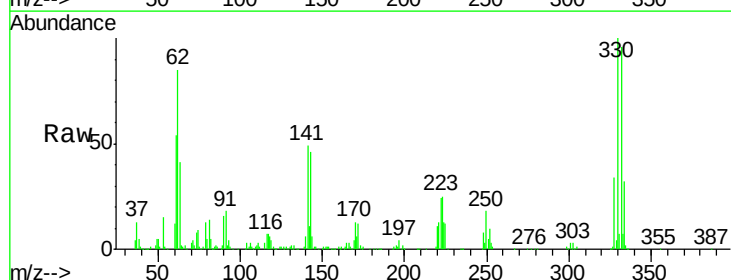




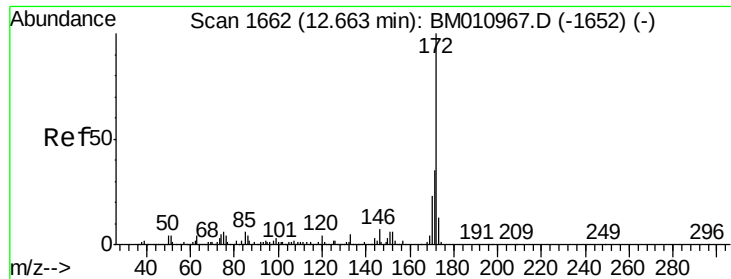


#44
 2-Fluorobiphenyl
 Concen: 143.69 ng
 RT: 12.66 min Scan# 1678
 Delta R.T. -0.01 min
 Lab File: BM011027.D
 Acq: 28 Jul 2017 00:59

Instrument :
 BNA_M
 ClientSampled :

Tot Ion:172 Resp: 2649707




Ion	Ratio	Lower	Upper
172	100		
171	35.3	28.5	42.7
170	23.9	18.8	28.2

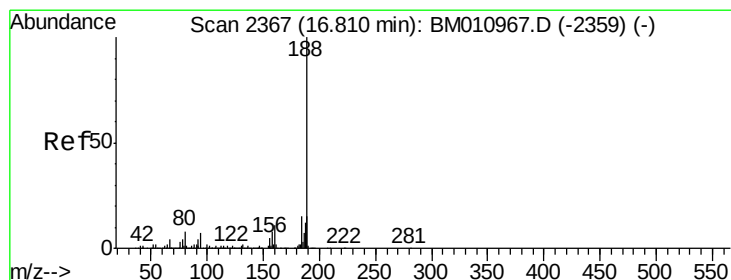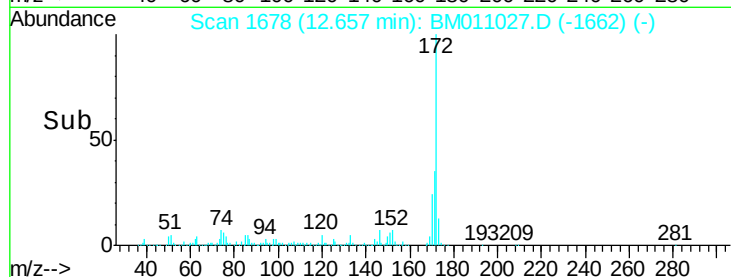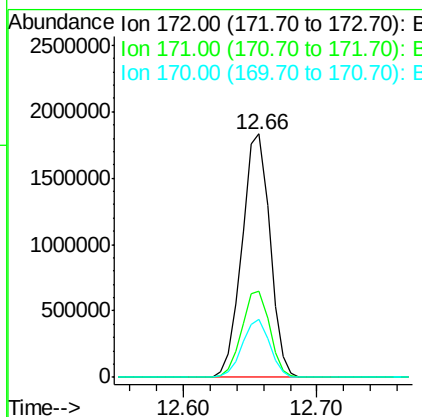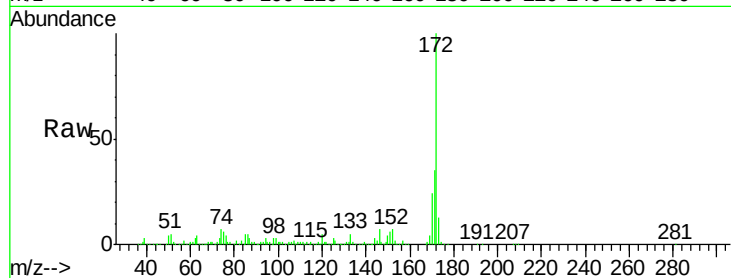


#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 16.80 min Scan# 2382
 Delta R.T. -0.01 min
 Lab File: BM011027.D
 Acq: 28 Jul 2017 00:59

Tgt Ion:188 Resp: 700248

Ion	Ratio	Lower	Upper
188	100		
94	7.0	8.7	13.1#
80	9.1	9.3	13.9#

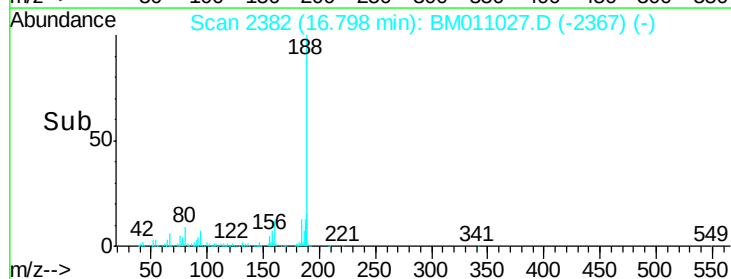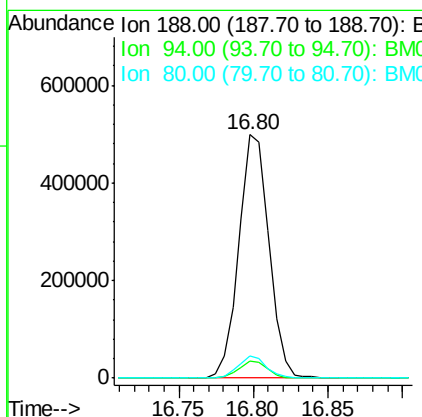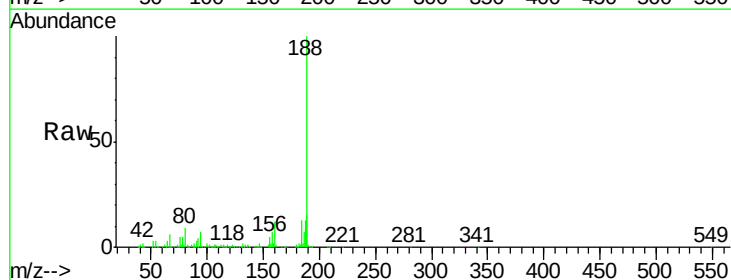

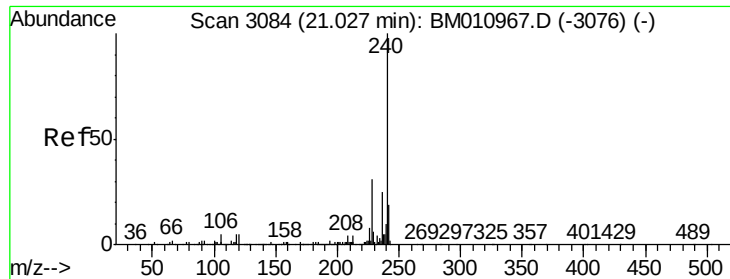

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.02 min Scan# 3100

Delta R.T. -0.01 min

Lab File: BM011027.D

Acq: 28 Jul 2017 00:59

Instrument :

BNA_M

ClientSampleId :


Tot Ion:240 Resp: 414460

Ion Ratio Lower Upper

240 100

120 4.0 8.2 12.2#




236 30.9 20.0 30.0#

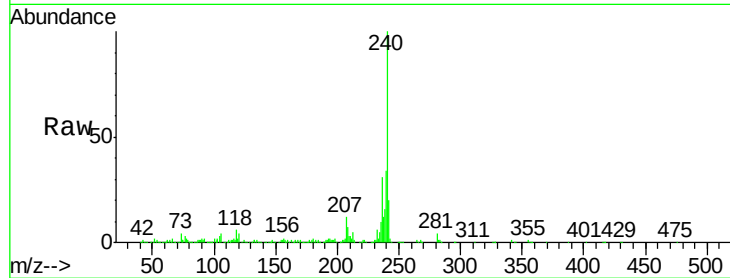

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

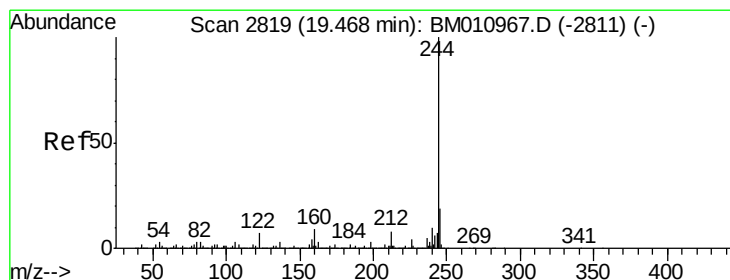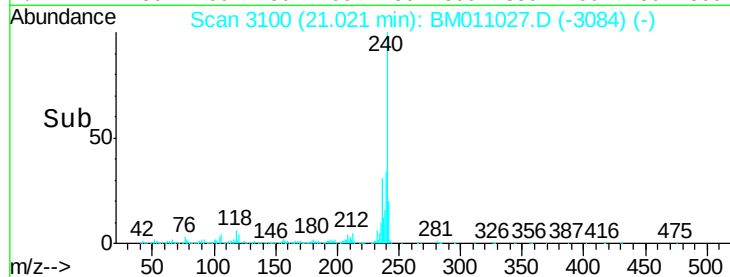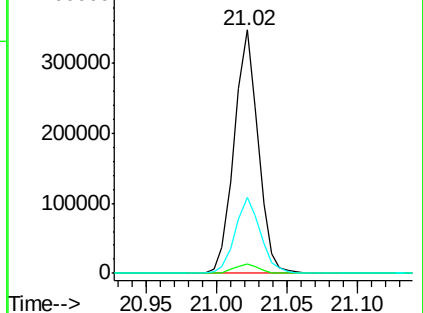

#78

Terphenyl-d14

Concen: 152.21 ng

RT: 19.47 min Scan# 2836

Delta R.T. 0.00 min

Lab File: BM011027.D

Acq: 28 Jul 2017 00:59


Tgt Ion:244 Resp: 3184659

Ion Ratio Lower Upper

244 100

212 8.8 4.9 7.3#



122 6.8 6.2 9.4

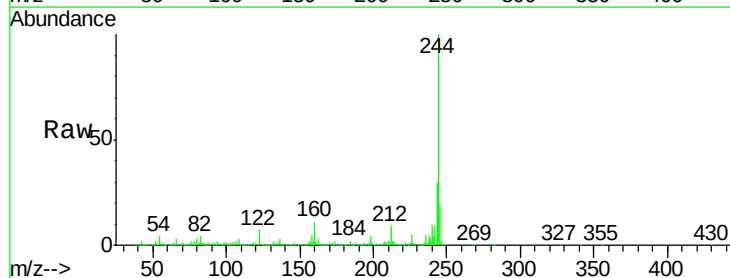


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

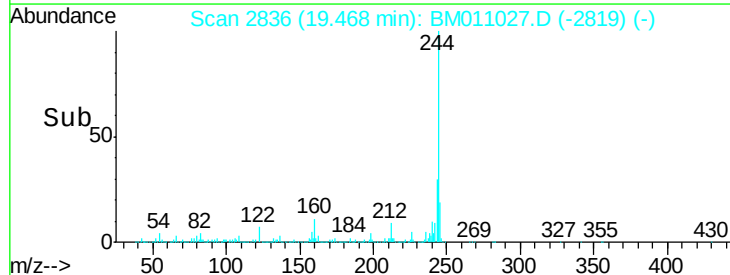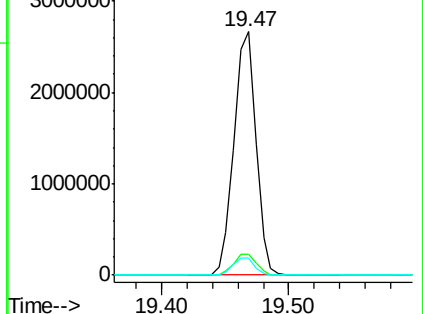

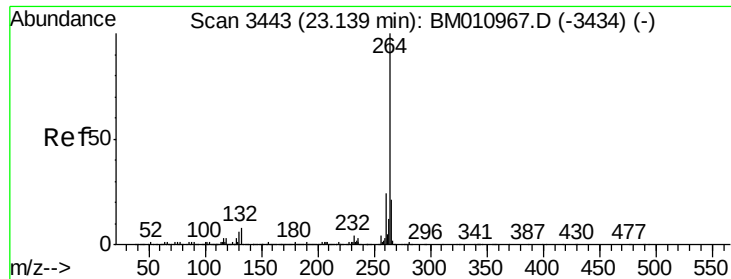

#86
Pervlene-d12
Concen: 20.00 ng
RT: 23.13 min Scan# 3459
Delta R.T. -0.01 min
Lab File: BM011027.D
Acq: 28 Jul 2017 00:59

Instrument :
BNA_M
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	108.6	18.6	27.8#
265	28.9	17.3	25.9#

