

Data Path : Z:\HPCHEM1\BNA M\DATA\BM072717\
 Data File : BM011012.D
 Acq On : 27 Jul 2017 15:59
 Operator : SJ/JU
 Sample : I4422-15
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 72-11940-COMP

Quant Time: Jul 28 03:26:04 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 26 17:29:06 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	161654	20.00	ng	0.00
21) Naphthalene-d8	10.15	136	573334	20.00	ng	0.00
38) Acenaphthene-d10	14.04	164	385781	20.00	ng	0.00
63) Phenanthrene-d10	16.80	188	1078306	20.00	ng	0.00
75) Chrysene-d12	21.02	240	1409168	20.00	ng	0.00
86) Perylene-d12	23.13	264	1249592	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.03	112	1323772	138.43	ng	0.00
7) Phenol-d6	6.59	99	1803044	132.70	ng	0.00
23) Nitrobenzene-d5	8.53	82	1556485	101.89	ng	0.00
41) 2,4,6-Tribromophenol	15.55	330	999037	161.57	ng	0.00
44) 2-Fluorobiphenyl	12.66	172	3010882	97.88	ng	0.00
78) Terphenyl-d14	19.47	244	6206851	87.25	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM072717\
Data File : BM011012.D
Acq On : 27 Jul 2017 15:59
Operator : SJ/JU
Sample : I4422-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
72-11940-COMP

Quant Time: Jul 28 03:26:04 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 17:29:06 2017
Response via : Initial Calibration

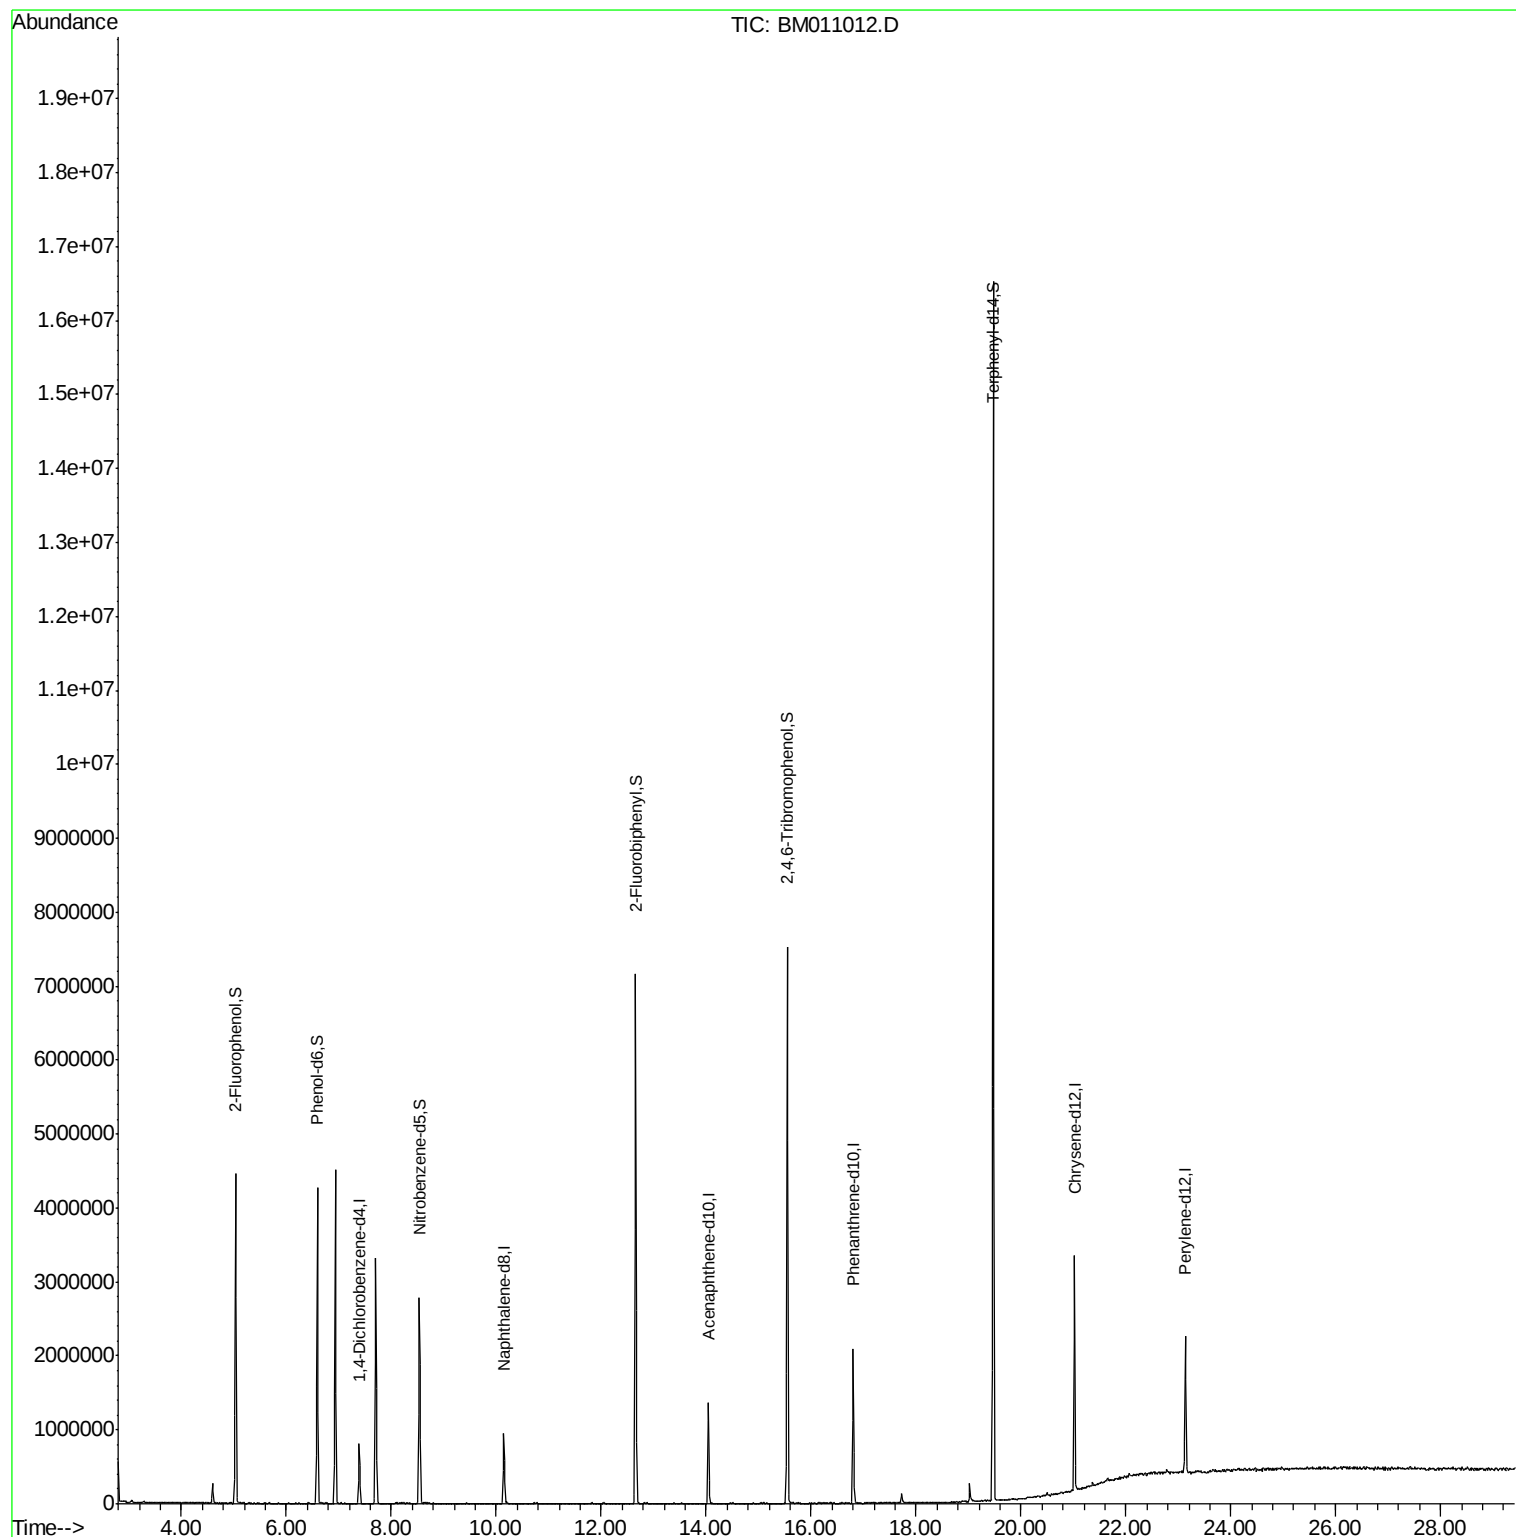




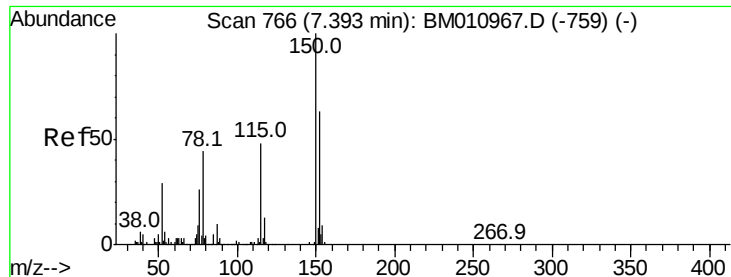


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.39 min Scan# 782
Delta R.T. -0.01 min
Lab File: BM011012.D
Acq: 27 Jul 2017 15:59

Instrument :
BNA_M
ClientSampleId :
72-11940-COMP




Tot Ion:152 Resp: 161654
Ion Ratio Lower Upper
152 100
150 146.3 119.5 179.3
115 66.2 43.0 64.4#

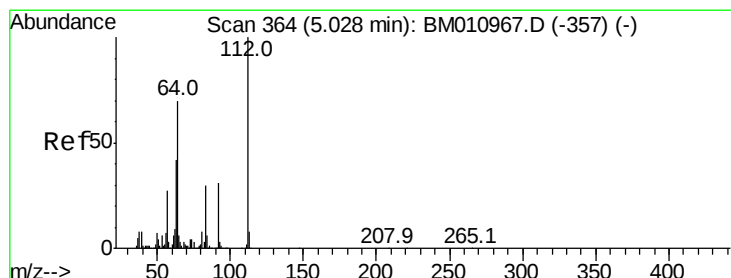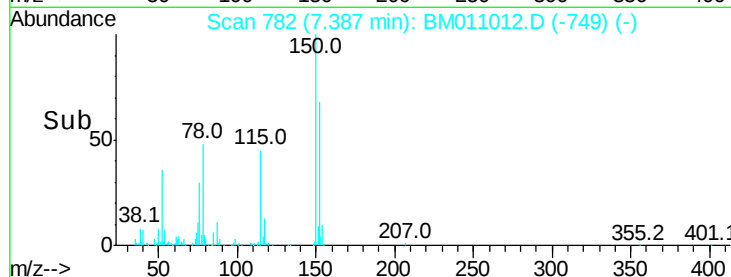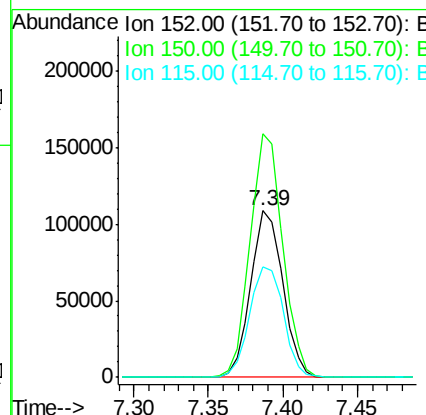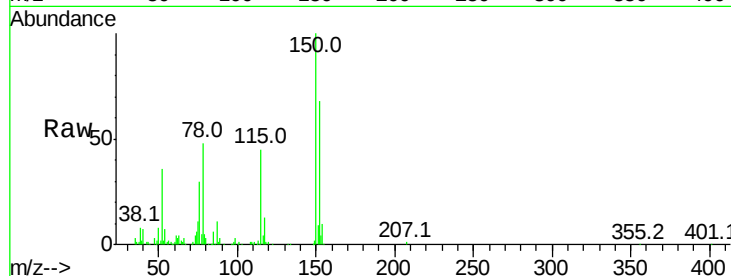


#5

2-Fluorophenol
Concen: 138.429 ng
RT: 5.03 min Scan# 382
Delta R.T. 0.01 min
Lab File: BM011012.D
Acq: 27 Jul 2017 15:59

Tgt Ion:112 Resp: 1323772
Ion Ratio Lower Upper
112 100
64 66.8 38.6 57.8#
63 44.5 19.3 28.9#

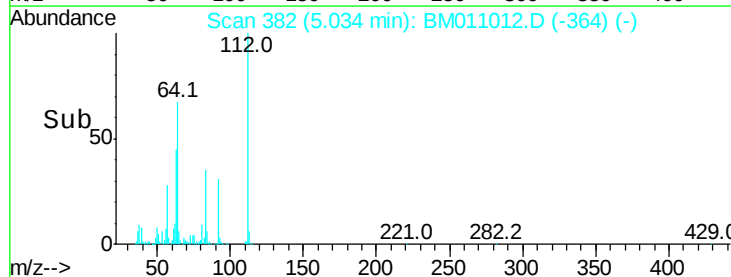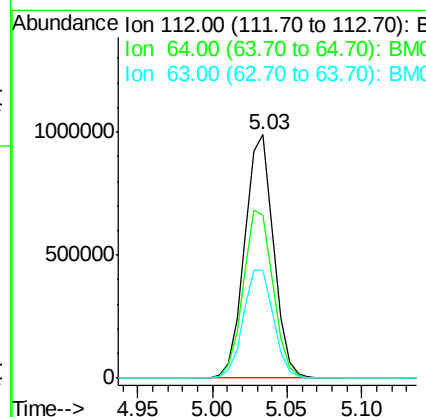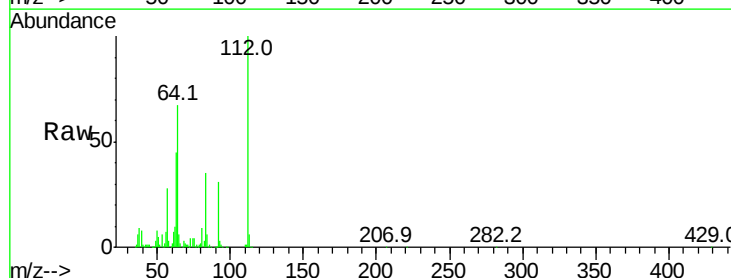

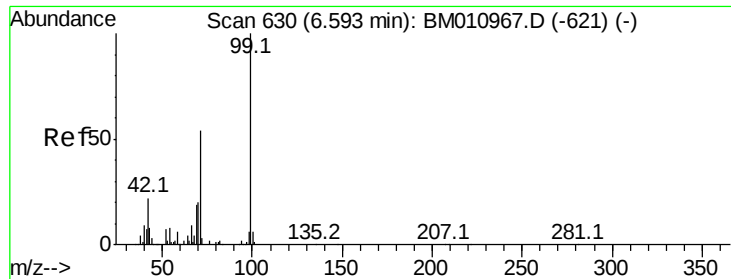

#7

Phenol-d6

Concen: 132.703 ng

RT: 6.59 min Scan# 647

Delta R.T. -0.00 min

Lab File: BM011012.D

Acq: 27 Jul 2017 15:59

Instrument :

BNA_M

ClientSampleId :

72-11940-COMP


Tot Ion: 99 Resp: 1803044

Ion Ratio Lower Upper

99 100

42 24.0 11.0 16.4#




71 58.9 23.4 35.2#

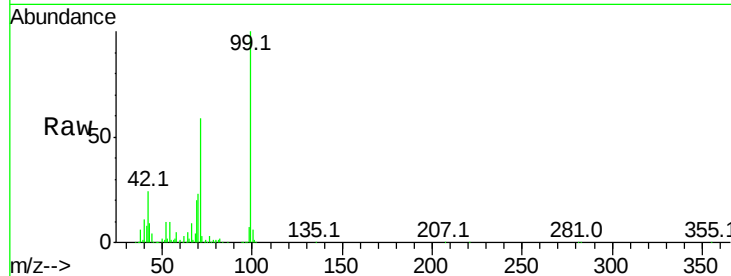

Abundance Ion 99.00 (98.70 to 99.70): BM011012.D (-630) (-)

Ion 42.00 (41.70 to 42.70): BM011012.D (-630) (-)

Ion 71.00 (70.70 to 71.70): BM011012.D (-630) (-)

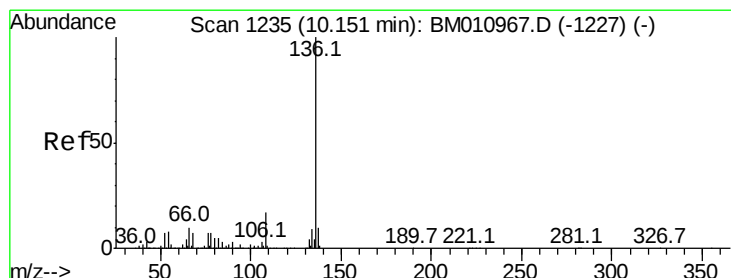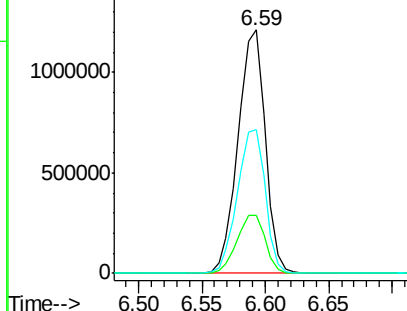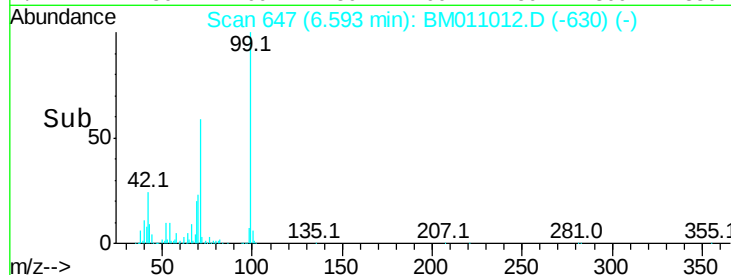

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.15 min Scan# 1251

Delta R.T. -0.01 min

Lab File: BM011012.D

Acq: 27 Jul 2017 15:59

Tgt Ion: 136 Resp: 573334


Ion Ratio Lower Upper

136 100

137 11.2 8.7 13.1

54 7.0 4.6 6.8#

68 6.6 3.7 5.5#


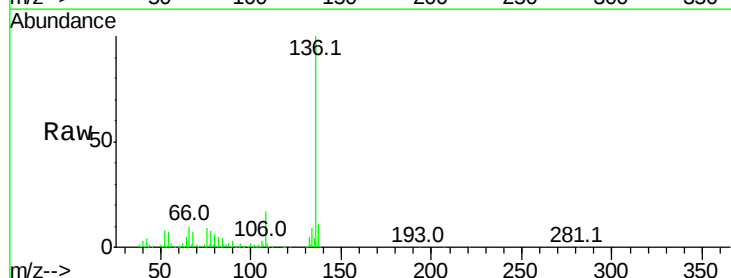


Abundance Ion 136.00 (135.70 to 136.70): BM011012.D (-1235) (-)

Ion 137.00 (136.70 to 137.70): BM011012.D (-1235) (-)

Ion 54.00 (53.70 to 54.70): BM011012.D (-1235) (-)

Ion 68.00 (67.70 to 68.70): BM011012.D (-1235) (-)

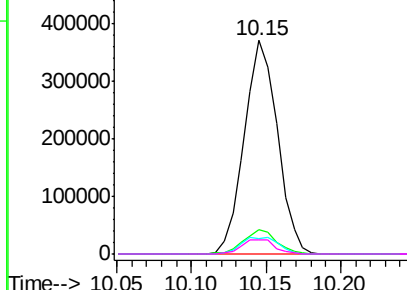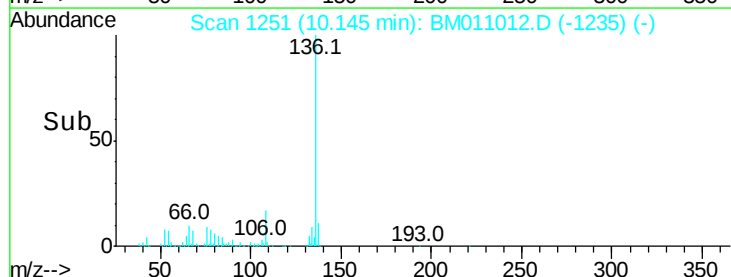



#23

Nitrobenzene-d5

Concen: 101.891 ng

RT: 8.53 min Scan# 977

Delta R.T. -0.01 min

Lab File: BM011012.D

Acq: 27 Jul 2017 15:59

Instrument :

BNA_M

ClientSampleId :

72-11940-COMP





Tot Ion: 82 Resp: 1556485

Ion Ratio Lower Upper

82 100

128 25.5 32.8 49.2#

54 49.6 40.6 60.8

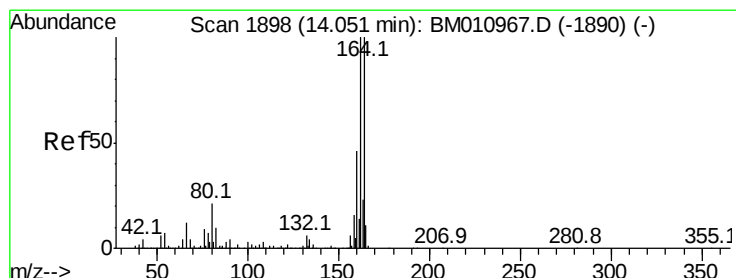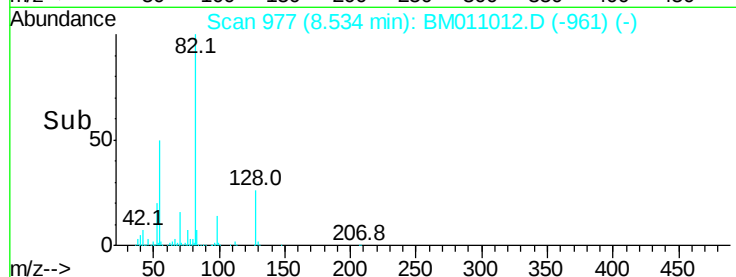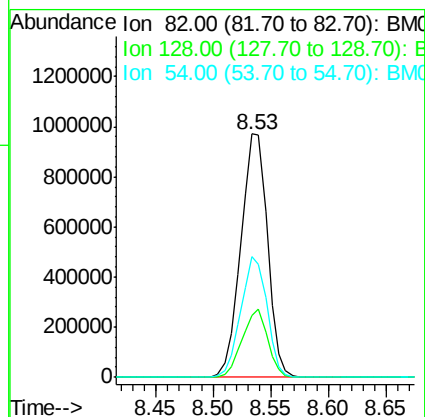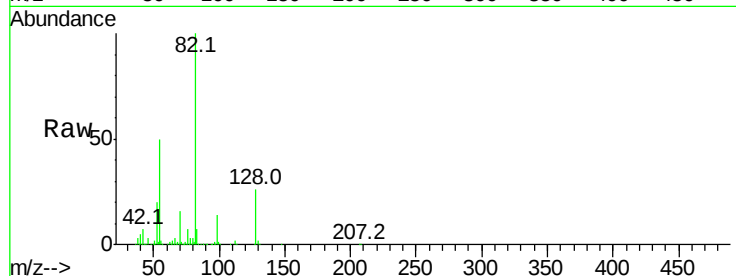

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.04 min Scan# 1914

Delta R.T. -0.01 min

Lab File: BM011012.D

Acq: 27 Jul 2017 15:59




Tgt Ion:164 Resp: 385781

Ion Ratio Lower Upper

164 100

162 101.6 82.4 123.6

160 44.4 35.8 53.6

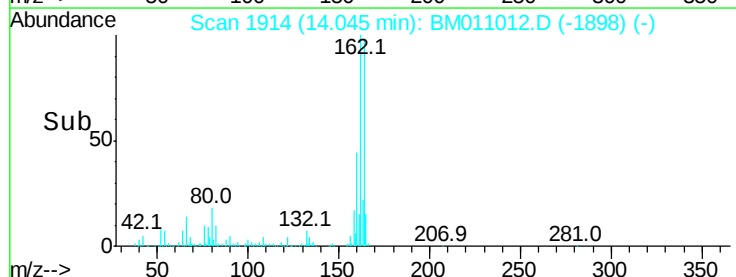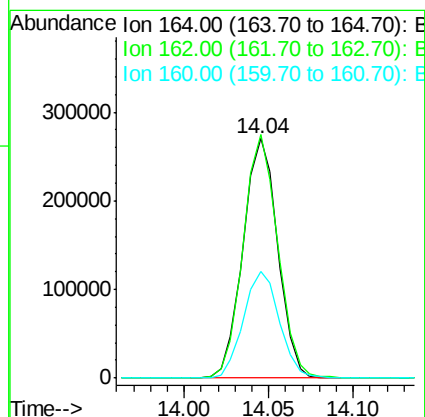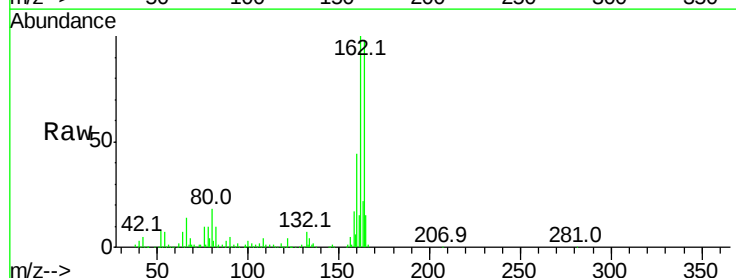






#41
 2,4,6-Tribromophenol
 Concen: 161.571 ng
 RT: 15.55 min Scan# 2170
 Delta R.T. -0.01 min
 Lab File: BM011012.D
 Acq: 27 Jul 2017 15:59

Instrument :
 BNA_M
 ClientSampleId :
 72-11940-COMP

Tot Ion:330 Resp: 999037
 Ion Ratio Lower Upper
 330 100
 332 95.9 0.0 0.0#
 141 45.2 0.0 0.0#

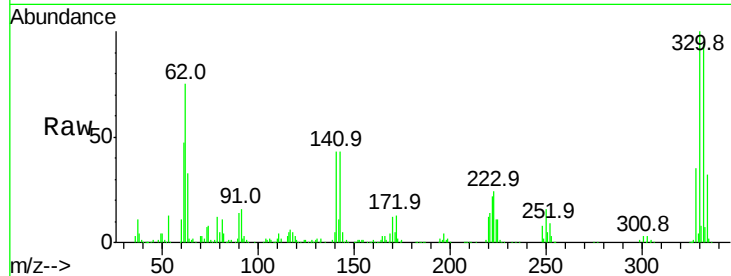


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

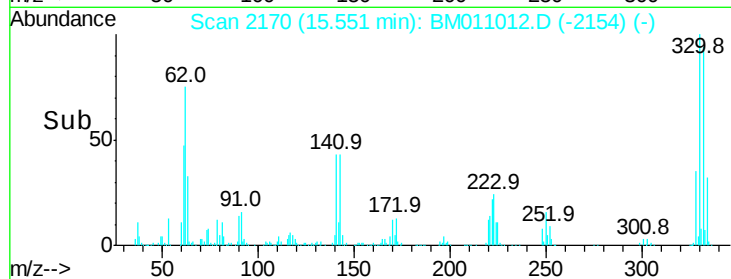
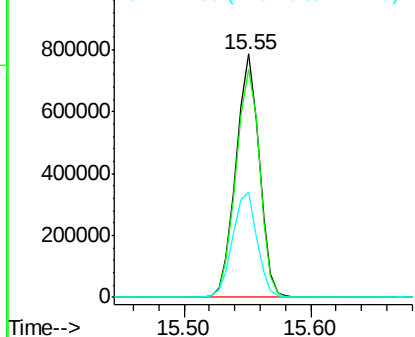



#44
 2-Fluorobiphenyl
 Concen: 97.881 ng
 RT: 12.66 min Scan# 1678
 Delta R.T. -0.01 min
 Lab File: BM011012.D
 Acq: 27 Jul 2017 15:59

Tgt Ion:172 Resp: 3010882
 Ion Ratio Lower Upper
 172 100
 171 35.2 28.5 42.7
 170 23.8 18.8 28.2

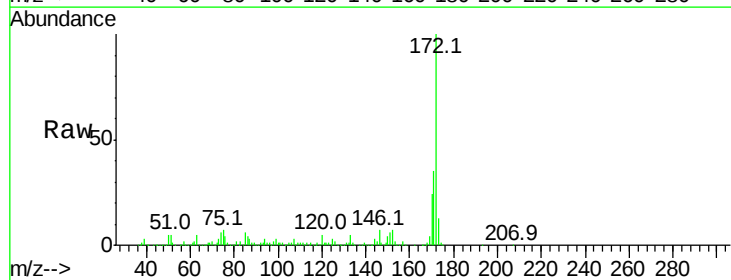

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



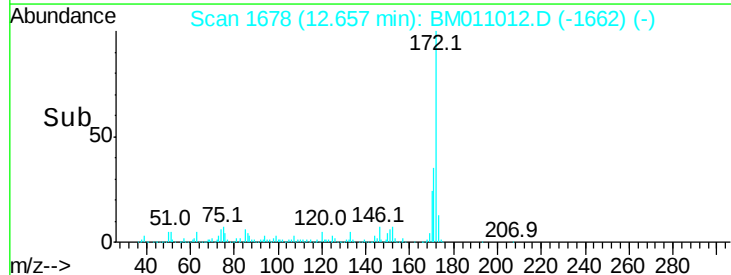
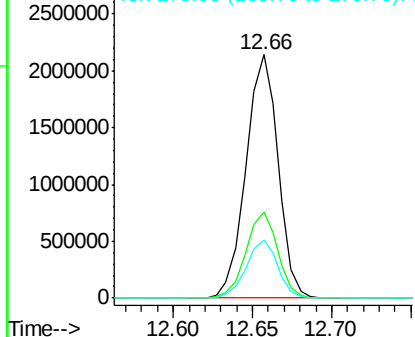


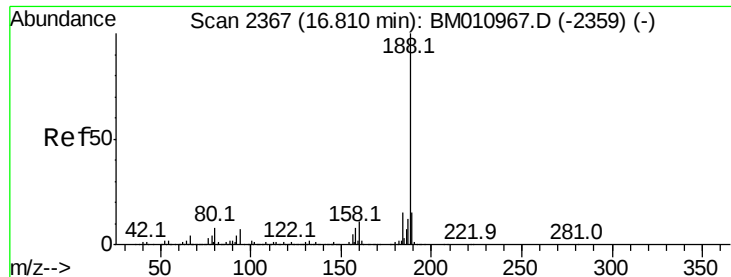

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.80 min Scan# 2383
Delta R.T. -0.01 min
Lab File: BM011012.D
Acq: 27 Jul 2017 15:59




Instrument :
BNA_M
ClientSampleId :
72-11940-COMP


Tot Ion:188 Resp: 1078306
Ion Ratio Lower Upper
188 100
94 6.3 8.7 13.1#
80 7.6 9.3 13.9#

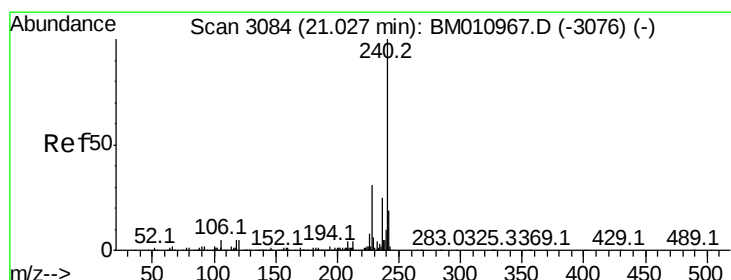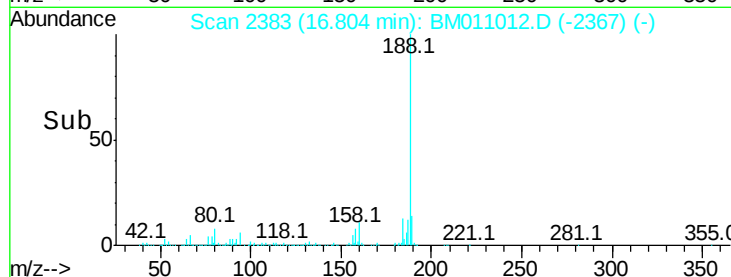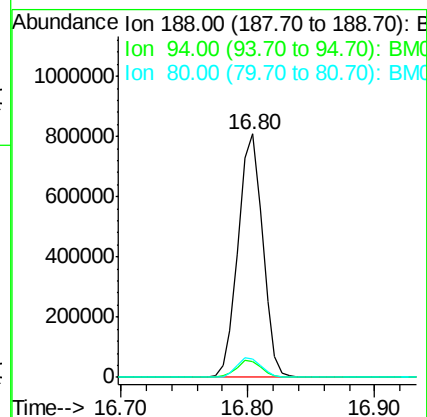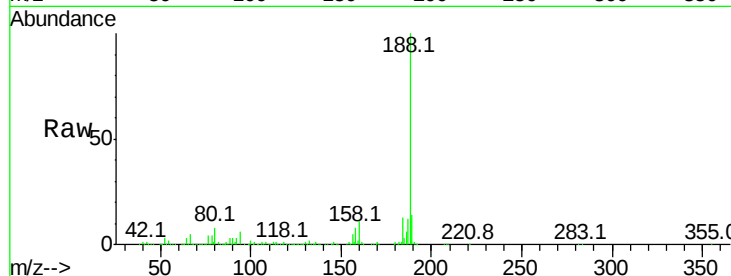

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.02 min Scan# 3100
Delta R.T. -0.01 min
Lab File: BM011012.D
Acq: 27 Jul 2017 15:59

Tgt Ion:240 Resp: 1409168
Ion Ratio Lower Upper
240 100
120 4.3 8.2 12.2#
236 24.6 20.0 30.0

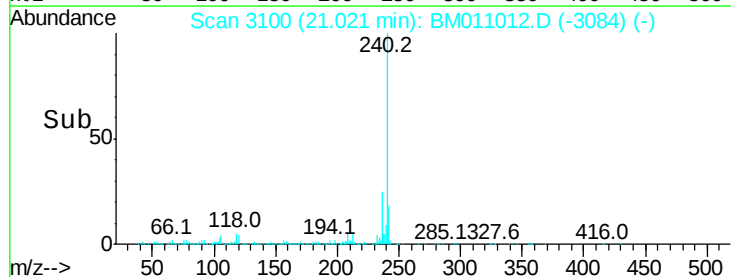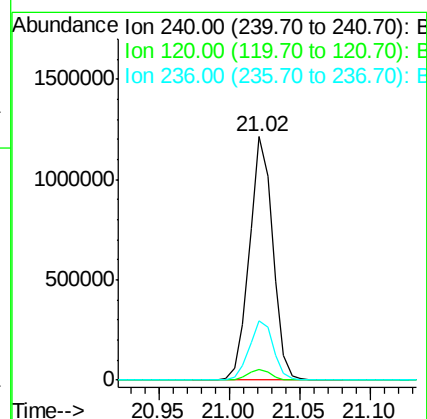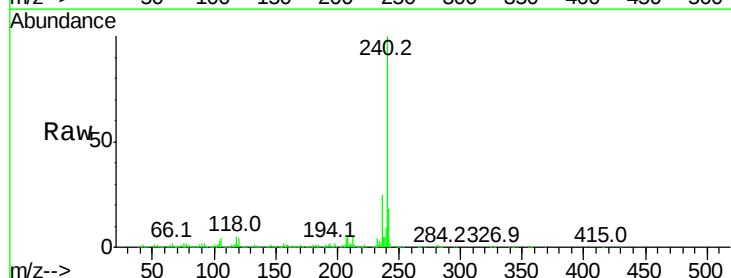

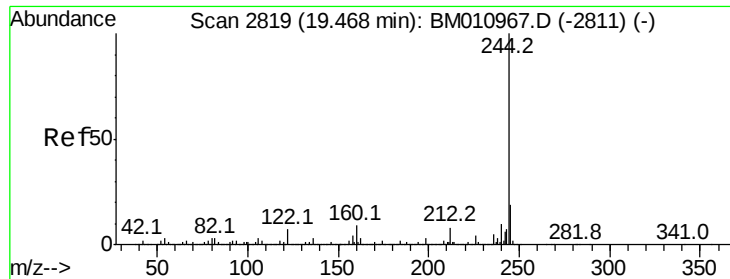

#78

Terphenyl-d14

Concen: 87.250 ng

RT: 19.47 min Scan# 2836

Delta R.T. -0.00 min

Lab File: BM011012.D

Acq: 27 Jul 2017 15:59

Instrument :

BNA_M

ClientSampleId :

72-11940-COMP


Tot Ion:244 Resp: 6206851

Ion Ratio Lower Upper

244 100

212 8.8 4.9 7.3#




122 7.0 6.2 9.4

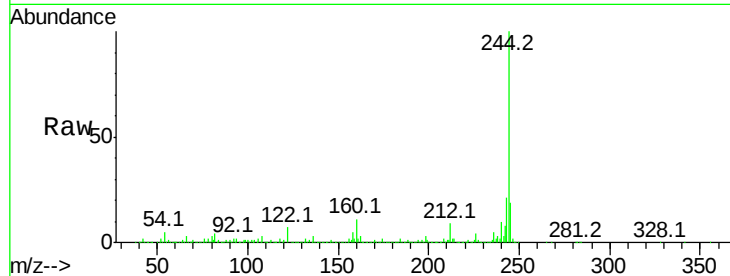

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

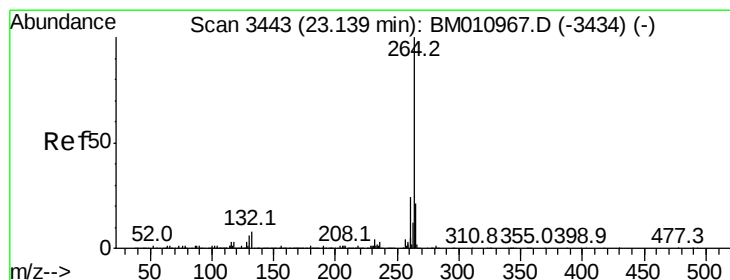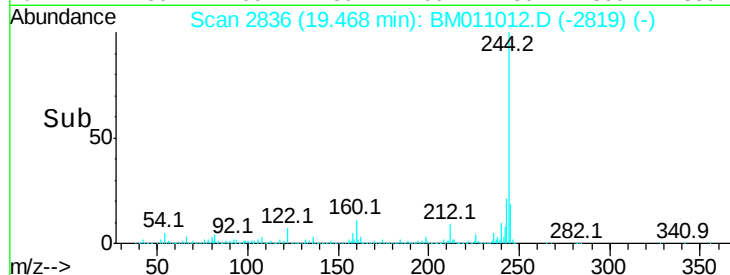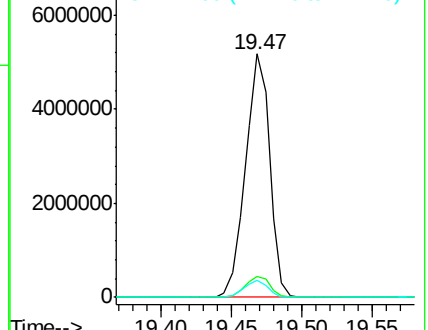

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.13 min Scan# 3459

Delta R.T. -0.01 min

Lab File: BM011012.D

Acq: 27 Jul 2017 15:59


Tgt Ion:264 Resp: 1249592

Ion Ratio Lower Upper

264 100

260 24.4 18.6 27.8

265 22.0 17.3 25.9

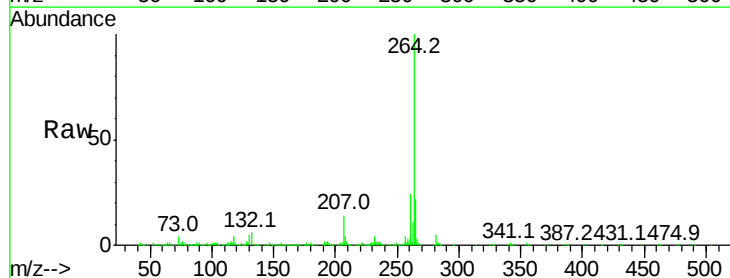

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

