

Data Path : Z:\HPCHEM1\BNA M\DATA\BM072717\
Data File : BM011014.D
Acq On : 27 Jul 2017 17:11
Operator : SJ/JU
Sample : I4432-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RINSEBLANK-GW

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.028	375	381	388	rBV	2165953	2895233	15.96%	4.112%
2	6.581	636	645	654	rBV	1308363	1950837	10.75%	2.771%
3	6.928	697	704	714	rBV	3731880	5493439	30.28%	7.803%
4	7.386	776	782	789	rBV	764849	1172155	6.46%	1.665%
5	7.704	827	836	845	rVB	3057324	4795997	26.43%	6.812%
6	8.533	970	977	986	rBV	2861385	4520835	24.92%	6.421%
7	10.145	1242	1251	1260	rBV	898442	1481097	8.16%	2.104%
8	12.657	1670	1678	1687	rBV	7013741	9977671	54.99%	14.172%
9	14.045	1907	1914	1922	rBV2	1359001	1977089	10.90%	2.808%
10	15.551	2163	2170	2180	rBV	7215905	9575055	52.77%	13.600%
11	16.804	2376	2383	2394	rVB2	2015537	2754224	15.18%	3.912%
12	19.468	2830	2836	2844	rBV	15819062	18143766	100.00%	25.770%
13	21.021	3095	3100	3106	rBV	2625037	3173192	17.49%	4.507%
14	23.133	3453	3459	3468	rVB	1460731	2494815	13.75%	3.543%


Sum of corrected areas: 70405405

Data Path : Z:\HPCHEM1\BNA M\DATA\BM072717\
Data File : BM011014.D
Acq On : 27 Jul 2017 17:11
Operator : SJ/JU
Sample : I4432-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RINSEBLANK-GW

Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

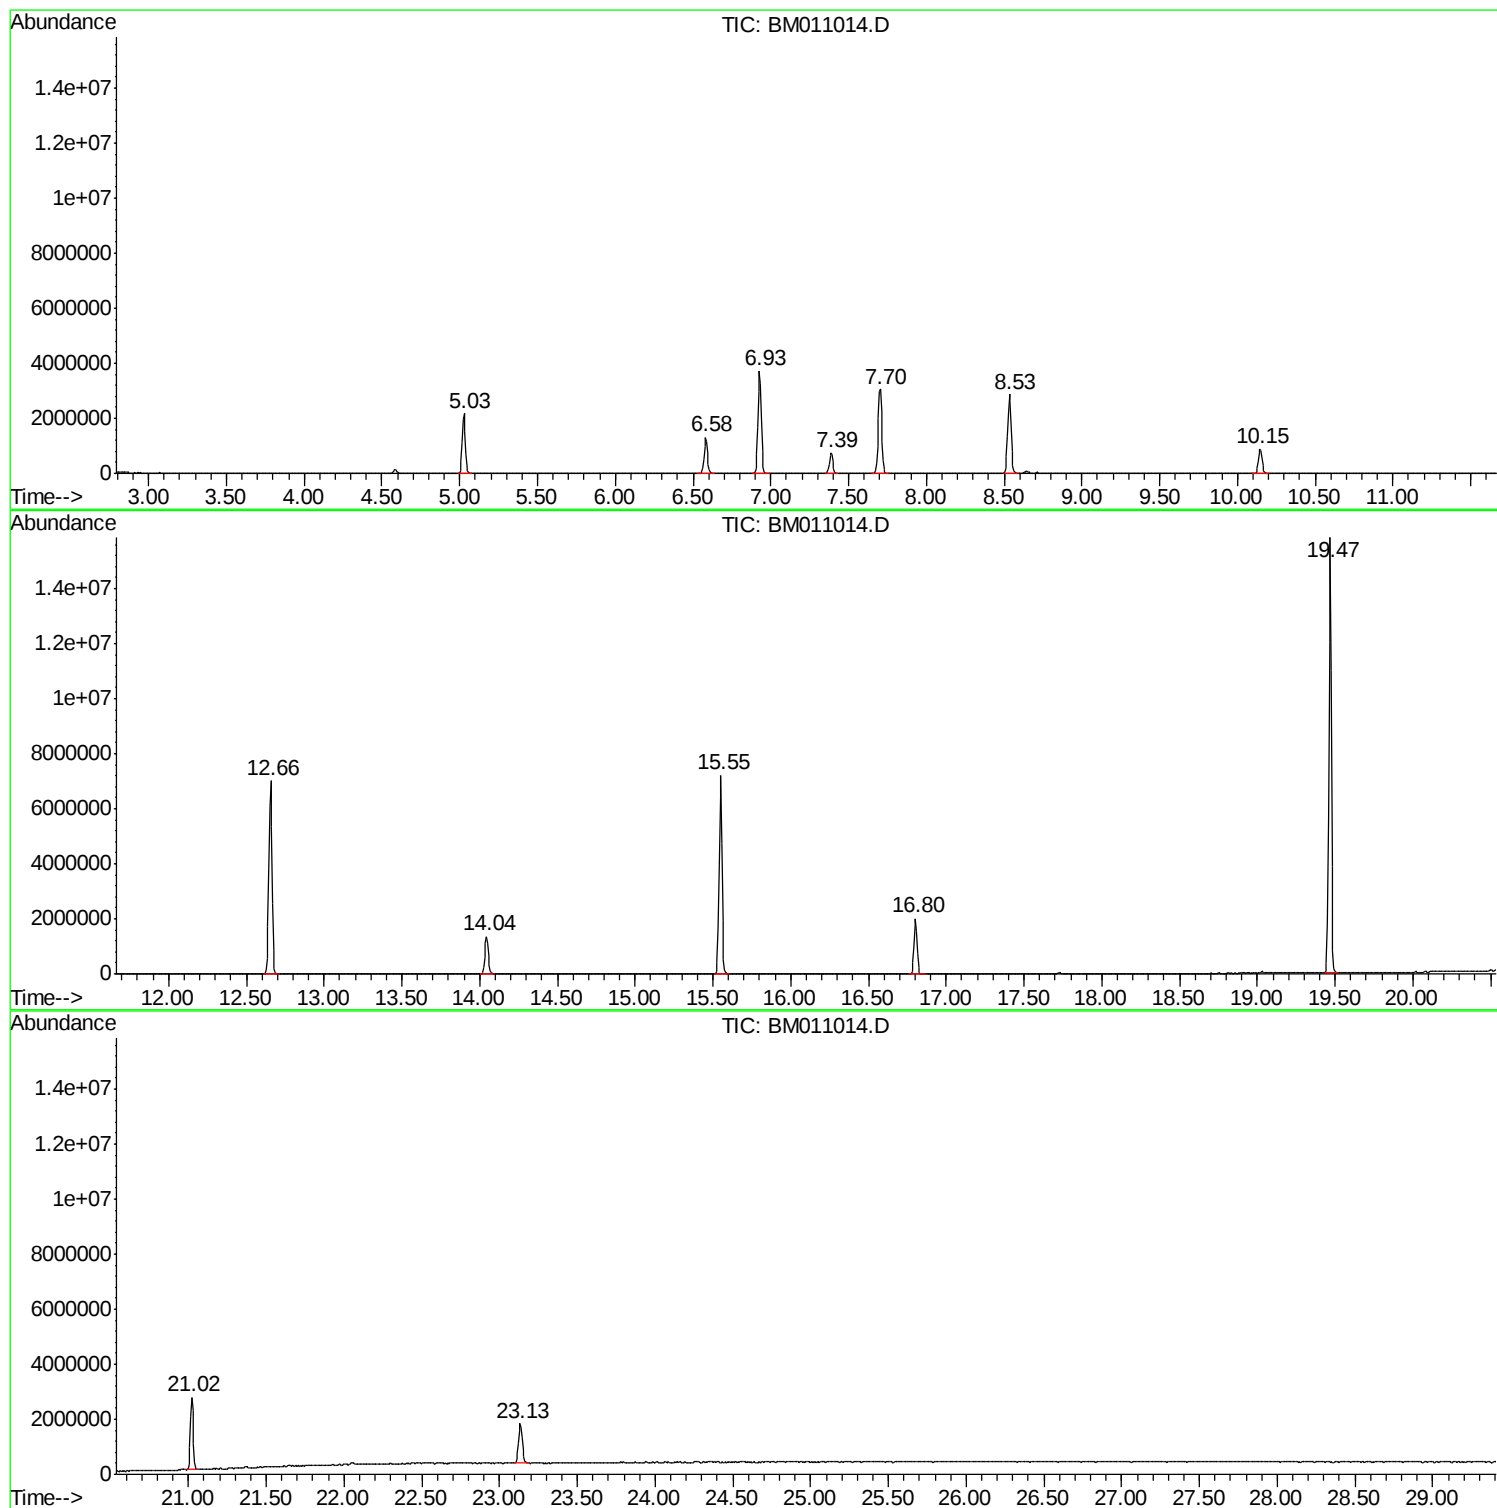

Data Path : Z:\HPCHEM1\BNA M\DATA\BM072717\
Data File : BM011014.D
Acq On : 27 Jul 2017 17:11
Operator : SJ/JU
Sample : I4432-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RINSEBLANK-GW










Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.93 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.93	93.73 ng	5493440	1,4-Dichlorobenzene-d4	7.39

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1-Penten-3-yne	66	C5H6	000646-05-9	38
2		3-Oxabicyclo[3.2.0]hept-6-ene-2,...	138	C7H6O3	064197-88-2	25
3		3-Penten-1-yne, (E)-	66	C5H6	002004-69-5	25
4		1,3-Cyclopentadiene	66	C5H6	000542-92-7	25
5		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	18

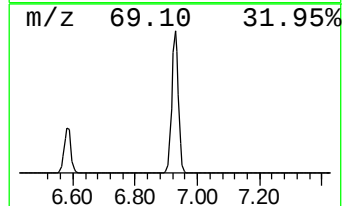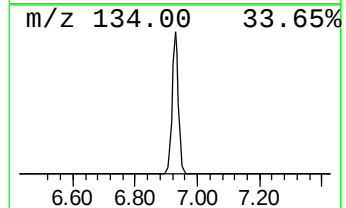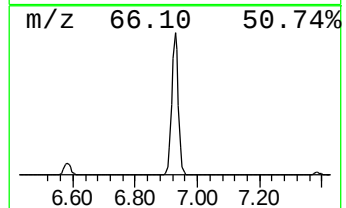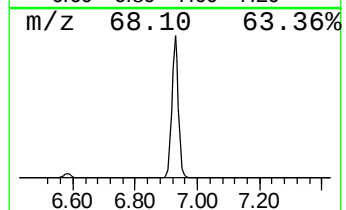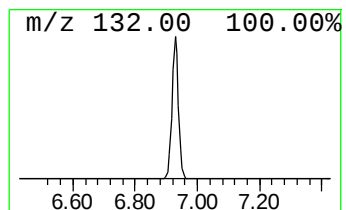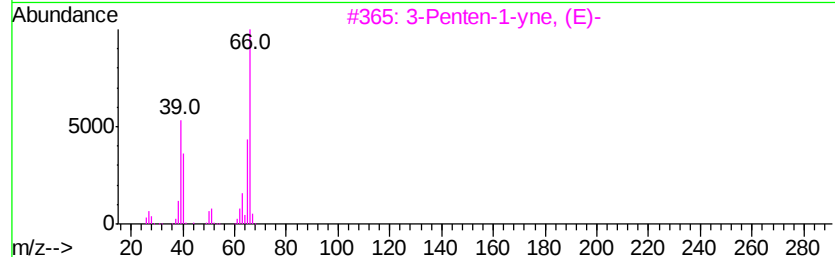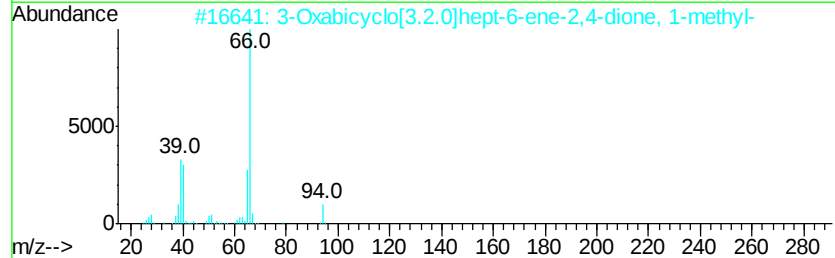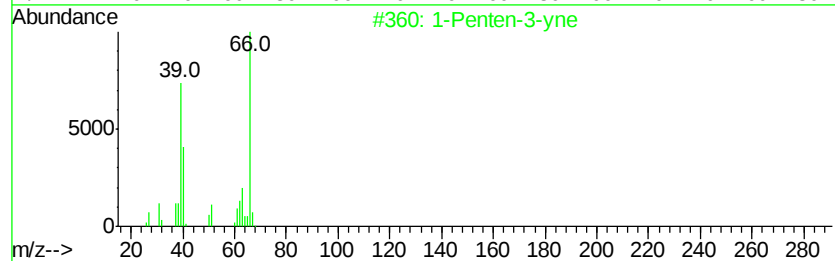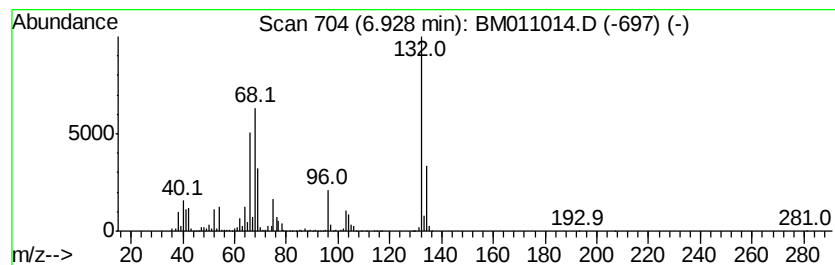

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072717\
Data File : BM011014.D
Acq On : 27 Jul 2017 17:11
Operator : SJ/JU
Sample : I4432-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RINSEBLANK-GW

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.93	6.93	93.7	ng	5493440	1	7.39	1172160	20.0