

Data Path : Z:\HPCHEM1\BNA M\DATA\BM072717\
 Data File : BM011016.D
 Acq On : 27 Jul 2017 18:23
 Operator : SJ/JU
 Sample : I4432-09
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MW-4

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.028	374	381	392	rVB	561872	824403	12.97%	2.338%
2	6.581	638	645	654	rBV2	379091	631029	9.93%	1.790%
3	6.928	697	704	717	rVB	1089202	1631673	25.67%	4.628%
4	7.387	776	782	789	rBV	735654	1109809	17.46%	3.148%
5	7.698	825	835	845	rVB	911367	1468043	23.10%	4.164%
6	8.534	970	977	988	rBV	866363	1365756	21.49%	3.874%
7	10.145	1244	1251	1262	rBV	917482	1475361	23.21%	4.185%
8	12.651	1671	1677	1685	rBV	2104800	3198922	50.33%	9.073%
9	13.516	1818	1824	1833	rBV	102066	149488	2.35%	0.424%
10	14.045	1906	1914	1922	rBV3	1447341	2207995	34.74%	6.263%
11	14.945	2061	2067	2072	rBV6	50975	74774	1.18%	0.212%
12	15.545	2163	2169	2177	rBV	2273749	3138299	49.37%	8.901%
13	16.657	2353	2358	2363	rBV3	194942	254112	4.00%	0.721%
14	16.804	2376	2383	2392	rBV	2204315	3061985	48.17%	8.685%
15	17.727	2534	2540	2547	rBV3	170927	246151	3.87%	0.698%
16	18.621	2688	2692	2696	rBV7	61346	72888	1.15%	0.207%
17	19.027	2754	2761	2768	rBV6	172181	252354	3.97%	0.716%
18	19.462	2829	2835	2843	rBV	5167014	6356417	100.00%	18.029%
19	21.021	3095	3100	3106	rBV	3413646	4097214	64.46%	11.621%
20	23.133	3453	3459	3467	rBV2	2136800	3639605	57.26%	10.323%


Sum of corrected areas: 35256278

Data Path : Z:\HPCHEM1\BNA M\DATA\BM072717\
Data File : BM011016.D
Acq On : 27 Jul 2017 18:23
Operator : SJ/JU
Sample : I4432-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MW-4

Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

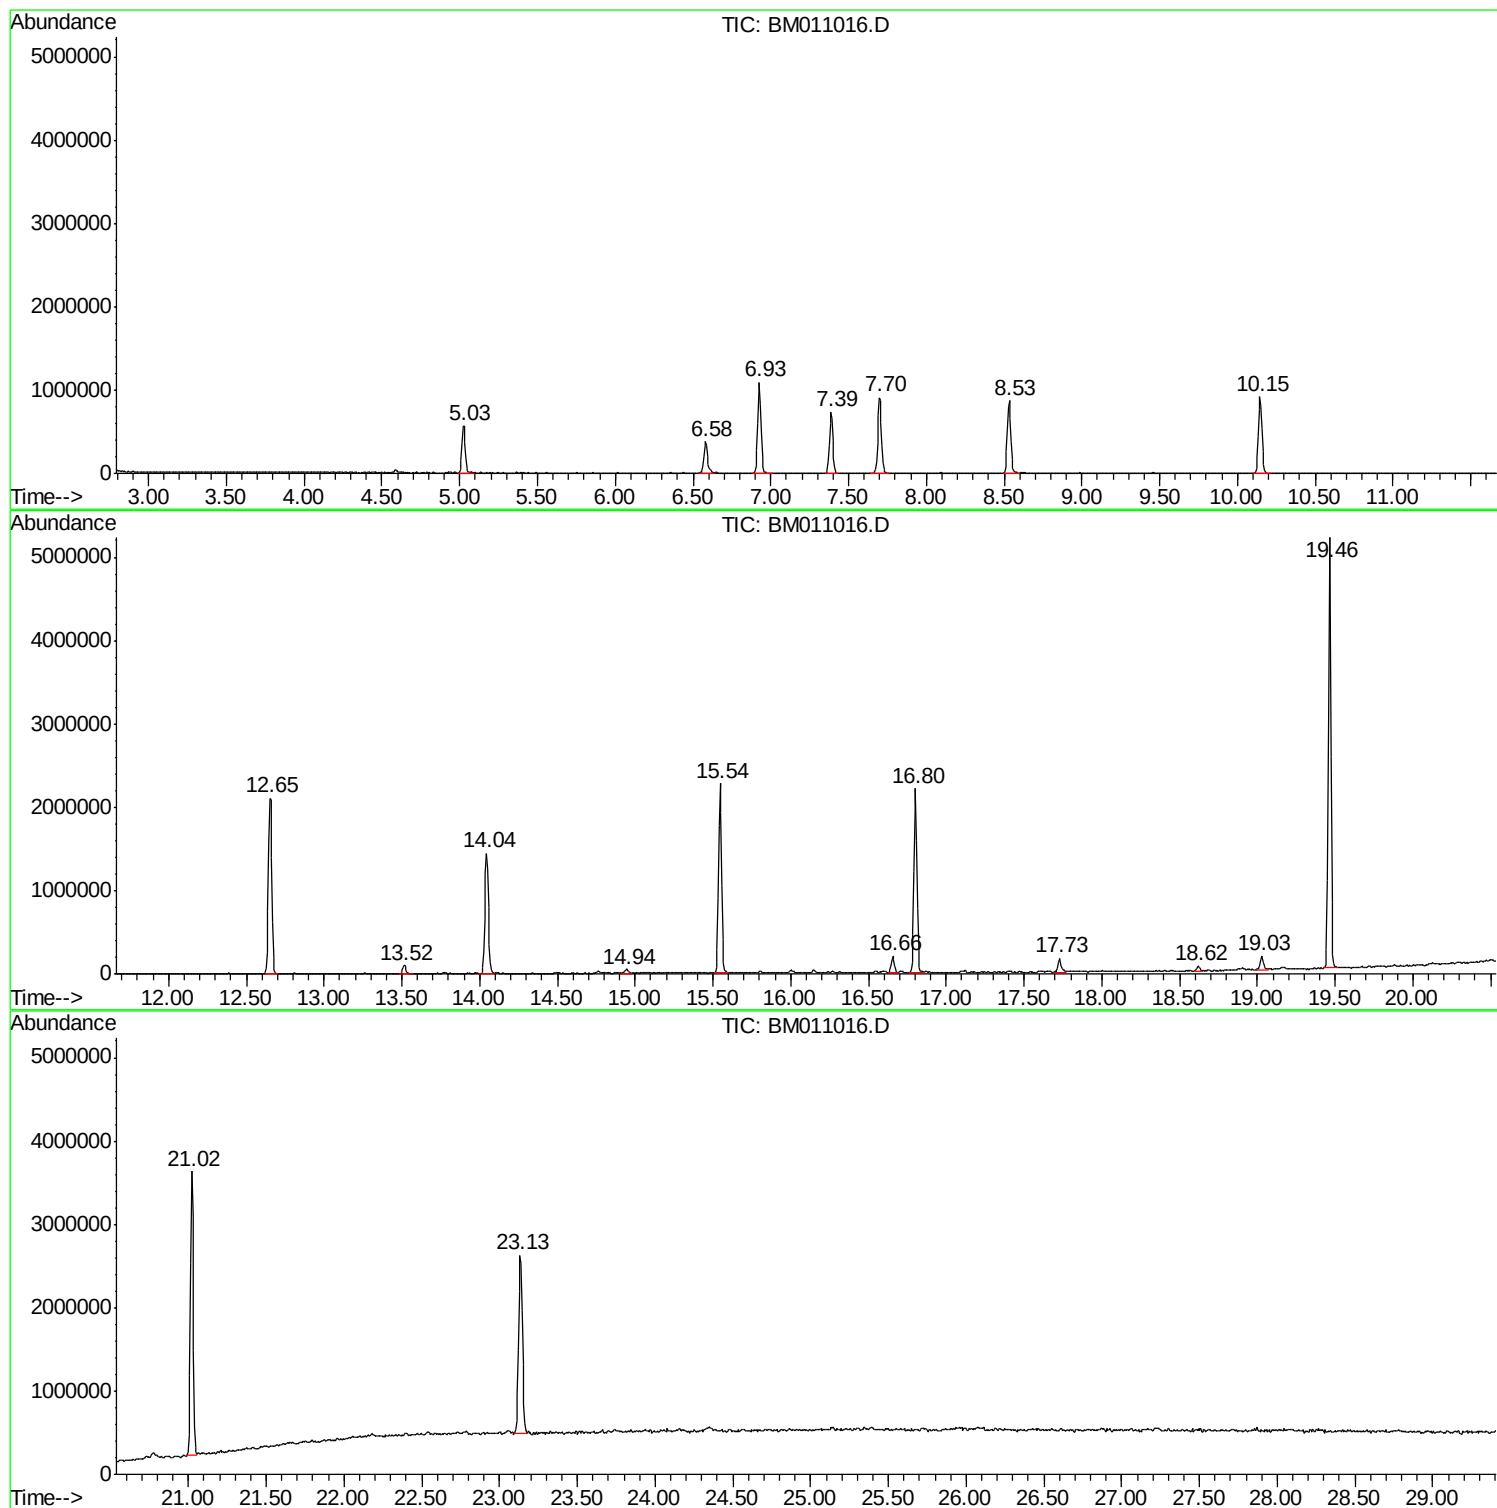

Data Path : Z:\HPCHEM1\BNA M\DATA\BM072717\
Data File : BM011016.D
Acq On : 27 Jul 2017 18:23
Operator : SJ/JU
Sample : I4432-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MW-4










Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.93 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.93	29.40 ng	1631670	1,4-Dichlorobenzene-d4	7.39

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1-Penten-3-yne	66	C5H6	000646-05-9	38
2		3-Penten-1-yne, (E)-	66	C5H6	002004-69-5	25
3		3-Oxabicyclo[3.2.0]hept-6-ene-2,...	138	C7H6O3	064197-88-2	25
4		endo-4-Oxatricyclo[5.2.1.0(2,6)]...	136	C9H12O	001528-23-0	25
5		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	18

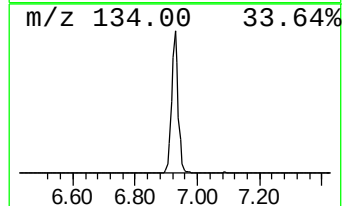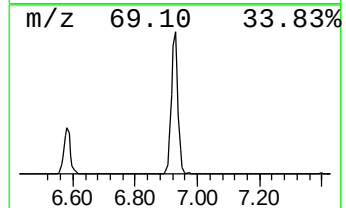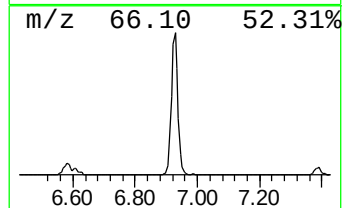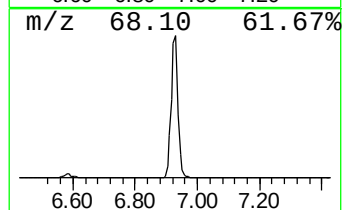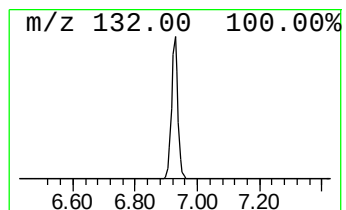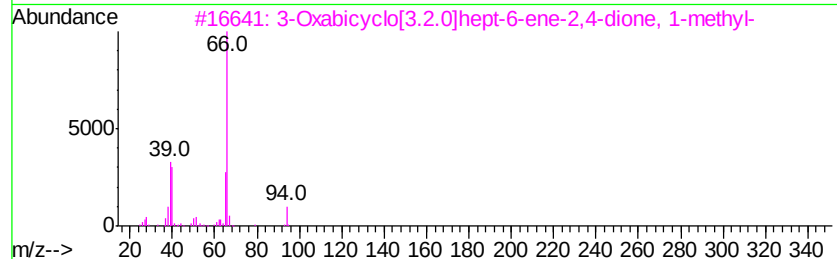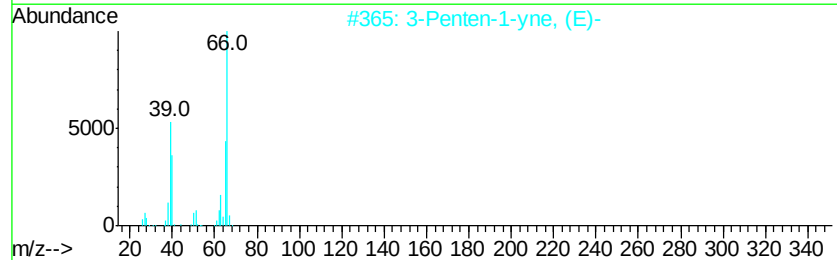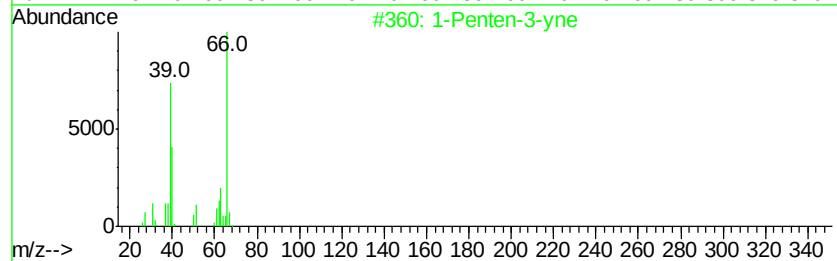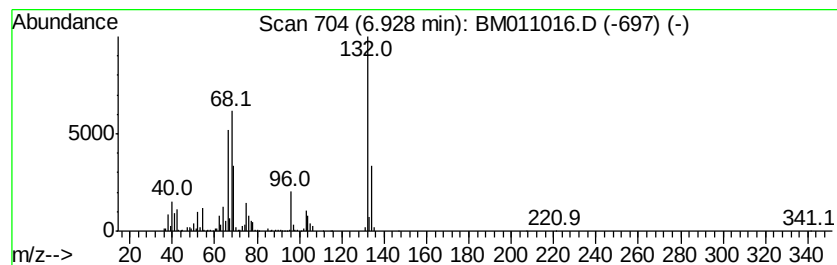

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072717\
Data File : BM011016.D
Acq On : 27 Jul 2017 18:23
Operator : SJ/JU
Sample : I4432-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MW-4

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.93	6.93	29.4	ng	1631670	1	7.39	1109810	20.0