


Data Path : Z:\HPCHEM1\BNA M\Data\BM072717\
 Data File : BM011000.D
 Acq On : 27 Jul 2017 08:49
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 26 17:29:06 2017

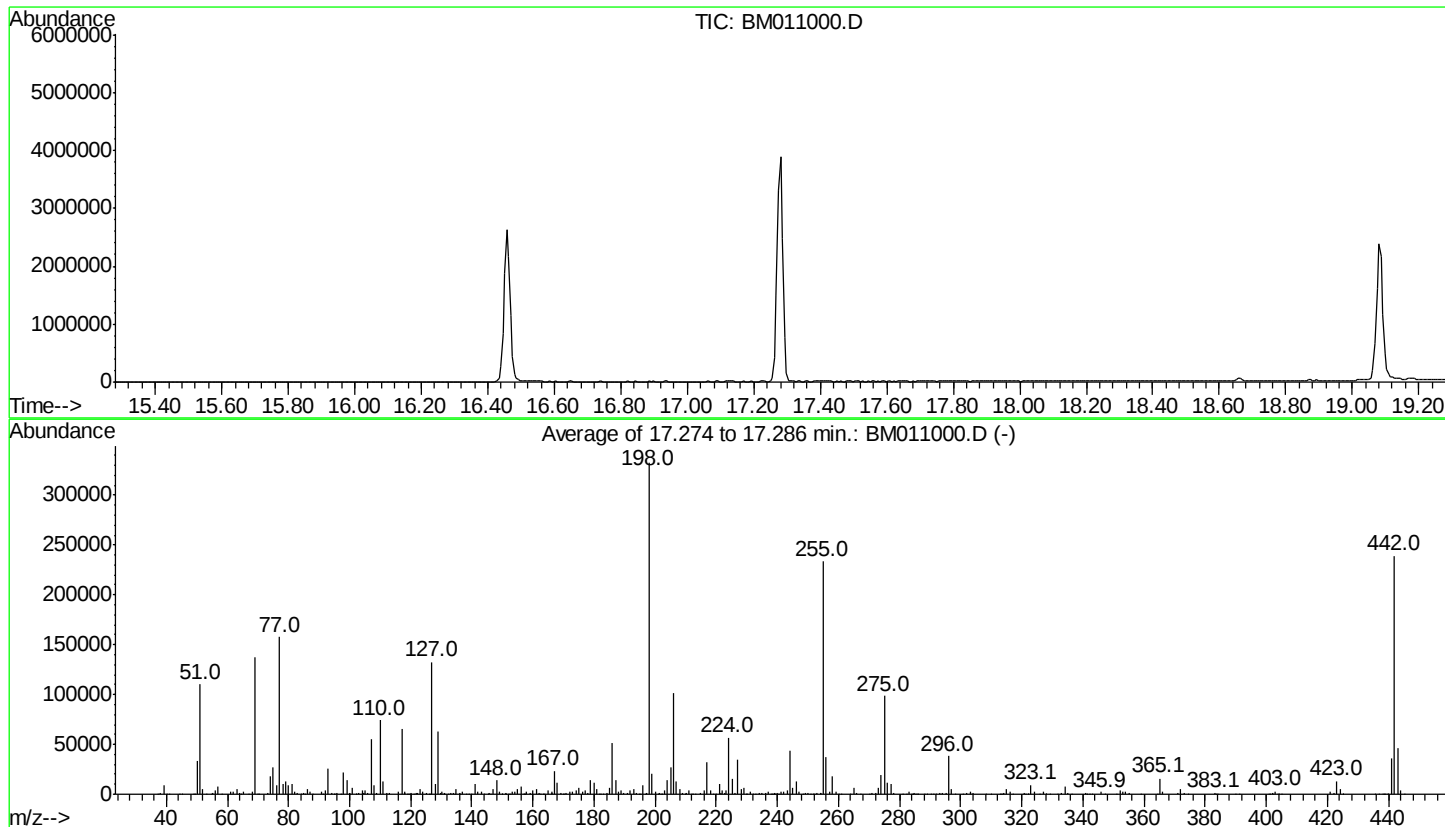

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	110368	PASS
68	69	0.00	2	1.5	2116	PASS
69	198	0.00	100	41.2	137010	PASS
70	69	0.00	2	0.3	409	PASS
127	198	10	80	39.9	132581	PASS
197	198	0.00	2	0.5	1633	PASS
198	198	100	100	100.0	332608	PASS
199	198	5	9	6.1	20179	PASS
275	198	10	60	29.7	98682	PASS
365	198	1	100	4.6	15417	PASS
441	443	0.01	100	78.2	35920	PASS
442	198	50	100	72.0	239445	PASS
443	442	15	24	19.2	45936	PASS