


Data Path : Z:\HPCHEM1\BNA M\Data\BM072717\
 Data File : BM011020.D
 Acq On : 27 Jul 2017 20:47
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 26 17:29:06 2017

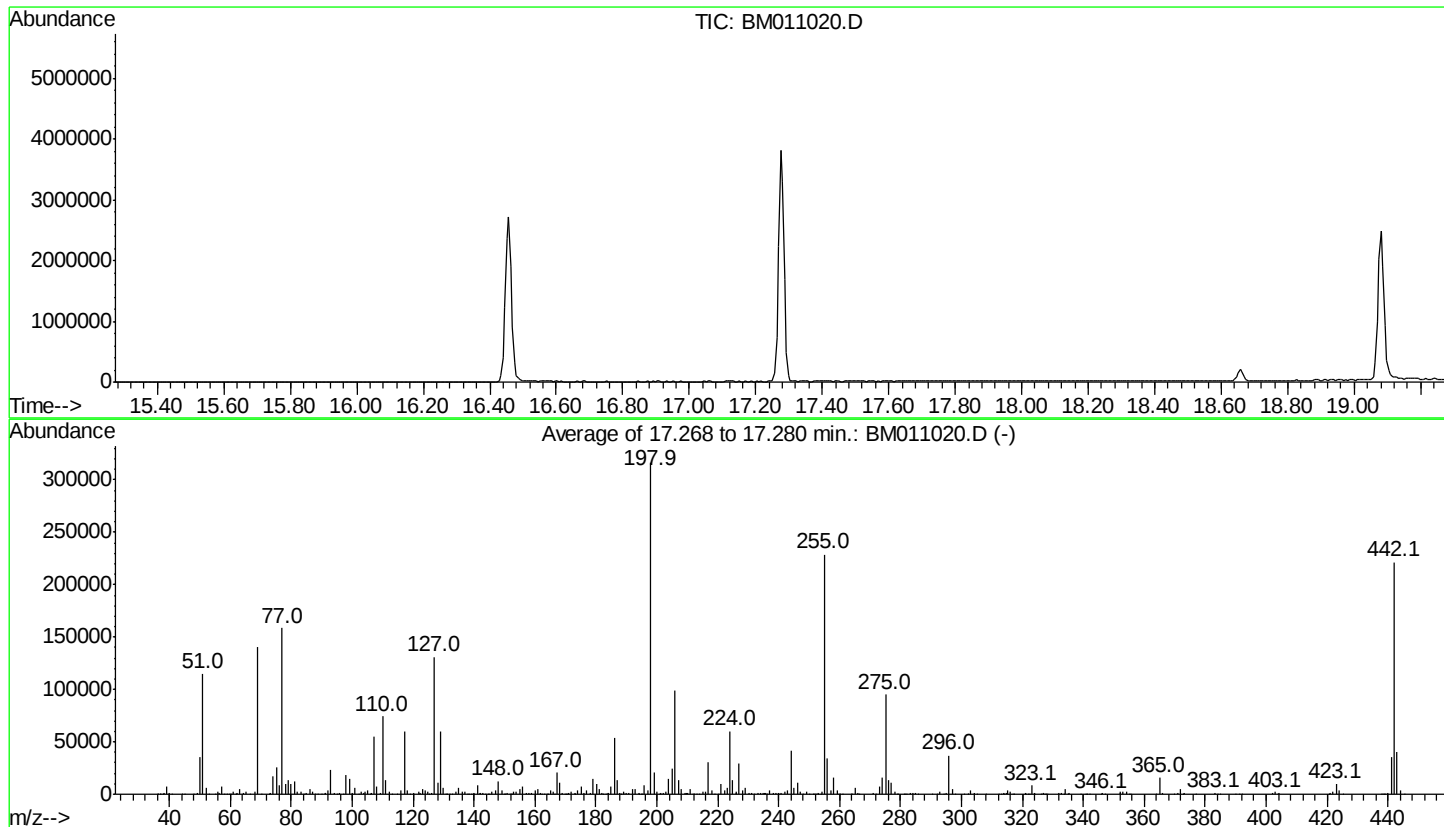

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	115448	PASS
68	69	0.00	2	1.7	2413	PASS
69	198	0.00	100	44.6	141109	PASS
70	69	0.00	2	0.4	573	PASS
127	198	10	80	41.5	131274	PASS
197	198	0.00	2	1.0	3146	PASS
198	198	100	100	100.0	316480	PASS
199	198	5	9	6.6	21006	PASS
275	198	10	60	30.0	94933	PASS
365	198	1	100	5.0	15795	PASS
441	443	0.01	100	86.4	35160	PASS
442	198	50	100	69.9	221320	PASS
443	442	15	24	18.4	40717	PASS