




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035984.D
Acq On : 28 Jul 2022 14:24
Operator : CG/JU
Sample : N3850-01
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0W27

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/29/2022
Supervised By :mohammad ahmed 07/29/2022

Quant Time: Jul 29 00:49:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 27 23:55:50 2022
Response via : Initial Calibration

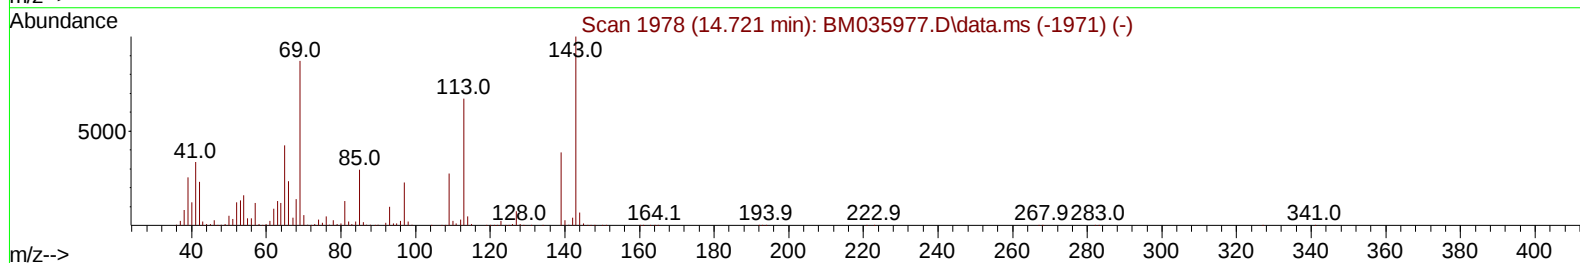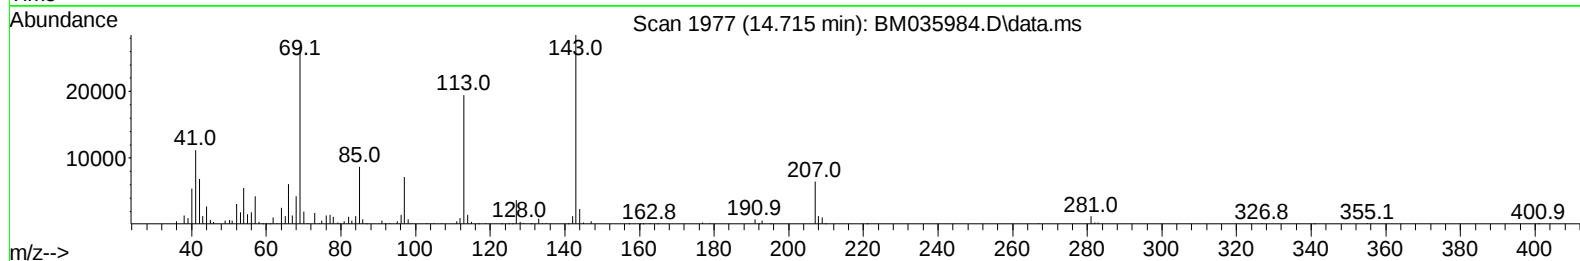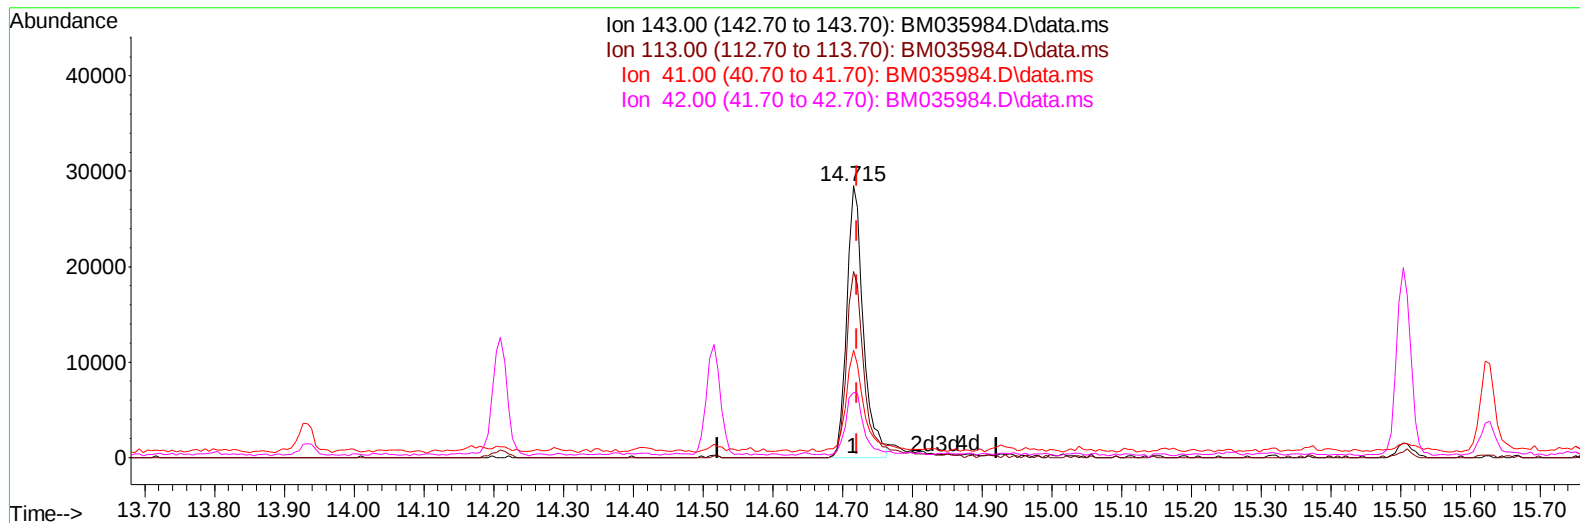

TIC: BM035984.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.715min (-0.006) 4.97 ng/u1

response 47022

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	61.40	68.49
41.00	41.00	39.49
42.00	29.30	24.01




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035984.D
Acq On : 28 Jul 2022 14:24
Operator : CG/JU
Sample : N3850-01
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COW27

Manual IntegrationsAPPROVED

Quant Time: Jul 29 00:49:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 27 23:55:50 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/29/2022
Supervised By :mohammad ahmed 07/29/2022

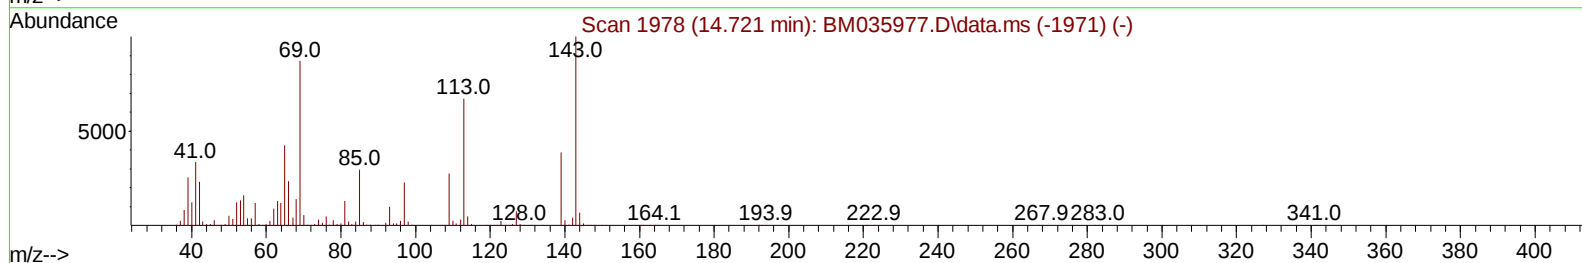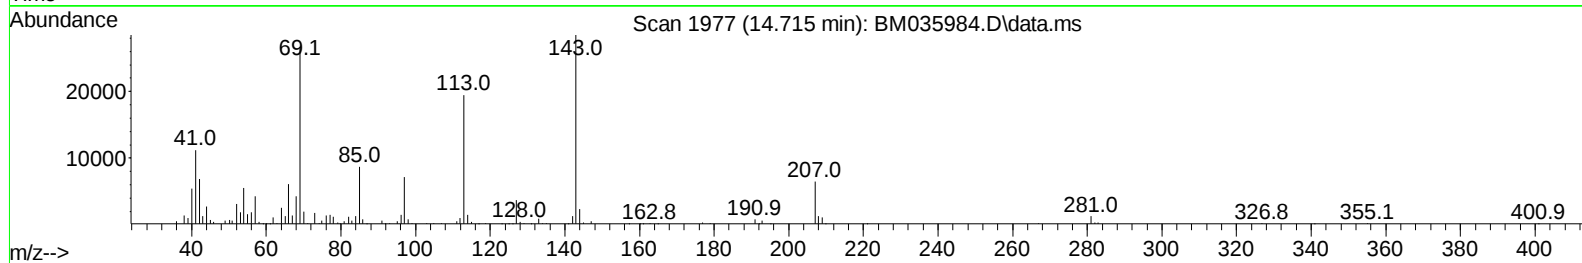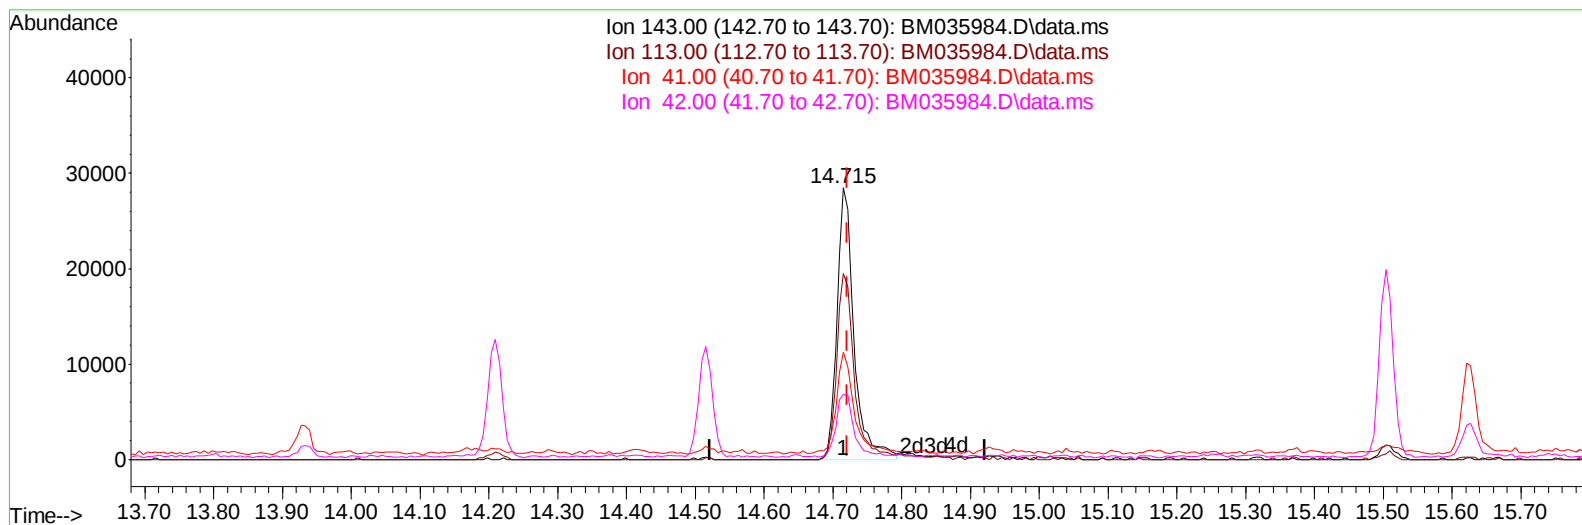

TIC: BM035984.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.715min (-0.006) 5.16 ng/ul m

response 48824

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	61.40	68.49
41.00	41.00	39.49
42.00	29.30	24.01

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
 Data File : BM035984.D
 Acq On : 28 Jul 2022 14:24
 Operator : CG/JU
 Sample : N3850-01
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COW27

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/29/2022
 Supervised By :mohammad ahmed 07/29/2022

Quant Time: Jul 29 00:49:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 27 23:55:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.881	152	294463	20.000	ng/ul	0.00
20) Naphthalene-d8	10.686	136	1212973	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.515	164	675960	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.256	188	1274083	20.000	ng/ul	0.00
79) Chrysene-d12	21.439	240	1182809	20.000	ng/ul	0.00
88) Perylene-d12	23.809	264	1213265	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	33241	4.248	ng/uL	0.00
4) Pyridine-d5	3.699	84	230081	10.732	ng/ul	0.00
7) Phenol-d5	7.045	99	164145	6.647	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.210	67	435972	26.484	ng/ul	0.00
11) 2-Chlorophenol-d4	7.410	132	474171	23.134	ng/ul	0.00
15) 4-Methylphenol-d8	8.592	113	288371	14.415	ng/ul	0.00
21) Nitrobenzene-d5	9.045	128	290783	30.253	ng/ul	0.00
24) 2-Nitrophenol-d4	9.769	143	279841	29.883	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.304	165	455749	26.909	ng/ul	0.00
31) 4-Chloroaniline-d4	10.827	131	677176	23.618	ng/ul	0.00
46) Dimethylphthalate-d6	13.933	166	1472823	31.987	ng/ul	0.00
49) Acenaphthylene-d8	14.210	160	1853178	31.544	ng/ul	0.00
54) 4-Nitrophenol-d4	14.715	143	48824m	5.164	ng/ul	0.00
60) Fluorene-d10	15.504	176	1308712	31.453	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.627	200	162732	23.761	ng/ul	0.00
73) Anthracene-d10	17.356	188	2074635	36.017	ng/ul	0.00
81) Pyrene-d10	19.645	212	2327997	35.513	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.656	264	2255011	36.610	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035984.D
Acq On : 28 Jul 2022 14:24
Operator : CG/JU
Sample : N3850-01
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COW27

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/29/2022
Supervised By :mohammad ahmed 07/29/2022

Quant Time: Jul 29 00:49:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 27 23:55:50 2022
Response via : Initial Calibration

