

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
 Data File : BM035975.D
 Acq On : 28 Jul 2022 06:31
 Operator : CG/JU
 Sample : N3741-04
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0B13

Quant Time: Jul 28 07:09:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 27 23:55:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.881	152	354417	20.000	ng/ul	0.00
20) Naphthalene-d8	10.686	136	1455873	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.515	164	815447	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.256	188	1526130	20.000	ng/ul	0.00
79) Chrysene-d12	21.433	240	1330599	20.000	ng/ul	0.00
88) Perylene-d12	23.803	264	1380814	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	42928	4.558	ng/uL	0.00
4) Pyridine-d5	3.699	84	205907	7.980	ng/ul	0.00
7) Phenol-d5	7.045	99	845852	28.460	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.216	67	478364	24.143	ng/ul	0.00
11) 2-Chlorophenol-d4	7.410	132	694302	28.143	ng/ul	0.00
15) 4-Methylphenol-d8	8.592	113	649690	26.983	ng/ul	0.00
21) Nitrobenzene-d5	9.051	128	321011	27.826	ng/ul	0.00
24) 2-Nitrophenol-d4	9.769	143	356616	31.728	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.310	165	627222	30.855	ng/ul	0.00
31) 4-Chloroaniline-d4	10.828	131	893045	25.950	ng/ul	0.00
46) Dimethylphthalate-d6	13.933	166	2126475	38.283	ng/ul	0.00
49) Acenaphthylene-d8	14.216	160	2374710	33.507	ng/ul	0.00
54) 4-Nitrophenol-d4	14.721	143	278487	24.415	ng/ul	0.00
60) Fluorene-d10	15.510	176	1773244	35.328	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.627	200	188712	23.004	ng/ul	0.00
73) Anthracene-d10	17.356	188	2660124	38.554	ng/ul	0.00
81) Pyrene-d10	19.645	212	2982815	40.448	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.650	264	2879060	41.069	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.350	149	55832	1.170	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035975.D
Acq On : 28 Jul 2022 06:31
Operator : CG/JU
Sample : N3741-04
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0B13

Quant Time: Jul 28 07:09:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 27 23:55:50 2022
Response via : Initial Calibration

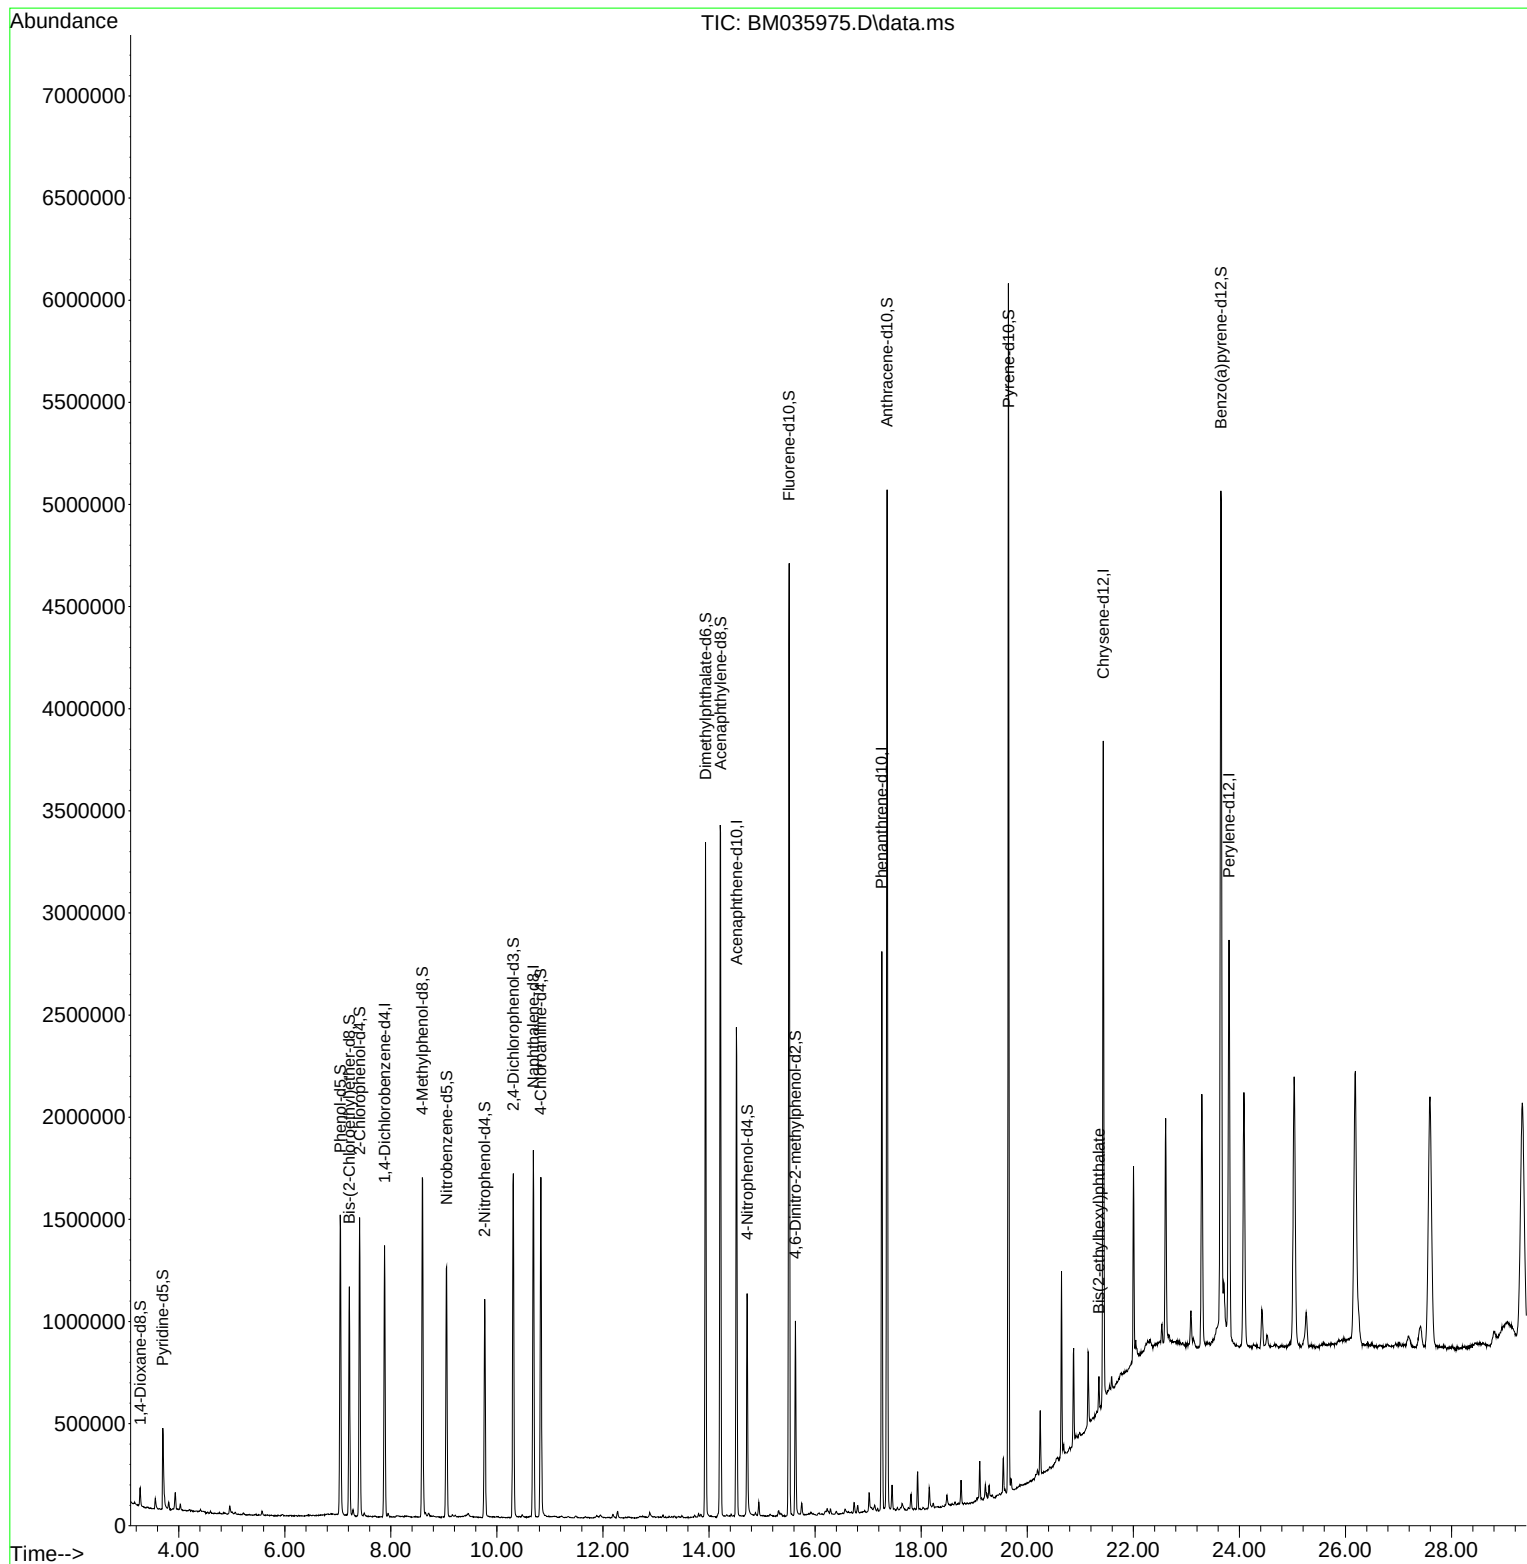

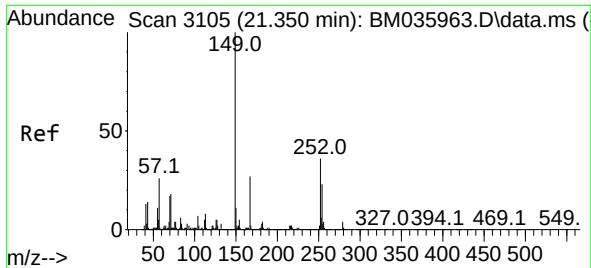

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.170 ng/ul
 RT: 21.350 min Scan# 3105
 Delta R.T. 0.000 min
 Lab File: BM035975.D
 Acq: 28 Jul 2022 06:31

Instrument :
 BNA_M
 ClientSampleId :
 H0B13

Tgt Ion:	149	Resp:	55832
Ion Ratio	Lower	Upper	
149	100		
167	29.1	21.5	32.3
279	4.6	3.4	5.2

