

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
 Data File : BM035947.D
 Acq On : 27 Jul 2022 12:54
 Operator : CG/JU
 Sample : PB146484BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK484

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035947.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	39	rVB	107593	141380	2.31%	0.191%
2	3.698	100	104	122	rBV	1184104	1676571	27.35%	2.270%
3	4.034	157	161	165	rVB	27240	39742	0.65%	0.054%
4	4.692	269	273	278	rBV8	6632	13107	0.21%	0.018%
5	6.487	574	578	579	rBV4	5577	7451	0.12%	0.010%
6	6.786	627	629	634	rBV6	5361	7805	0.13%	0.011%
7	7.057	665	675	684	rBV	1256326	1994525	32.53%	2.700%
8	7.222	697	703	712	rVB	1063255	1656947	27.03%	2.243%
9	7.422	729	737	749	rBV	1382946	2133822	34.81%	2.889%
10	7.892	808	817	826	rBV	1165058	1797359	29.32%	2.433%
11	8.257	877	879	885	rBV7	6049	9776	0.16%	0.013%
12	8.610	931	939	950	rBV	1547871	2521369	41.13%	3.413%
13	8.804	970	972	976	rVB5	6976	8061	0.13%	0.011%
14	9.063	1008	1016	1024	rBV	1214169	2005574	32.71%	2.715%
15	9.780	1131	1138	1145	rBV	971162	1632104	26.62%	2.210%
16	10.322	1223	1230	1242	rBV	1500751	2451076	39.98%	3.318%
17	10.527	1263	1265	1269	rVB5	5537	6822	0.11%	0.009%
18	10.698	1286	1294	1302	rBV	1599699	2616295	42.68%	3.542%
19	10.839	1310	1318	1329	rBV	1578746	2674293	43.62%	3.620%
20	11.057	1354	1355	1359	rVB4	5779	6918	0.11%	0.009%
21	11.116	1363	1365	1368	rVV4	5813	6326	0.10%	0.009%
22	11.886	1489	1496	1501	rBV6	13526	32655	0.53%	0.044%
23	12.286	1559	1564	1573	rVB2	33361	58176	0.95%	0.079%
24	12.710	1631	1636	1637	rBV5	5674	7160	0.12%	0.010%
25	12.757	1639	1644	1649	rVV5	13768	25185	0.41%	0.034%
26	12.892	1659	1667	1671	rVV2	26004	56008	0.91%	0.076%
27	12.968	1677	1680	1686	rVB7	10119	19417	0.32%	0.026%
28	13.268	1727	1731	1735	rVB7	7485	12312	0.20%	0.017%
29	13.321	1735	1740	1742	rBV6	8602	10430	0.17%	0.014%
30	13.504	1769	1771	1775	rVB5	9244	11802	0.19%	0.016%
31	13.668	1796	1799	1802	rBV5	5174	7717	0.13%	0.010%
32	13.810	1817	1823	1828	rBV2	20738	42201	0.69%	0.057%
33	13.945	1839	1846	1857	rVB	2665662	3524934	57.50%	4.772%
34	14.227	1881	1894	1904	rBV	3101552	4557906	74.35%	6.170%
35	14.421	1924	1927	1932	rBV7	5899	9368	0.15%	0.013%
36	14.533	1938	1946	1953	rBV	2276642	3390411	55.30%	4.590%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
 Data File : BM035947.D
 Acq On : 27 Jul 2022 12:54
 Operator : CG/JU
 Sample : PB146484BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK484

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	14.633	1961	1963	1969	rVB7	8167	11085	0.18%	0.015%
38	14.733	1973	1980	1994	rBV	1128190	1738053	28.35%	2.353%
39	14.892	2004	2007	2010	rVB5	7207	9401	0.15%	0.013%
40	14.945	2014	2016	2020	rVB5	7182	8007	0.13%	0.011%
41	15.145	2047	2050	2052	rBV3	6513	6964	0.11%	0.009%
42	15.309	2073	2078	2082	rBV2	23762	41912	0.68%	0.057%
43	15.345	2082	2084	2088	rVB2	11799	15692	0.26%	0.021%
44	15.521	2105	2114	2124	rBV	3894937	5382750	87.80%	7.287%
45	15.651	2130	2136	2149	rBV	1105577	1536043	25.06%	2.079%
46	15.756	2150	2154	2161	rVB2	50729	80022	1.31%	0.108%
47	15.833	2166	2167	2172	rVV5	7074	9926	0.16%	0.013%
48	15.892	2172	2177	2180	rVV7	10706	19208	0.31%	0.026%
49	15.927	2180	2183	2188	rVV4	17211	29764	0.49%	0.040%
50	15.986	2188	2193	2197	rVB8	5907	12324	0.20%	0.017%
51	16.080	2206	2209	2211	rBV4	5459	6475	0.11%	0.009%
52	16.180	2221	2226	2231	rBV7	16394	39330	0.64%	0.053%
53	16.233	2233	2235	2242	rVV4	23490	43853	0.72%	0.059%
54	16.304	2243	2247	2251	rVB4	14348	22000	0.36%	0.030%
55	16.409	2260	2265	2271	rVB6	10051	16989	0.28%	0.023%
56	16.574	2288	2293	2296	rBV6	29425	53362	0.87%	0.072%
57	16.639	2302	2304	2309	rVB5	13293	13821	0.23%	0.019%
58	16.692	2310	2313	2316	rBV5	11014	12653	0.21%	0.017%
59	16.745	2317	2322	2327	rVV	70409	98447	1.61%	0.133%
60	16.809	2330	2333	2336	rBV4	14003	17190	0.28%	0.023%
61	17.027	2366	2370	2373	rBV	43357	59081	0.96%	0.080%
62	17.056	2373	2375	2376	rVV2	13001	8985	0.15%	0.012%
63	17.192	2395	2398	2401	rVB5	13075	16124	0.26%	0.022%
64	17.274	2405	2412	2418	rBV	2582646	3659536	59.69%	4.954%
65	17.368	2419	2428	2440	rVB	3855803	5702708	93.02%	7.720%
66	17.498	2448	2450	2457	rVB7	10066	12865	0.21%	0.017%
67	17.562	2457	2461	2464	rBV3	14677	23777	0.39%	0.032%
68	17.815	2500	2504	2512	rVB2	49061	75659	1.23%	0.102%
69	18.168	2560	2564	2567	rBV6	17725	24363	0.40%	0.033%
70	18.762	2661	2665	2670	rBV2	44376	61607	1.00%	0.083%
71	19.227	2740	2744	2747	rBV	51826	71593	1.17%	0.097%
72	19.297	2753	2756	2761	rBV	44296	62345	1.02%	0.084%
73	19.662	2812	2818	2824	rBV	4753404	6130594	100.00%	8.300%
74	20.656	2984	2987	2991	rBV	228562	264913	4.32%	0.359%
75	21.450	3118	3122	3129	rBV	2944781	3539793	57.74%	4.792%
76	23.685	3495	3502	3509	rBV2	3146438	6055855	98.78%	8.198%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035947.D
Acq On : 27 Jul 2022 12:54
Operator : CG/JU
Sample : PB146484BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK484

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Title : SVOA CALIBRATION

77 23.838 3522 3528 3537 rVB2 1905107 3698605 60.33% 5.007%


Sum of corrected areas: 73866679

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035947.D
Acq On : 27 Jul 2022 12:54
Operator : CG/JU
Sample : PB146484BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK484

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

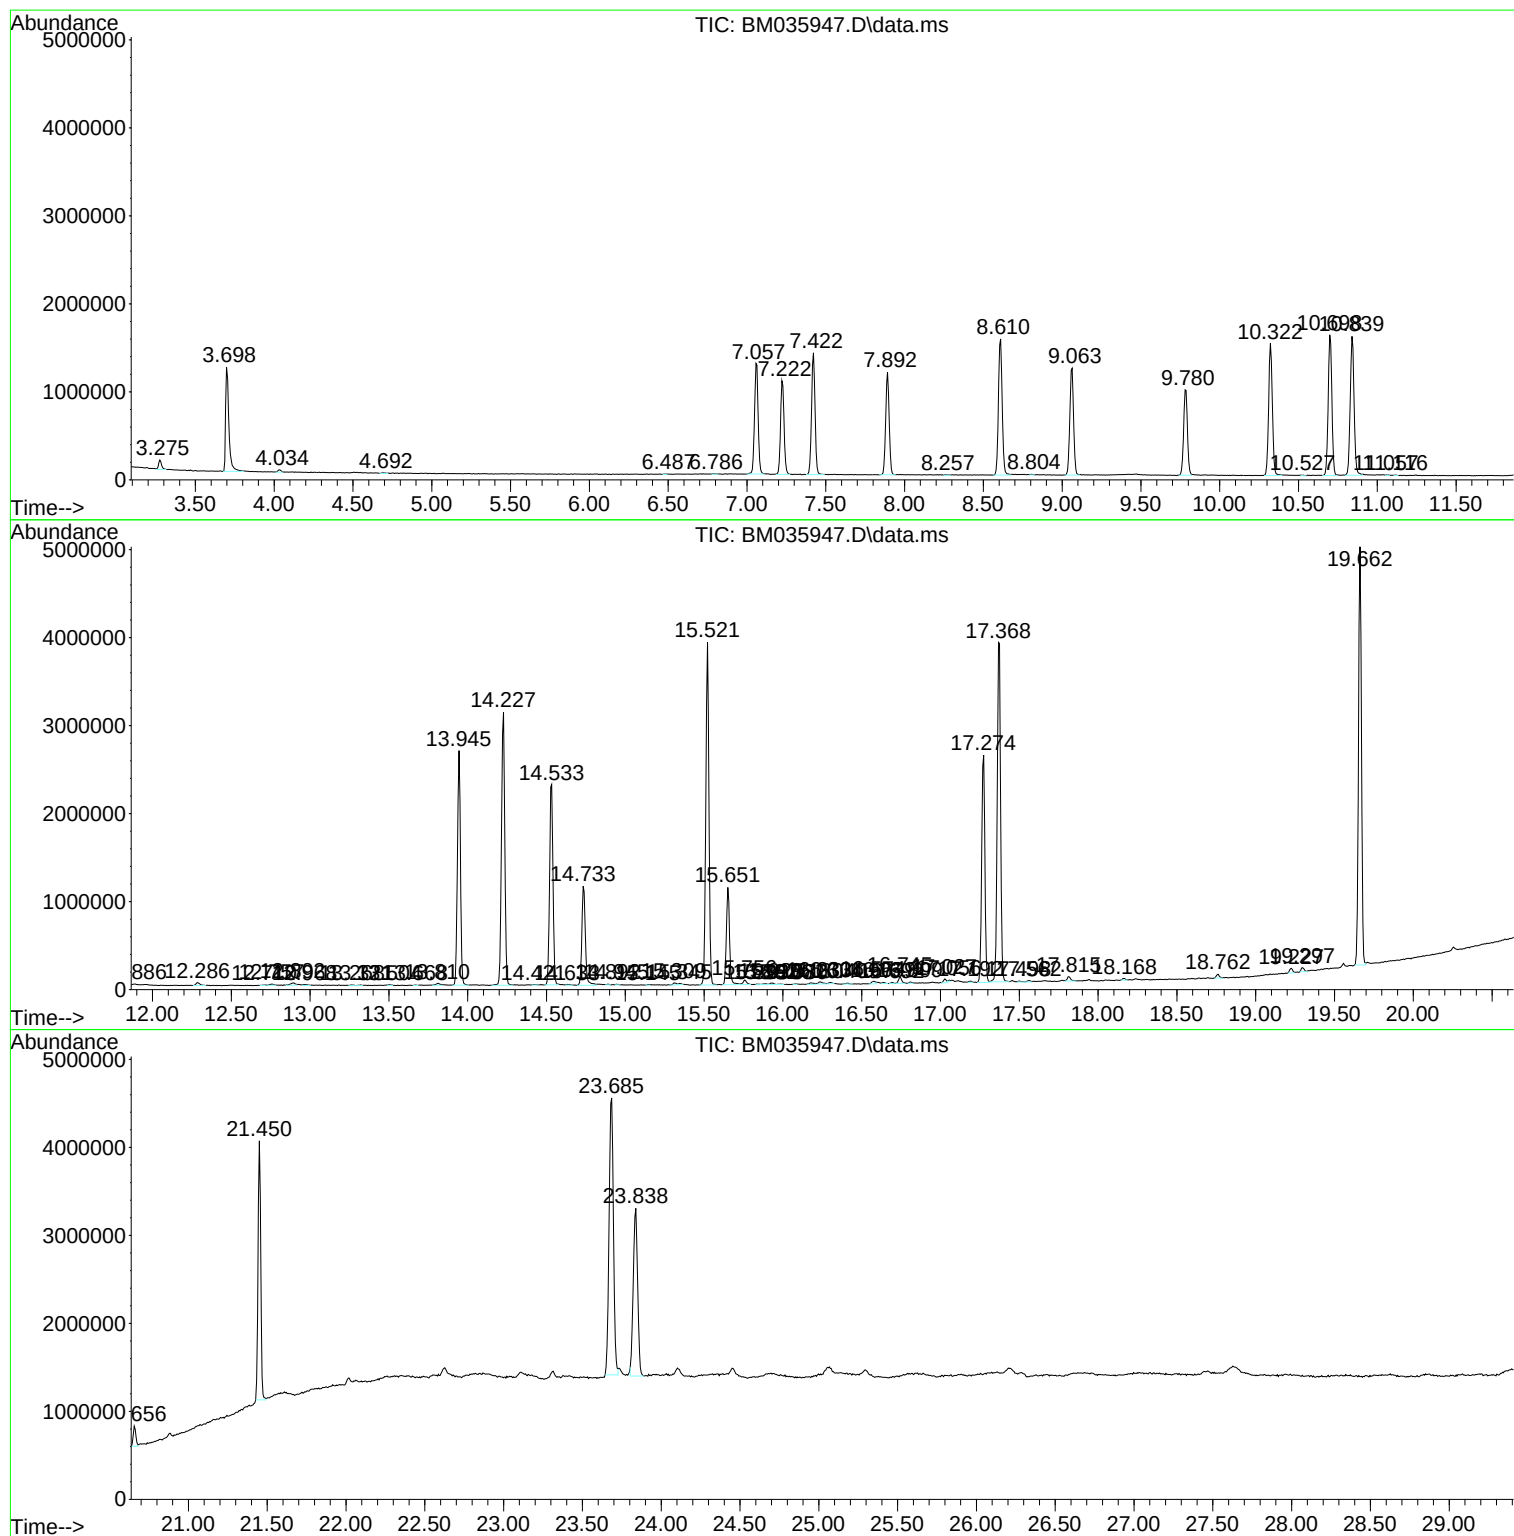

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035947.D
Acq On : 27 Jul 2022 12:54
Operator : CG/JU
Sample : PB146484BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK484

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035947.D
Acq On : 27 Jul 2022 12:54
Operator : CG/JU
Sample : PB146484BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK484

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc