

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
 Data File : BM035948.D
 Acq On : 27 Jul 2022 13:31
 Operator : CG/JU
 Sample : PB146378BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK378

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035948.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	29	32	42	rVB	120601	162189	2.34%	0.201%
2	3.699	101	104	123	rBV	1332308	1911593	27.59%	2.374%
3	4.034	158	161	168	rVB	28604	43588	0.63%	0.054%
4	5.546	416	418	420	rBV3	8835	8722	0.13%	0.011%
5	7.057	664	675	692	rBV	1436379	2321140	33.50%	2.883%
6	7.222	697	703	712	rVB	1237543	1880770	27.15%	2.336%
7	7.422	730	737	745	rBV	1554400	2449308	35.35%	3.042%
8	7.893	810	817	825	rVB	1200223	1834831	26.49%	2.279%
9	8.604	931	938	951	rBV	1751087	2847159	41.10%	3.536%
10	9.063	1008	1016	1026	rBV	1349810	2239298	32.32%	2.781%
11	9.469	1084	1085	1097	rVB	13363	28255	0.41%	0.035%
12	9.681	1118	1121	1125	rBV6	6569	7981	0.12%	0.010%
13	9.781	1130	1138	1148	rBV	1127975	1850821	26.72%	2.298%
14	10.016	1177	1178	1181	rBV3	8079	6996	0.10%	0.009%
15	10.322	1221	1230	1243	rBV	1688291	2797072	40.37%	3.474%
16	10.698	1286	1294	1301	rBV	1624342	2629230	37.95%	3.265%
17	10.839	1310	1318	1332	rBV	1729552	2950173	42.58%	3.664%
18	11.875	1490	1494	1495	rBV4	9071	8017	0.12%	0.010%
19	11.892	1495	1497	1501	rVB5	8430	9367	0.14%	0.012%
20	12.286	1559	1564	1573	rVB	34985	65841	0.95%	0.082%
21	12.498	1597	1600	1604	rVB6	5689	7885	0.11%	0.010%
22	12.757	1637	1644	1653	rVB5	12748	30282	0.44%	0.038%
23	12.886	1660	1666	1672	rBV2	23334	50648	0.73%	0.063%
24	13.075	1696	1698	1701	rBV4	5954	7384	0.11%	0.009%
25	13.257	1727	1729	1732	rBV4	6599	8723	0.13%	0.011%
26	13.810	1818	1823	1829	rBV4	21746	47586	0.69%	0.059%
27	13.945	1839	1846	1855	rBV	2863684	3853667	55.63%	4.786%
28	14.227	1880	1894	1903	rBV	3303791	4999721	72.17%	6.209%
29	14.421	1923	1927	1932	rVB8	7257	9933	0.14%	0.012%
30	14.527	1938	1945	1958	rVB	2292358	3329777	48.06%	4.135%
31	14.633	1960	1963	1972	rVB	11256	19561	0.28%	0.024%
32	14.733	1974	1980	1989	rBV	1271959	1877898	27.11%	2.332%
33	15.163	2050	2053	2060	rBV9	6336	8084	0.12%	0.010%
34	15.316	2074	2079	2081	rVV4	19552	28804	0.42%	0.036%
35	15.351	2081	2085	2088	rVB	10369	16935	0.24%	0.021%
36	15.421	2095	2097	2103	rVB7	6150	9769	0.14%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
 Data File : BM035948.D
 Acq On : 27 Jul 2022 13:31
 Operator : CG/JU
 Sample : PB146378BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK378

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	15.521	2105	2114	2124	rBV	4278943	5963826	86.09%	7.406%
38	15.651	2130	2136	2145	rBV	1247308	1692899	24.44%	2.102%
39	15.757	2150	2154	2164	rVB	54230	87282	1.26%	0.108%
40	15.886	2173	2176	2179	rBV5	7977	9826	0.14%	0.012%
41	15.927	2179	2183	2187	rVV3	14335	25685	0.37%	0.032%
42	15.974	2190	2191	2198	rVB6	7142	12698	0.18%	0.016%
43	16.086	2208	2210	2214	rVB5	8243	10118	0.15%	0.013%
44	16.127	2214	2217	2221	rBV6	4966	7466	0.11%	0.009%
45	16.174	2221	2225	2227	rBV4	17481	22107	0.32%	0.027%
46	16.233	2232	2235	2242	rVV3	28424	55750	0.80%	0.069%
47	16.304	2243	2247	2253	rVB4	20695	32812	0.47%	0.041%
48	16.410	2262	2265	2268	rVB5	9829	12166	0.18%	0.015%
49	16.580	2288	2294	2297	rBV5	25524	52984	0.76%	0.066%
50	16.639	2301	2304	2309	rVB7	12838	19177	0.28%	0.024%
51	16.692	2311	2313	2317	rVV5	11513	12998	0.19%	0.016%
52	16.745	2317	2322	2328	rVV2	70911	100012	1.44%	0.124%
53	16.810	2330	2333	2337	rVB2	15467	17804	0.26%	0.022%
54	16.886	2342	2346	2348	rBV4	7445	10826	0.16%	0.013%
55	16.951	2353	2357	2362	rVB8	8974	14340	0.21%	0.018%
56	17.027	2366	2370	2373	rBV2	41710	58022	0.84%	0.072%
57	17.104	2381	2383	2390	rVB8	15823	27303	0.39%	0.034%
58	17.192	2395	2398	2402	rVB6	13286	17123	0.25%	0.021%
59	17.268	2405	2411	2419	rBV	2555979	3662542	52.87%	4.548%
60	17.368	2419	2428	2438	rVV2	4351440	6248027	90.19%	7.759%
61	17.457	2441	2443	2446	rVB4	13333	12866	0.19%	0.016%
62	17.562	2459	2461	2465	rVB4	11177	13256	0.19%	0.016%
63	17.762	2493	2495	2499	rBV5	9988	12215	0.18%	0.015%
64	17.815	2500	2504	2509	rVB2	49602	70971	1.02%	0.088%
65	18.168	2559	2564	2567	rBV6	16127	26336	0.38%	0.033%
66	18.757	2660	2664	2669	rBV2	46504	69880	1.01%	0.087%
67	19.227	2740	2744	2748	rBV	54371	76403	1.10%	0.095%
68	19.298	2752	2756	2759	rBV	55374	76743	1.11%	0.095%
69	19.662	2812	2818	2823	rBV	5255434	6927803	100.00%	8.603%
70	20.656	2984	2987	2991	rBV	253870	260368	3.76%	0.323%
71	21.445	3117	3121	3127	rBV	2868062	3749852	54.13%	4.657%
72	23.680	3494	3501	3507	rBV2	3563423	6825076	98.52%	8.476%
73	23.833	3521	3527	3535	rVB2	1906904	3869936	55.86%	4.806%



Sum of corrected areas: 80524506

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035948.D
Acq On : 27 Jul 2022 13:31
Operator : CG/JU
Sample : PB146378BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK378

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

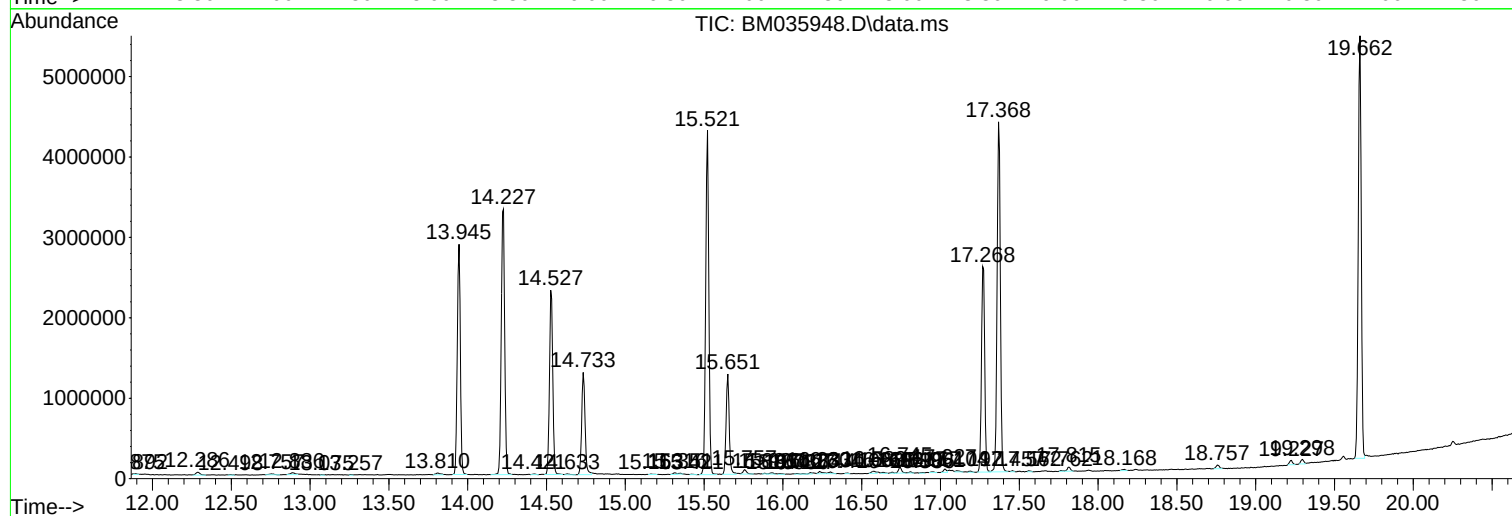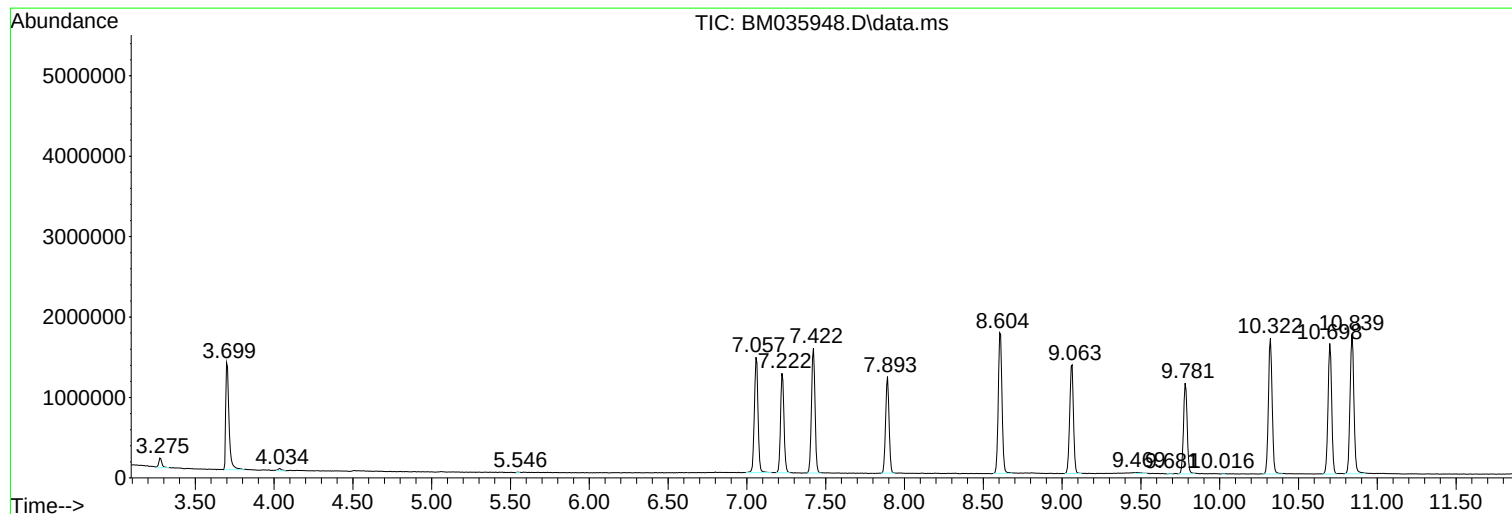

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035948.D
Acq On : 27 Jul 2022 13:31
Operator : CG/JU
Sample : PB146378BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK378

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035948.D
Acq On : 27 Jul 2022 13:31
Operator : CG/JU
Sample : PB146378BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK378

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc