

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
 Data File : BM035955.D
 Acq On : 27 Jul 2022 17:48
 Operator : CG/JU
 Sample : N3874-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBJ27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035955.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	35	rBV	87262	105763	1.55%	0.157%
2	3.310	35	38	49	rVB	277625	348312	5.10%	0.516%
3	3.563	78	81	89	rVB	32282	45367	0.66%	0.067%
4	3.704	101	105	116	rBV	464876	697067	10.21%	1.034%
5	3.934	140	144	151	rVB2	58735	95336	1.40%	0.141%
6	3.987	151	153	156	rVV4	7118	8636	0.13%	0.013%
7	4.034	158	161	165	rVB	23743	31313	0.46%	0.046%
8	4.969	316	320	325	rVB6	7462	13036	0.19%	0.019%
9	5.010	325	327	333	rBV6	7898	9575	0.14%	0.014%
10	5.957	486	488	492	rVB3	9077	10744	0.16%	0.016%
11	6.787	625	629	631	rBV5	5466	7773	0.11%	0.012%
12	6.887	641	646	653	rBV2	15458	26429	0.39%	0.039%
13	7.051	668	674	681	rVB	381648	593994	8.70%	0.881%
14	7.222	696	703	712	rBV	1059475	1619388	23.72%	2.401%
15	7.292	712	715	720	rVB	11958	15826	0.23%	0.023%
16	7.416	727	736	745	rBV	1092068	1703212	24.95%	2.525%
17	7.498	748	750	756	rVB7	7290	11205	0.16%	0.017%
18	7.886	809	816	824	rBV	964143	1478076	21.65%	2.192%
19	7.951	824	827	834	rVB3	15005	25056	0.37%	0.037%
20	8.604	931	938	951	rBV	898857	1467701	21.50%	2.176%
21	8.998	998	1005	1008	rBV	38751	61682	0.90%	0.091%
22	9.057	1008	1015	1027	rVV	1216311	1968058	28.83%	2.918%
23	9.175	1029	1035	1038	rVV8	9959	14837	0.22%	0.022%
24	9.463	1081	1084	1092	rVB9	11674	22621	0.33%	0.034%
25	9.775	1130	1137	1150	rBV	898537	1549558	22.70%	2.298%
26	10.316	1221	1229	1239	rBV	1373021	2265362	33.18%	3.359%
27	10.486	1253	1258	1263	rBV3	14970	29110	0.43%	0.043%
28	10.692	1286	1293	1301	rBV	1245103	2079177	30.46%	3.083%
29	10.833	1310	1317	1336	rBV	1228931	2148440	31.47%	3.185%
30	11.516	1432	1433	1441	rVB8	6126	8049	0.12%	0.012%
31	11.886	1489	1496	1501	rBV10	10473	27605	0.40%	0.041%
32	11.957	1503	1508	1512	rVB8	11106	20558	0.30%	0.030%
33	12.280	1558	1563	1568	rVB2	30487	46198	0.68%	0.068%
34	12.486	1593	1598	1603	rBV8	5680	11625	0.17%	0.017%
35	12.757	1636	1644	1649	rVB8	8466	19861	0.29%	0.029%
36	12.892	1657	1667	1672	rBV	24304	54151	0.79%	0.080%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
 Data File : BM035955.D
 Acq On : 27 Jul 2022 17:48
 Operator : CG/JU
 Sample : N3874-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBJ27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	13.139	1704	1709	1714	rBV6	10410	14491	0.21%	0.021%
38	13.304	1734	1737	1742	rBV7	4755	7818	0.11%	0.012%
39	13.374	1742	1749	1754	rVV	112507	158895	2.33%	0.236%
40	13.498	1765	1770	1775	rVV9	7071	13388	0.20%	0.020%
41	13.815	1819	1824	1826	rBV5	13524	21738	0.32%	0.032%
42	13.851	1826	1830	1837	rVB2	28088	46721	0.68%	0.069%
43	13.939	1839	1845	1857	rBV	2696365	3680359	53.91%	5.457%
44	14.221	1886	1893	1902	rVB	3080683	4434189	64.96%	6.575%
45	14.286	1902	1904	1913	rVB10	12392	25405	0.37%	0.038%
46	14.427	1925	1928	1930	rVB4	6133	7062	0.10%	0.010%
47	14.527	1938	1945	1950	rBV	1847183	2659307	38.96%	3.943%
48	14.568	1950	1952	1956	rVB	49018	54346	0.80%	0.081%
49	14.727	1973	1979	1995	rBV2	337125	606028	8.88%	0.899%
50	14.892	2003	2007	2010	rVB6	7858	10291	0.15%	0.015%
51	14.945	2012	2016	2020	rVB7	8367	15326	0.22%	0.023%
52	15.162	2050	2053	2058	rVB7	6548	12338	0.18%	0.018%
53	15.268	2065	2071	2074	rBV	13383	19148	0.28%	0.028%
54	15.321	2075	2080	2082	rVV2	58684	85578	1.25%	0.127%
55	15.345	2082	2084	2092	rVB	55382	72962	1.07%	0.108%
56	15.515	2106	2113	2119	rBV	3966432	5605135	82.11%	8.311%
57	15.639	2128	2134	2145	rBV	1187622	1618088	23.70%	2.399%
58	15.751	2148	2153	2162	rVV2	50710	90028	1.32%	0.133%
59	15.839	2162	2168	2169	rVV6	6479	11706	0.17%	0.017%
60	15.886	2172	2176	2179	rVV6	8386	14019	0.21%	0.021%
61	15.933	2179	2184	2188	rVV5	12731	22103	0.32%	0.033%
62	15.992	2190	2194	2197	rVB4	13967	18037	0.26%	0.027%
63	16.068	2203	2207	2209	rBV5	9344	15201	0.22%	0.023%
64	16.192	2221	2228	2231	rBV9	11753	23357	0.34%	0.035%
65	16.233	2231	2235	2237	rBV3	20746	23621	0.35%	0.035%
66	16.298	2242	2246	2250	rVB6	18769	27729	0.41%	0.041%
67	16.409	2259	2265	2269	rBV6	11056	20969	0.31%	0.031%
68	16.515	2279	2283	2285	rBV5	6418	8657	0.13%	0.013%
69	16.574	2288	2293	2297	rBV5	25599	46665	0.68%	0.069%
70	16.745	2316	2322	2328	rBV	53966	83822	1.23%	0.124%
71	16.804	2330	2332	2337	rVB4	9386	10359	0.15%	0.015%
72	16.939	2353	2355	2359	rVB5	8572	9636	0.14%	0.014%
73	17.027	2366	2370	2373	rBV	78613	102893	1.51%	0.153%
74	17.186	2394	2397	2401	rVB5	15951	20987	0.31%	0.031%
75	17.268	2404	2411	2419	rVV	2058194	2928416	42.90%	4.342%
76	17.362	2419	2427	2437	rVV	4224898	6149929	90.09%	9.118%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
 Data File : BM035955.D
 Acq On : 27 Jul 2022 17:48
 Operator : CG/JU
 Sample : N3874-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBJ27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

77	17.456	2440	2443	2447	rVB6	16454	23259	0.34%	0.034%
78	17.556	2456	2460	2465	rBV2	26356	38006	0.56%	0.056%
79	17.762	2492	2495	2497	rBV4	9633	12571	0.18%	0.019%
80	17.809	2500	2503	2509	rVB	45198	65792	0.96%	0.098%
81	17.939	2521	2525	2529	rVB	37711	51225	0.75%	0.076%
82	18.156	2559	2562	2569	rBV4	43109	58765	0.86%	0.087%
83	18.233	2572	2575	2580	rVB	62463	78870	1.16%	0.117%
84	18.756	2661	2664	2667	rBV2	35695	42716	0.63%	0.063%
85	19.215	2739	2742	2749	rVB3	52799	74608	1.09%	0.111%
86	19.292	2751	2755	2760	rVV	50236	70005	1.03%	0.104%
87	19.656	2811	2817	2822	rBV	5101761	6826526	100.00%	10.122%
88	20.650	2983	2986	2990	rBV	203372	215092	3.15%	0.319%
89	21.156	3069	3072	3077	rBV	264848	314474	4.61%	0.466%
90	21.439	3116	3120	3126	rBV	2294955	2949517	43.21%	4.373%
91	23.668	3493	3499	3506	rVB2	3232067	6187385	90.64%	9.174%
92	23.821	3519	3525	3534	rVB2	1493626	2998409	43.92%	4.446%




Sum of corrected areas: 67444668

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035955.D
Acq On : 27 Jul 2022 17:48
Operator : CG/JU
Sample : N3874-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBJ27

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

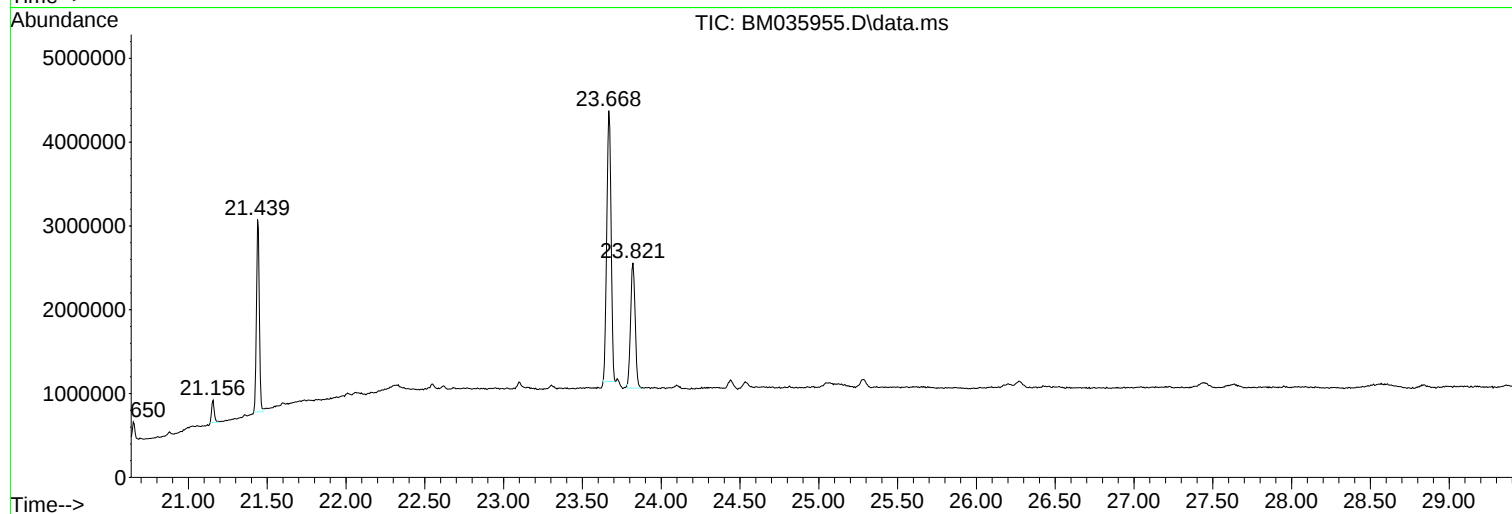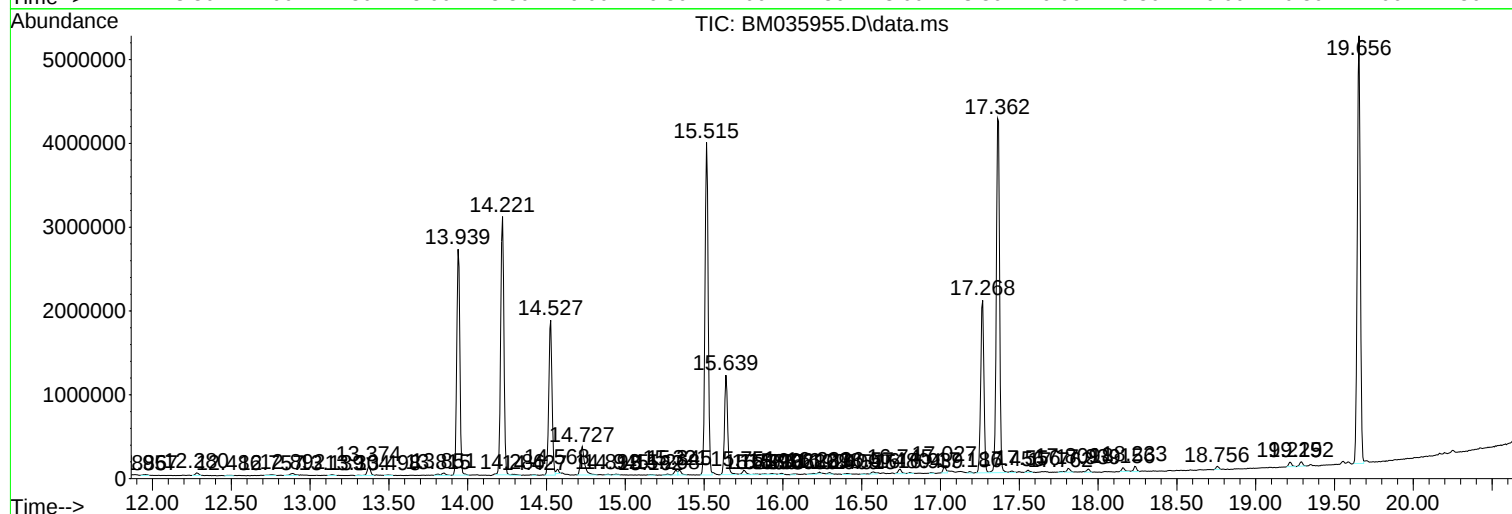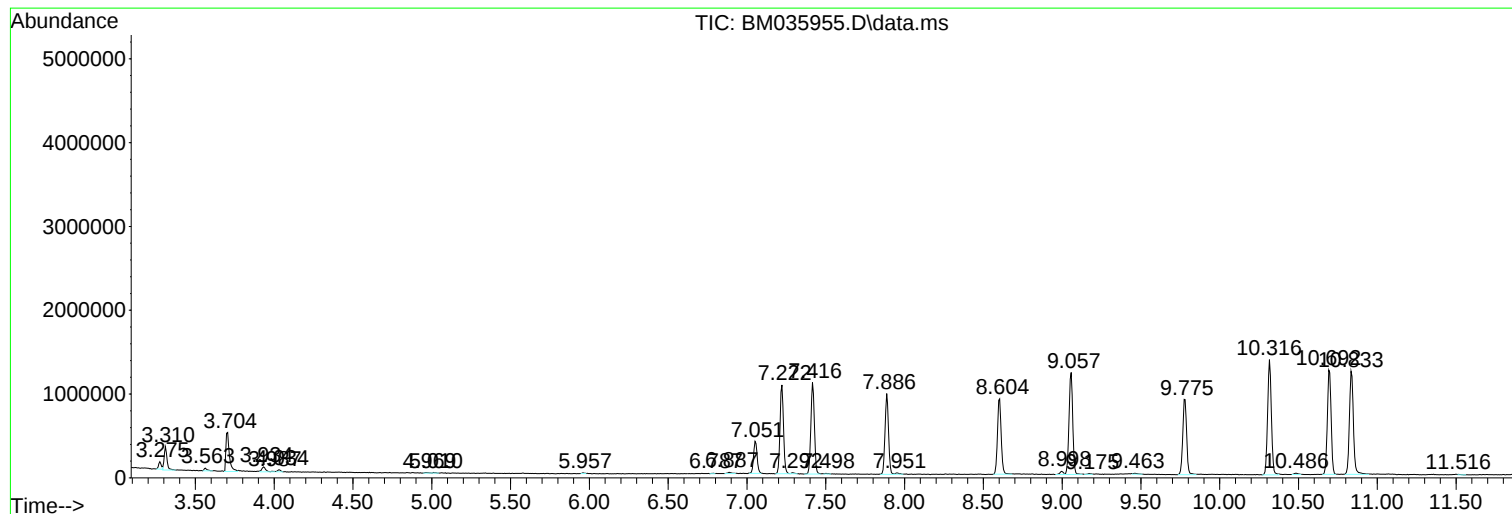

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035955.D
Acq On : 27 Jul 2022 17:48
Operator : CG/JU
Sample : N3874-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBJ27










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Trifluoroacetic acid, penta... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.156	2.13 ng/ul	314474	Chrysene-d12	21.439

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Trifluoroacetic acid, pentadecyl...	324	C17H31F3O2	959010-23-2	94
2			Pentafluoropropionic acid, penta...	374	C18H31F5O2	959092-08-1	94
3			Heptafluorobutyric acid, n-tetra...	410	C18H29F7O2	007365-36-8	94
4			Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	94
5			Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	94

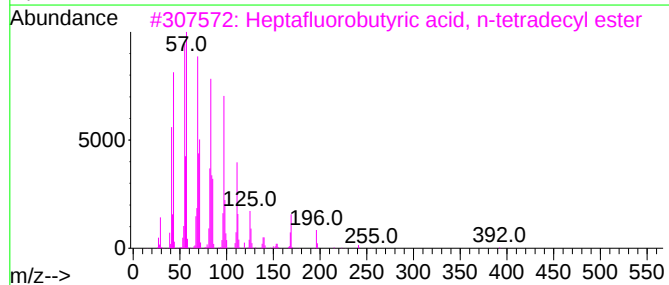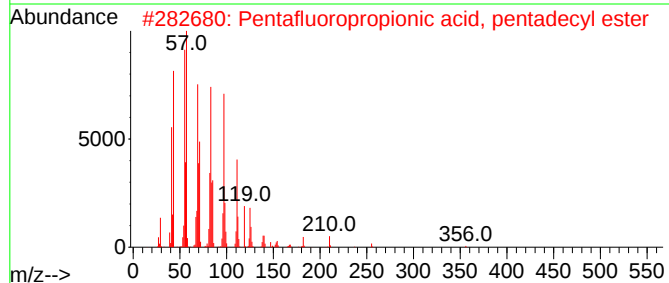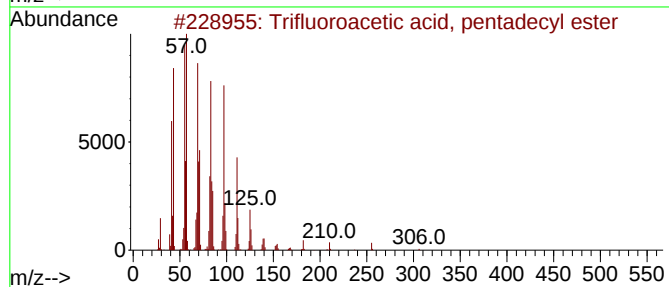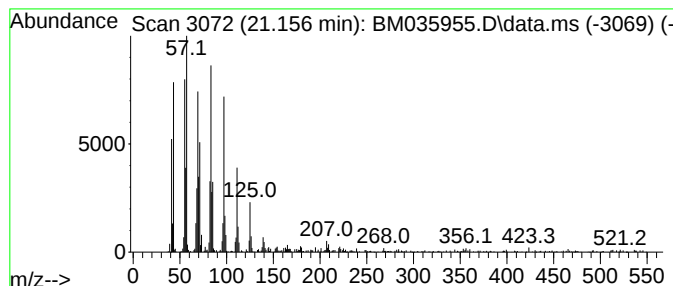

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035955.D
Acq On : 27 Jul 2022 17:48
Operator : CG/JU
Sample : N3874-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBJ27

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Trifluoroacetic...	21.156	2.1	ng/ul	314474	5	21.439	2949520	20.0