

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
 Data File : BM035964.D
 Acq On : 27 Jul 2022 23:54
 Operator : CG/JU
 Sample : PB146378BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK378

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035964.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	42	rVB	124110	161138	2.09%	0.184%
2	3.693	100	103	124	rBV	1433928	2059702	26.65%	2.352%
3	4.028	156	160	164	rBV	25629	34457	0.45%	0.039%
4	7.051	665	674	685	rBV	1577221	2485677	32.16%	2.838%
5	7.216	695	702	714	rVB	1344105	2049549	26.52%	2.340%
6	7.410	727	735	747	rBV	1700084	2641757	34.18%	3.016%
7	7.881	807	815	826	rBV	1266199	1995457	25.82%	2.278%
8	8.598	929	937	951	rBV	1967310	3073052	39.77%	3.509%
9	9.051	1004	1014	1026	rBV	1524162	2443845	31.62%	2.790%
10	9.457	1082	1083	1089	rVB6	10772	14380	0.19%	0.016%
11	9.775	1129	1137	1149	rBV	1164532	1962279	25.39%	2.240%
12	10.310	1219	1228	1242	rBV	1823985	3000510	38.83%	3.426%
13	10.686	1285	1292	1302	rBV	1677345	2823772	36.54%	3.224%
14	10.827	1309	1316	1329	rBV	1878597	3183866	41.20%	3.635%
15	11.880	1487	1495	1501	rBV10	9819	23985	0.31%	0.027%
16	11.957	1501	1508	1516	rVB8	8424	26185	0.34%	0.030%
17	12.274	1556	1562	1571	rBV2	36948	71982	0.93%	0.082%
18	12.880	1658	1665	1670	rBV4	16350	34986	0.45%	0.040%
19	13.492	1766	1769	1773	rVB4	7749	8074	0.10%	0.009%
20	13.804	1817	1822	1828	rBV3	12657	22443	0.29%	0.026%
21	13.933	1838	1844	1854	rBV	2983162	4111836	53.21%	4.695%
22	14.216	1885	1892	1902	rVB	3776970	5305462	68.65%	6.057%
23	14.521	1937	1944	1955	rBV	2469071	3521519	45.57%	4.021%
24	14.721	1971	1978	1995	rBV	1399223	2093695	27.09%	2.390%
25	15.310	2072	2078	2081	rBV3	15164	26441	0.34%	0.030%
26	15.333	2081	2082	2093	rVB3	12490	24002	0.31%	0.027%
27	15.510	2105	2112	2124	rBV	4591743	6343036	82.08%	7.242%
28	15.633	2126	2133	2147	rVV	1273053	1823078	23.59%	2.081%
29	15.751	2147	2153	2157	rVB	52706	80166	1.04%	0.092%
30	15.927	2179	2183	2188	rVB8	9642	14930	0.19%	0.017%
31	16.080	2204	2209	2213	rBV8	7144	10786	0.14%	0.012%
32	16.192	2221	2228	2231	rBV9	8452	17814	0.23%	0.020%
33	16.227	2231	2234	2237	rVV3	17398	24042	0.31%	0.027%
34	16.292	2241	2245	2252	rVB4	20383	32897	0.43%	0.038%
35	16.404	2262	2264	2271	rVB7	8997	7835	0.10%	0.009%
36	16.574	2287	2293	2296	rBV6	19724	39638	0.51%	0.045%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
 Data File : BM035964.D
 Acq On : 27 Jul 2022 23:54
 Operator : CG/JU
 Sample : PB146378BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK378

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	16.633	2301	2303	2308	rVV5	11732	11324	0.15%	0.013%
38	16.680	2309	2311	2316	rVV6	6518	9954	0.13%	0.011%
39	16.739	2316	2321	2326	rVV2	46091	65711	0.85%	0.075%
40	16.804	2329	2332	2337	rVB7	9580	12976	0.17%	0.015%
41	17.021	2365	2369	2371	rBV	31064	39704	0.51%	0.045%
42	17.174	2393	2395	2401	rVB6	7774	10925	0.14%	0.012%
43	17.262	2403	2410	2418	rVV	2731502	3946574	51.07%	4.506%
44	17.356	2418	2426	2438	rVV	4729905	6682701	86.47%	7.630%
45	17.756	2492	2494	2498	rBV5	7013	10699	0.14%	0.012%
46	17.809	2499	2503	2507	rVB	43773	59603	0.77%	0.068%
47	17.933	2520	2524	2527	rVB6	8107	12970	0.17%	0.015%
48	18.156	2558	2562	2565	rBV6	9536	13762	0.18%	0.016%
49	18.227	2571	2574	2578	rVB2	9998	14291	0.18%	0.016%
50	18.756	2659	2664	2672	rBV2	48462	73974	0.96%	0.084%
51	19.215	2738	2742	2746	rVB	65298	82627	1.07%	0.094%
52	19.280	2749	2753	2759	rBV	60851	96909	1.25%	0.111%
53	19.550	2795	2799	2803	rBV	58696	78257	1.01%	0.089%
54	19.650	2809	2816	2822	rBV	5773051	7728028	100.00%	8.823%
55	20.245	2914	2917	2923	rBV2	76738	108056	1.40%	0.123%
56	20.645	2981	2985	2990	rBV	333848	417483	5.40%	0.477%
57	20.874	3021	3024	3027	rBV2	88434	105295	1.36%	0.120%
58	21.433	3114	3119	3125	rBV	3427647	4419073	57.18%	5.045%
59	23.656	3490	3497	3503	rBV2	3930245	7652736	99.03%	8.737%
60	23.809	3516	3523	3533	rVB2	2216719	4339619	56.15%	4.955%



Sum of corrected areas: 87587524

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035964.D
Acq On : 27 Jul 2022 23:54
Operator : CG/JU
Sample : PB146378BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK378

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

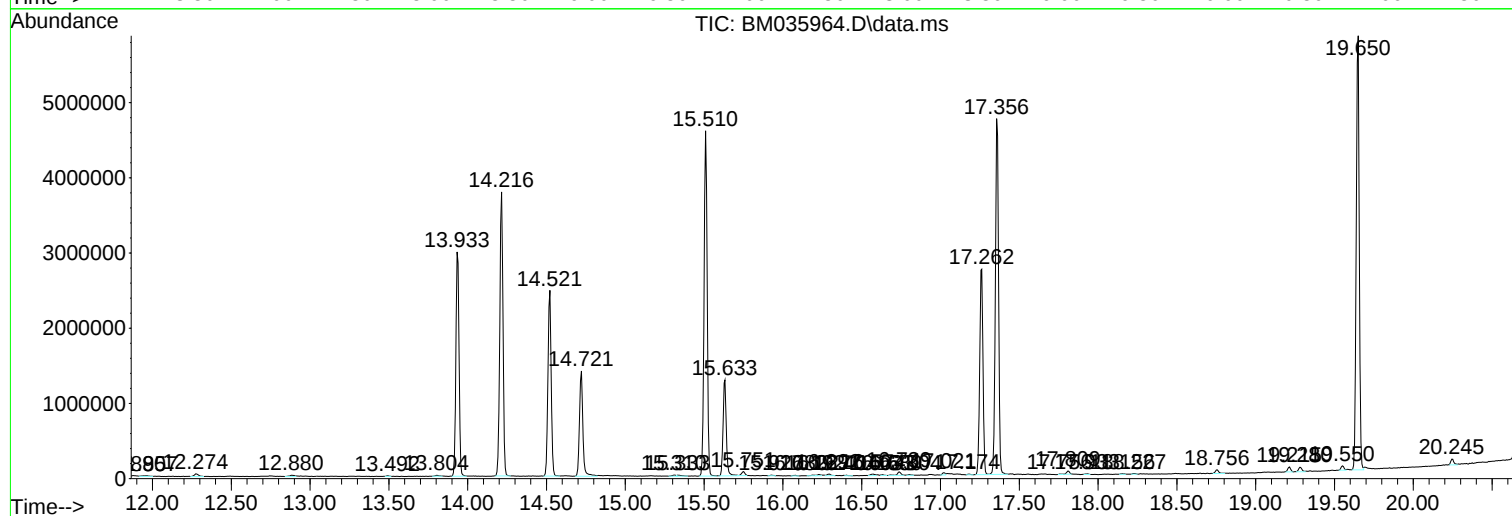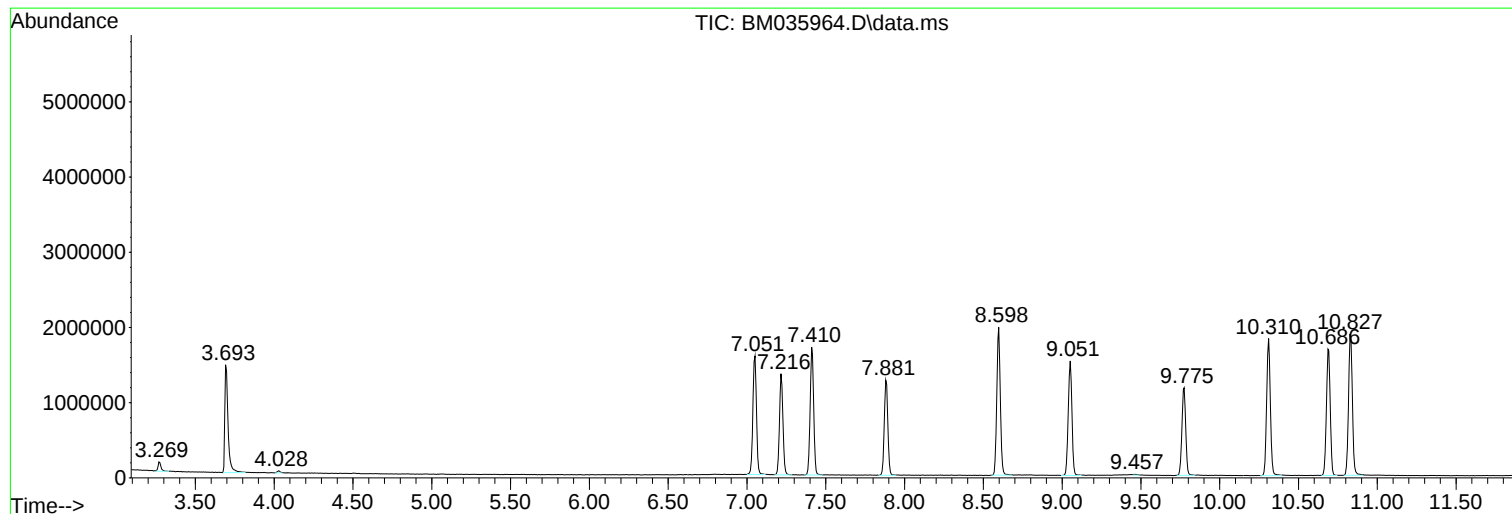

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035964.D
Acq On : 27 Jul 2022 23:54
Operator : CG/JU
Sample : PB146378BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK378

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035964.D
Acq On : 27 Jul 2022 23:54
Operator : CG/JU
Sample : PB146378BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK378

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------