

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
 Data File : BM035965.D
 Acq On : 28 Jul 2022 00:30
 Operator : CG/JU
 Sample : PB146419BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK419

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035965.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	36	rVB	93571	109406	1.81%	0.149%
2	3.693	99	103	117	rBV	1127801	1551845	25.67%	2.112%
3	4.028	156	160	169	rVB	26929	37798	0.63%	0.051%
4	7.046	667	673	688	rVB	1202674	1906019	31.53%	2.594%
5	7.216	696	702	712	rVB	1070463	1616746	26.74%	2.200%
6	7.410	728	735	745	rBV	1301913	2042530	33.79%	2.780%
7	7.881	808	815	824	rBV	1291830	1994348	32.99%	2.714%
8	8.598	929	937	951	rBV	1493253	2426036	40.13%	3.301%
9	9.051	1006	1014	1028	rVB	1193593	1921318	31.78%	2.615%
10	9.769	1126	1136	1150	rBV	910657	1572988	26.02%	2.141%
11	10.310	1221	1228	1239	rBV	1412420	2364882	39.12%	3.218%
12	10.687	1285	1292	1304	rBV	1735994	2904684	48.05%	3.953%
13	10.828	1307	1316	1331	rBV	1482965	2549446	42.17%	3.469%
14	11.892	1488	1497	1500	rBV10	9270	26292	0.43%	0.036%
15	11.951	1502	1507	1513	rVV7	9580	25865	0.43%	0.035%
16	12.281	1558	1563	1570	rVB2	25879	47444	0.78%	0.065%
17	12.757	1637	1644	1649	rBV10	3800	8314	0.14%	0.011%
18	12.886	1660	1666	1675	rBV3	14042	33487	0.55%	0.046%
19	12.969	1679	1680	1685	rVB5	5173	6831	0.11%	0.009%
20	13.498	1765	1770	1773	rVB6	5081	8946	0.15%	0.012%
21	13.675	1797	1800	1802	rBV4	5436	6428	0.11%	0.009%
22	13.804	1814	1822	1833	rVB3	14271	38480	0.64%	0.052%
23	13.933	1838	1844	1854	rVV	2504511	3371986	55.78%	4.589%
24	14.216	1885	1892	1905	rVB	2989364	4316269	71.40%	5.874%
25	14.404	1923	1924	1929	rVB5	4266	6679	0.11%	0.009%
26	14.522	1937	1944	1958	rVB	2571165	3748777	62.01%	5.101%
27	14.622	1958	1961	1966	rVB7	6907	10166	0.17%	0.014%
28	14.722	1966	1978	1993	rBV	1037421	1613099	26.68%	2.195%
29	14.880	2003	2005	2009	rVB5	4928	6937	0.11%	0.009%
30	14.945	2012	2016	2021	rVB8	5729	9868	0.16%	0.013%
31	15.310	2073	2078	2082	rBV3	15547	30873	0.51%	0.042%
32	15.510	2103	2112	2119	rBV	3725344	5169183	85.51%	7.034%
33	15.627	2126	2132	2141	rBV	956902	1380470	22.83%	1.879%
34	15.745	2148	2152	2159	rVB2	44760	73021	1.21%	0.099%
35	15.880	2172	2175	2178	rBV4	4974	6957	0.12%	0.009%
36	15.921	2180	2182	2190	rVB9	7942	13787	0.23%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
 Data File : BM035965.D
 Acq On : 28 Jul 2022 00:30
 Operator : CG/JU
 Sample : PB146419BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK419

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	16.074	2204	2208	2212	rVB7	8914	12899	0.21%	0.018%
38	16.192	2225	2228	2230	rBV3	6922	8184	0.14%	0.011%
39	16.227	2231	2234	2241	rVV5	15061	28007	0.46%	0.038%
40	16.292	2241	2245	2251	rVB6	14070	24117	0.40%	0.033%
41	16.398	2260	2263	2264	rBV3	4935	6118	0.10%	0.008%
42	16.574	2287	2293	2297	rBV8	17240	38405	0.64%	0.052%
43	16.633	2301	2303	2307	rVB4	8176	10045	0.17%	0.014%
44	16.692	2310	2313	2316	rBV5	6794	7966	0.13%	0.011%
45	16.739	2316	2321	2327	rVB2	42893	60813	1.01%	0.083%
46	16.798	2329	2331	2336	rVB6	8294	10262	0.17%	0.014%
47	16.939	2352	2355	2359	rBV5	7625	12090	0.20%	0.016%
48	17.021	2365	2369	2372	rBV2	28758	43005	0.71%	0.059%
49	17.257	2403	2409	2417	rBV	2880446	4111186	68.00%	5.595%
50	17.357	2418	2426	2438	rVB	3900023	5422249	89.69%	7.379%
51	17.492	2448	2449	2456	rVB7	8774	11344	0.19%	0.015%
52	17.763	2492	2495	2498	rBV4	7933	10920	0.18%	0.015%
53	17.810	2499	2503	2509	rVB	45179	61787	1.02%	0.084%
54	17.927	2521	2523	2528	rVB6	13083	15580	0.26%	0.021%
55	18.227	2571	2574	2578	rBV	10964	15176	0.25%	0.021%
56	18.757	2659	2664	2670	rBV	45445	70835	1.17%	0.096%
57	19.215	2738	2742	2748	rVB2	50095	69692	1.15%	0.095%
58	19.280	2750	2753	2759	rVB	45456	64029	1.06%	0.087%
59	19.551	2796	2799	2803	rBV	45386	53944	0.89%	0.073%
60	19.645	2809	2815	2822	rBV	4443230	6045418	100.00%	8.227%
61	20.245	2914	2917	2921	rBV2	59020	78433	1.30%	0.107%
62	20.645	2982	2985	2990	rBV	285393	328353	5.43%	0.447%
63	21.433	3114	3119	3126	rBV	3394814	4259902	70.46%	5.797%
64	23.650	3490	3496	3503	rBV2	2903151	5525676	91.40%	7.519%
65	23.803	3516	3522	3533	rVB2	1998362	4120654	68.16%	5.607%



Sum of corrected areas: 73485294

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035965.D
Acq On : 28 Jul 2022 00:30
Operator : CG/JU
Sample : PB146419BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK419

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

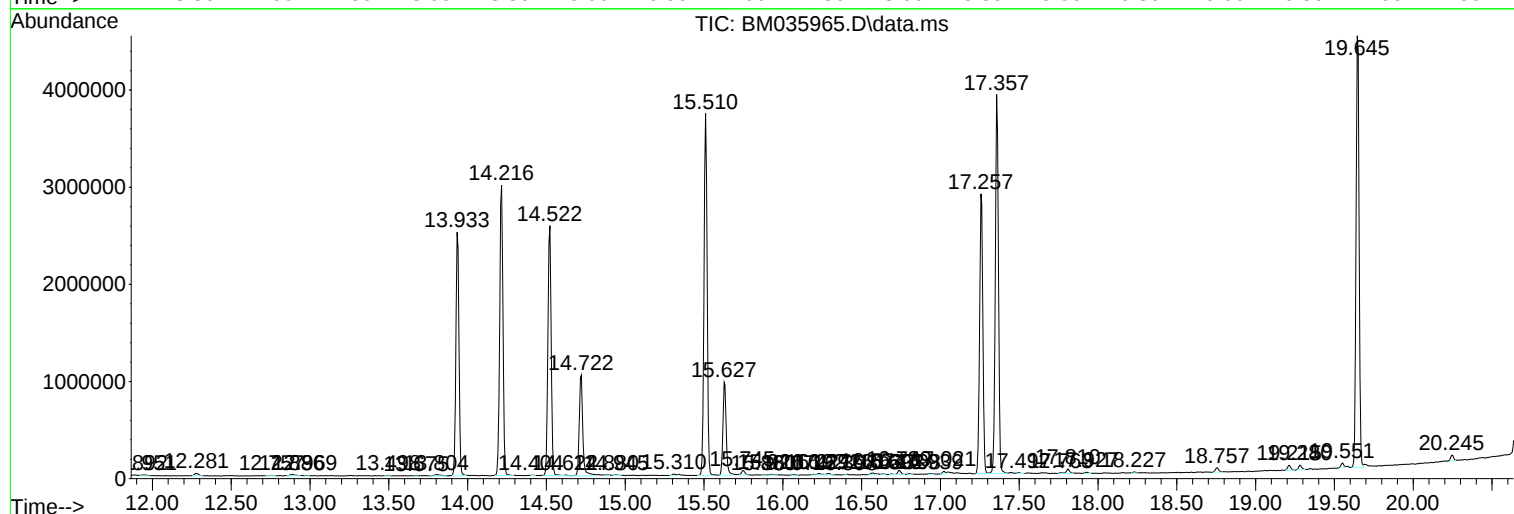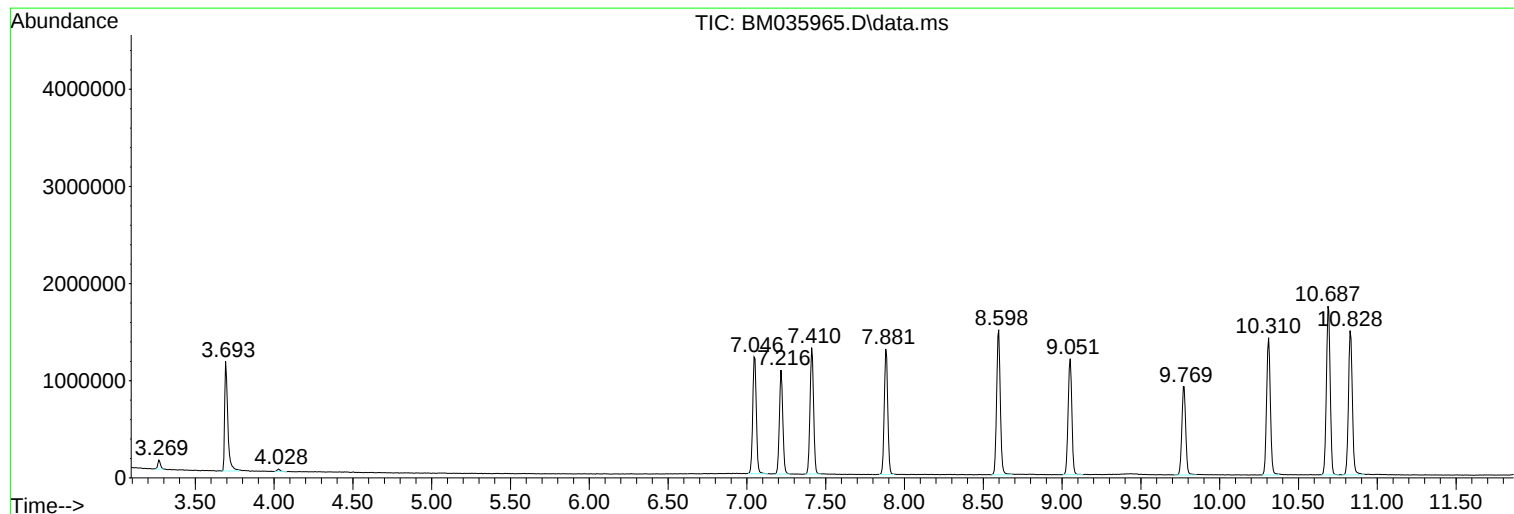

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035965.D
Acq On : 28 Jul 2022 00:30
Operator : CG/JU
Sample : PB146419BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK419

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035965.D
Acq On : 28 Jul 2022 00:30
Operator : CG/JU
Sample : PB146419BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK419

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------