

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
 Data File : BM035972.D
 Acq On : 28 Jul 2022 04:43
 Operator : CG/JU
 Sample : N3741-12
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0B37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035972.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	29	32	40	rVB2	23808	34576	0.87%	0.076%
2	3.716	104	107	112	rVB2	23992	28180	0.71%	0.062%
3	3.810	119	123	128	rVB	52839	64589	1.62%	0.141%
4	3.934	139	144	148	rBV	57719	78316	1.97%	0.172%
5	4.028	157	160	166	rVB	29539	40768	1.02%	0.089%
6	4.263	196	200	205	rVB3	18774	27254	0.68%	0.060%
7	4.599	255	257	262	rVB5	11155	12309	0.31%	0.027%
8	4.846	295	299	304	rBV8	7637	14678	0.37%	0.032%
9	4.963	315	319	327	rVB3	20208	42106	1.06%	0.092%
10	5.063	333	336	342	rVB6	10116	14871	0.37%	0.033%
11	5.569	420	422	427	rVB4	8487	12253	0.31%	0.027%
12	6.222	528	533	534	rBV5	4311	6691	0.17%	0.015%
13	6.275	539	542	545	rBV5	3503	4426	0.11%	0.010%
14	7.046	666	673	687	rVB	548246	884754	22.23%	1.938%
15	7.216	696	702	712	rVB	499523	763068	19.17%	1.672%
16	7.410	728	735	742	rBV	622888	962606	24.18%	2.109%
17	7.498	747	750	758	rVB6	10987	18826	0.47%	0.041%
18	7.881	808	815	823	rBV	1173583	1804843	45.34%	3.954%
19	7.945	824	826	829	rVB3	7945	8513	0.21%	0.019%
20	8.175	862	865	869	rBV6	2673	4700	0.12%	0.010%
21	8.592	930	936	946	rBV	520361	840196	21.11%	1.841%
22	8.710	952	956	961	rVB3	10758	19637	0.49%	0.043%
23	9.045	1007	1013	1022	rBV	554093	920044	23.11%	2.015%
24	9.216	1040	1042	1045	rVB4	6618	6237	0.16%	0.014%
25	9.457	1080	1083	1087	rVB5	11832	17824	0.45%	0.039%
26	9.581	1103	1104	1109	rVB4	4687	5525	0.14%	0.012%
27	9.769	1129	1136	1145	rVV	391243	642256	16.14%	1.407%
28	9.922	1160	1162	1168	rVB6	3211	5093	0.13%	0.011%
29	10.310	1221	1228	1240	rBV	661457	1105718	27.78%	2.422%
30	10.592	1271	1276	1277	rBV5	3726	4585	0.12%	0.010%
31	10.686	1285	1292	1305	rVB	1556731	2563368	64.40%	5.615%
32	10.828	1305	1316	1325	rBV	459666	825290	20.73%	1.808%
33	11.210	1380	1381	1386	rBV4	4645	5528	0.14%	0.012%
34	11.298	1392	1396	1399	rBV6	2675	4625	0.12%	0.010%
35	11.492	1423	1429	1433	rBV9	7856	16417	0.41%	0.036%
36	11.522	1433	1434	1440	rVB6	4466	5070	0.13%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
 Data File : BM035972.D
 Acq On : 28 Jul 2022 04:43
 Operator : CG/JU
 Sample : N3741-12
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0B37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	11.781	1474	1478	1482	rBV7	2818	5072	0.13%	0.011%
38	11.880	1488	1495	1499	rBV10	9316	23708	0.60%	0.052%
39	11.951	1502	1507	1508	rBV5	6044	8534	0.21%	0.019%
40	12.104	1532	1533	1537	rVB4	4174	5176	0.13%	0.011%
41	12.275	1557	1562	1569	rVB2	17222	29717	0.75%	0.065%
42	12.492	1596	1599	1601	rBV4	4015	5106	0.13%	0.011%
43	12.598	1616	1617	1622	rVB5	3831	4892	0.12%	0.011%
44	12.745	1639	1642	1644	rBV4	5106	6239	0.16%	0.014%
45	12.845	1656	1659	1661	rBV4	4892	4975	0.12%	0.011%
46	12.886	1661	1666	1669	rBV4	16353	26900	0.68%	0.059%
47	13.069	1692	1697	1699	rBV6	3970	6540	0.16%	0.014%
48	13.133	1705	1708	1711	rVB5	5324	6519	0.16%	0.014%
49	13.251	1722	1728	1731	rBV8	6280	10161	0.26%	0.022%
50	13.345	1741	1744	1749	rVB2	15235	18010	0.45%	0.039%
51	13.422	1751	1757	1761	rVV9	5042	9487	0.24%	0.021%
52	13.651	1791	1796	1799	rBV7	3213	6025	0.15%	0.013%
53	13.804	1817	1822	1825	rVV5	16770	28628	0.72%	0.063%
54	13.869	1825	1833	1838	rVV4	24528	69367	1.74%	0.152%
55	13.933	1838	1844	1851	rVV	1017018	1376282	34.58%	3.015%
56	14.004	1853	1856	1859	rVV3	18921	22543	0.57%	0.049%
57	14.045	1859	1863	1867	rVB7	6927	9550	0.24%	0.021%
58	14.210	1885	1891	1898	rVB	1487314	2169072	54.49%	4.752%
59	14.416	1922	1926	1932	rVB	32655	41697	1.05%	0.091%
60	14.469	1932	1935	1936	rBV3	4681	4657	0.12%	0.010%
61	14.516	1936	1943	1953	rBV	2221626	3271323	82.18%	7.166%
62	14.627	1959	1962	1968	rBV8	5385	10577	0.27%	0.023%
63	14.721	1972	1978	1989	rBV	221036	374697	9.41%	0.821%
64	14.874	2001	2004	2007	rVB5	6871	8262	0.21%	0.018%
65	14.939	2008	2015	2020	rVB4	41179	64921	1.63%	0.142%
66	15.027	2025	2030	2038	rVB2	82452	135280	3.40%	0.296%
67	15.104	2038	2043	2046	rBV5	6190	11931	0.30%	0.026%
68	15.310	2075	2078	2081	rBV3	19076	26733	0.67%	0.059%
69	15.363	2084	2087	2092	rVB	46325	61829	1.55%	0.135%
70	15.510	2105	2112	2119	rBV	1899345	2759195	69.32%	6.044%
71	15.627	2127	2132	2140	rVB	67329	108240	2.72%	0.237%
72	15.751	2148	2153	2154	rBV	23973	32700	0.82%	0.072%
73	15.868	2171	2173	2175	rBV2	6464	6593	0.17%	0.014%
74	15.921	2180	2182	2186	rVB5	10834	13350	0.34%	0.029%
75	16.074	2203	2208	2212	rBV8	12013	21283	0.53%	0.047%
76	16.227	2230	2234	2236	rBV	88110	117949	2.96%	0.258%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
 Data File : BM035972.D
 Acq On : 28 Jul 2022 04:43
 Operator : CG/JU
 Sample : N3741-12
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0B37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

77	16.392	2259	2262	2263	rBV3	7716	9025	0.23%	0.020%
78	16.568	2288	2292	2295	rBV5	24989	38915	0.98%	0.085%
79	16.627	2300	2302	2303	rBV2	7900	4829	0.12%	0.011%
80	16.739	2317	2321	2326	rBV2	40468	56122	1.41%	0.123%
81	16.804	2327	2332	2338	rVB	73261	102567	2.58%	0.225%
82	17.015	2364	2368	2372	rBV	82603	109655	2.75%	0.240%
83	17.068	2374	2377	2382	rVB	59802	88380	2.22%	0.194%
84	17.257	2403	2409	2415	rBV	2717912	3724414	93.57%	8.159%
85	17.357	2420	2426	2435	rVV	2076041	2909457	73.09%	6.374%
86	17.451	2439	2442	2446	rVB6	27400	33046	0.83%	0.072%
87	17.592	2463	2466	2470	rBV3	34312	48138	1.21%	0.105%
88	17.757	2490	2494	2498	rBV	68211	81038	2.04%	0.178%
89	17.810	2500	2503	2508	rVB	35742	49693	1.25%	0.109%
90	17.933	2520	2524	2528	rVB	86759	99607	2.50%	0.218%
91	18.451	2609	2612	2615	rBV2	64575	72424	1.82%	0.159%
92	18.751	2660	2663	2668	rVB2	41623	55676	1.40%	0.122%
93	19.080	2717	2719	2727	rBV	54942	76133	1.91%	0.167%
94	19.645	2810	2815	2823	rBV	2596812	3537304	88.87%	7.749%
95	20.021	2877	2879	2882	rVB	96977	87893	2.21%	0.193%
96	20.645	2983	2985	2989	rVB	189599	178763	4.49%	0.392%
97	21.150	3067	3071	3076	rBV	490737	621191	15.61%	1.361%
98	21.433	3114	3119	3124	rBV	3197315	3980480	100.00%	8.720%
99	23.650	3491	3496	3502	rVB2	1682923	3042495	76.44%	6.665%
100	23.803	3516	3522	3532	rVB2	2023837	3902241	98.03%	8.548%




Sum of corrected areas: 45648946

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035972.D
Acq On : 28 Jul 2022 04:43
Operator : CG/JU
Sample : N3741-12
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0B37

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

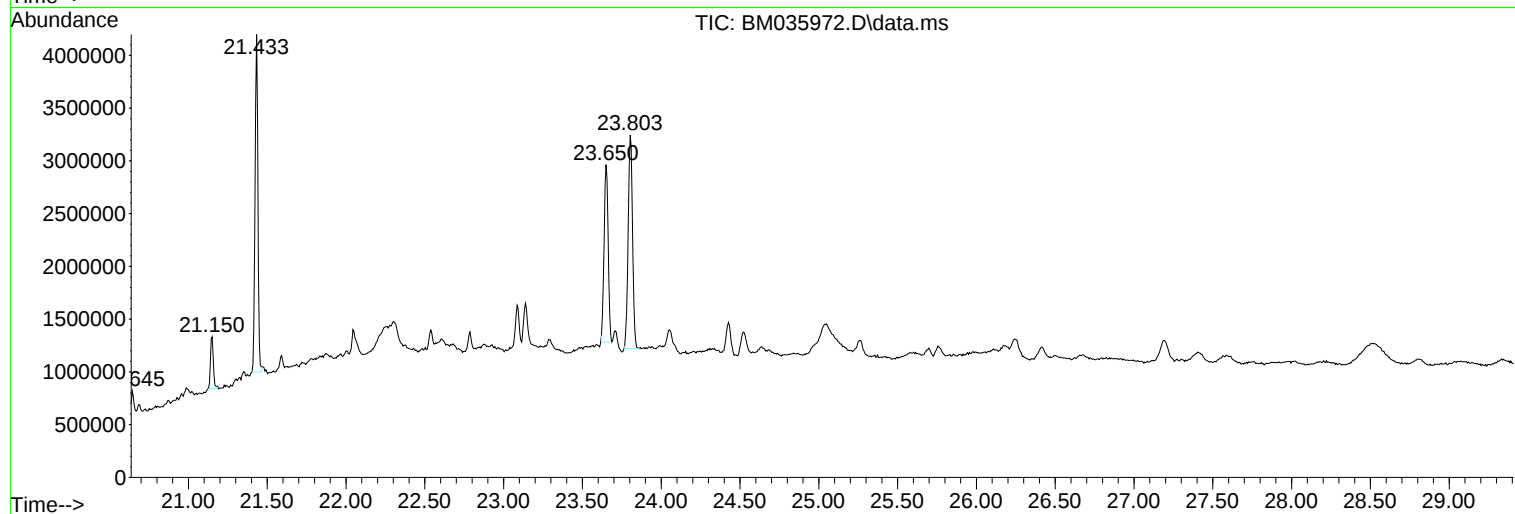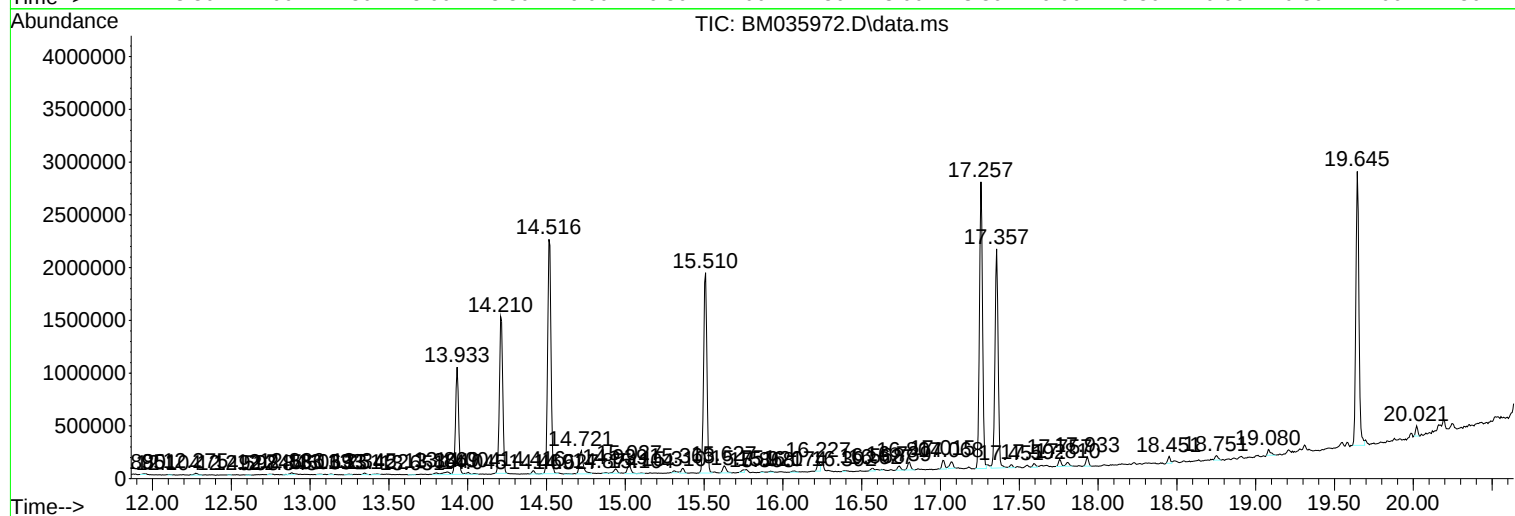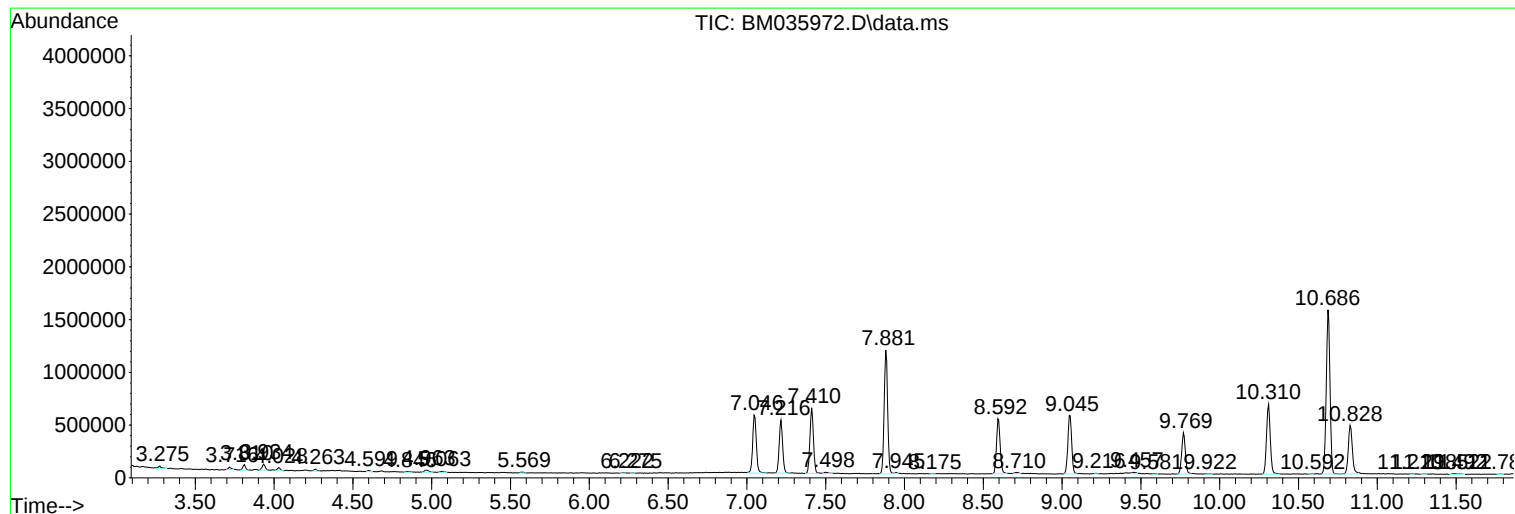

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035972.D
Acq On : 28 Jul 2022 04:43
Operator : CG/JU
Sample : N3741-12
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0B37










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(tetradecyloxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.151	3.12 ng/ul	621191	Chrysene-d12	21.433

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(tetradecyloxy)-	258	C16H34O2	002136-70-1	95
2			1-Hexacosanol	382	C26H54O	000506-52-5	90
3			Oxalic acid, isobutyl hexadecyl ...	370	C22H42O4	1000309-38-1	90
4			Oxalic acid, isobutyl tetradecyl...	342	C20H38O4	1000309-37-9	87
5			Methoxyacetic acid, heptadecyl e...	328	C20H40O3	1000282-99-1	87

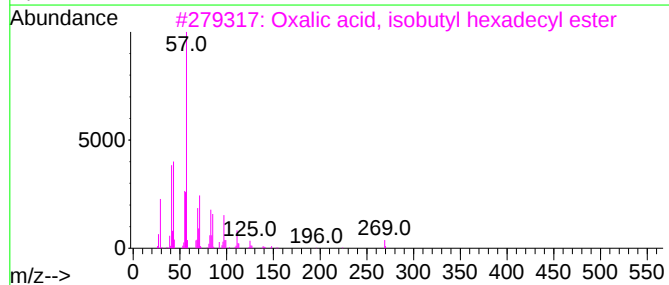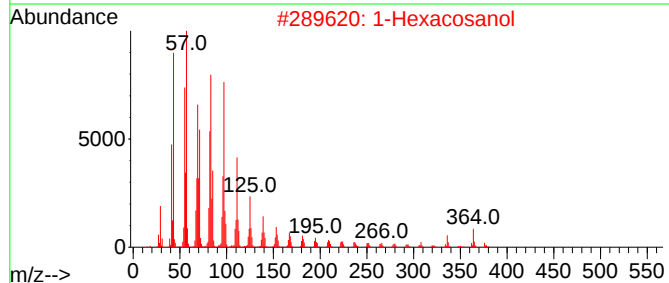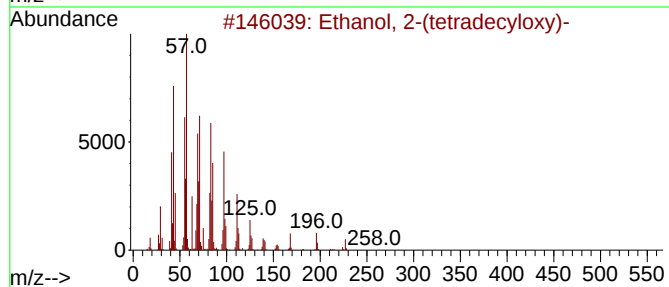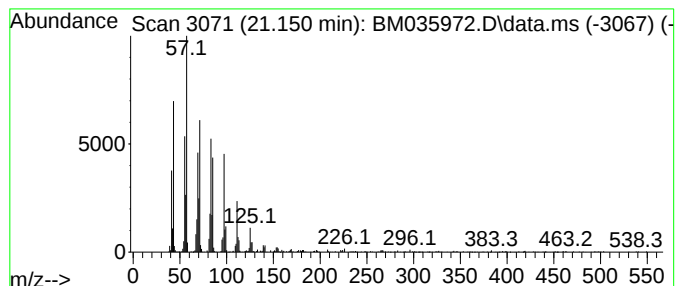

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035972.D
Acq On : 28 Jul 2022 04:43
Operator : CG/JU
Sample : N3741-12
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0B37

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(tet...	21.151	3.1	ng/u1	621191	5	21.433	3980480	20.0