

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
 Data File : BM035978.D
 Acq On : 28 Jul 2022 08:56
 Operator : CG/JU
 Sample : PB146485BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK485

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035978.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	36	rVB	92587	109271	1.98%	0.172%
2	3.693	99	103	121	rBV	1073467	1536183	27.90%	2.413%
3	4.028	156	160	166	rVB	28016	40801	0.74%	0.064%
4	7.045	666	673	683	rVB	1183616	1826693	33.18%	2.870%
5	7.216	695	702	713	rVB	986271	1548460	28.12%	2.432%
6	7.410	728	735	743	rBV	1253953	1961208	35.62%	3.081%
7	7.598	764	767	770	rBV5	3712	6010	0.11%	0.009%
8	7.881	807	815	822	rBV	1009247	1583339	28.76%	2.487%
9	8.592	929	936	948	rBV	1433143	2286239	41.52%	3.591%
10	9.045	1006	1013	1023	rBV	1125931	1798671	32.67%	2.826%
11	9.769	1127	1136	1148	rBV	877164	1433454	26.03%	2.252%
12	9.863	1150	1152	1156	rVB4	4096	6039	0.11%	0.009%
13	10.304	1220	1227	1241	rBV	1335985	2200147	39.96%	3.456%
14	10.686	1284	1292	1300	rVB	1366638	2239424	40.67%	3.518%
15	10.828	1307	1316	1329	rBV	1361635	2335666	42.42%	3.669%
16	10.951	1336	1337	1341	rVB4	5558	5575	0.10%	0.009%
17	11.063	1354	1356	1363	rVB8	5652	10133	0.18%	0.016%
18	11.875	1489	1494	1497	rBV6	4692	8018	0.15%	0.013%
19	11.945	1502	1506	1510	rVB6	6719	11704	0.21%	0.018%
20	12.275	1556	1562	1570	rVB3	26369	50671	0.92%	0.080%
21	12.680	1626	1631	1633	rBV6	5296	9024	0.16%	0.014%
22	12.739	1638	1641	1645	rVV5	4735	7594	0.14%	0.012%
23	12.886	1660	1666	1670	rBV4	13710	23145	0.42%	0.036%
24	12.939	1673	1675	1679	rVB5	4369	5533	0.10%	0.009%
25	13.098	1694	1702	1710	rBV5	3372	11092	0.20%	0.017%
26	13.251	1723	1728	1730	rBV6	3966	5961	0.11%	0.009%
27	13.304	1734	1737	1740	rBV5	4226	5822	0.11%	0.009%
28	13.486	1765	1768	1772	rBV5	4707	6818	0.12%	0.011%
29	13.733	1804	1810	1812	rVV7	4977	6614	0.12%	0.010%
30	13.798	1817	1821	1830	rVB9	9734	21277	0.39%	0.033%
31	13.933	1836	1844	1853	rBV	2172395	2975675	54.04%	4.675%
32	14.210	1882	1891	1903	rBV	2663927	3825164	69.47%	6.009%
33	14.516	1936	1943	1956	rBV	1906170	2723269	49.46%	4.278%
34	14.616	1956	1960	1963	rVB6	5367	8783	0.16%	0.014%
35	14.716	1971	1977	1993	rBV	931338	1409473	25.60%	2.214%
36	15.151	2047	2051	2056	rBV8	6078	11463	0.21%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
 Data File : BM035978.D
 Acq On : 28 Jul 2022 08:56
 Operator : CG/JU
 Sample : PB146485BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK485

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	15.304	2073	2077	2080	rBV5	9902	14290	0.26%	0.022%
38	15.504	2104	2111	2120	rBV	3196815	4552225	82.67%	7.151%
39	15.627	2126	2132	2147	rBV	789975	1092599	19.84%	1.716%
40	15.745	2147	2152	2160	rVB	41965	67217	1.22%	0.106%
41	15.874	2171	2174	2176	rBV3	4185	5562	0.10%	0.009%
42	15.927	2180	2183	2187	rVB6	8366	13186	0.24%	0.021%
43	16.186	2223	2227	2230	rBV6	7443	12538	0.23%	0.020%
44	16.227	2230	2234	2237	rVV4	12507	19695	0.36%	0.031%
45	16.292	2241	2245	2248	rVB5	13069	18041	0.33%	0.028%
46	16.398	2258	2263	2268	rBV7	8144	16953	0.31%	0.027%
47	16.568	2287	2292	2295	rBV4	17381	29642	0.54%	0.047%
48	16.627	2300	2302	2307	rVB6	8403	8924	0.16%	0.014%
49	16.733	2316	2320	2327	rBV2	34607	47362	0.86%	0.074%
50	16.792	2327	2330	2335	rBV6	4642	8124	0.15%	0.013%
51	16.927	2351	2353	2357	rVV4	7346	10216	0.19%	0.016%
52	17.015	2365	2368	2371	rBV2	21747	28817	0.52%	0.045%
53	17.257	2403	2409	2417	rBV	2113560	2922913	53.08%	4.592%
54	17.357	2417	2426	2438	rVV	3449420	4806801	87.30%	7.551%
55	17.445	2438	2441	2446	rVB7	8350	15354	0.28%	0.024%
56	17.486	2446	2448	2451	rBV4	5807	7343	0.13%	0.012%
57	17.809	2498	2503	2509	rVB	34864	50622	0.92%	0.080%
58	18.145	2557	2560	2561	rBV3	5712	6657	0.12%	0.010%
59	18.751	2660	2663	2668	rBV2	33095	46499	0.84%	0.073%
60	19.209	2737	2741	2747	rBV2	47043	65258	1.19%	0.103%
61	19.280	2749	2753	2758	rVB2	44395	59337	1.08%	0.093%
62	19.551	2796	2799	2803	rBV	26116	31810	0.58%	0.050%
63	19.645	2809	2815	2821	rBV	4244513	5506206	100.00%	8.650%
64	20.245	2915	2917	2922	rVB4	38117	40361	0.73%	0.063%
65	20.645	2982	2985	2989	rBV	166202	188706	3.43%	0.296%
66	21.433	3114	3119	3125	rBV	2526891	3181830	57.79%	4.998%
67	23.650	3490	3496	3504	rBV2	2843927	5413751	98.32%	8.504%
68	23.803	3516	3522	3536	rVB2	1672803	3314282	60.19%	5.206%




Sum of corrected areas: 63657534

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035978.D
Acq On : 28 Jul 2022 08:56
Operator : CG/JU
Sample : PB146485BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK485

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

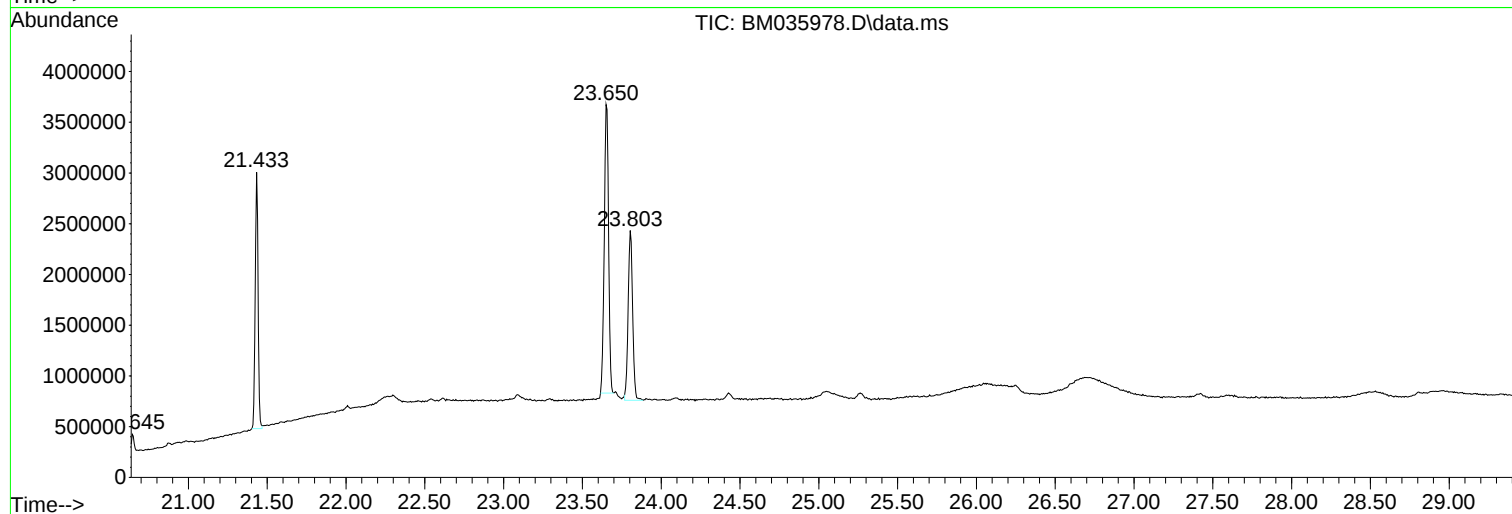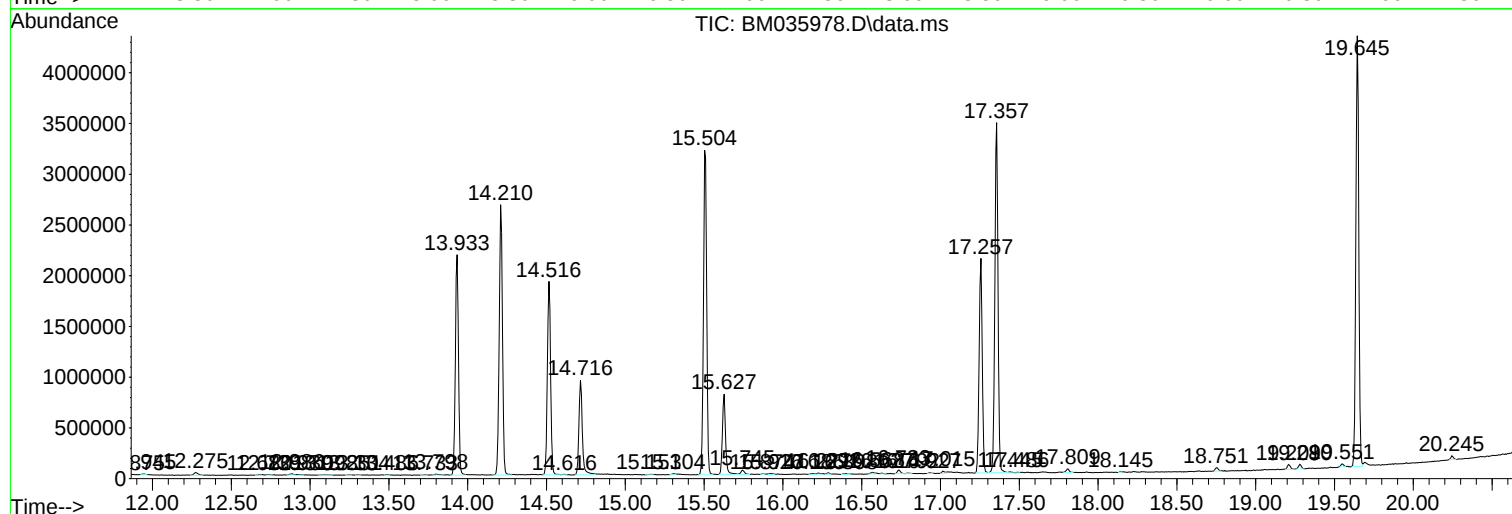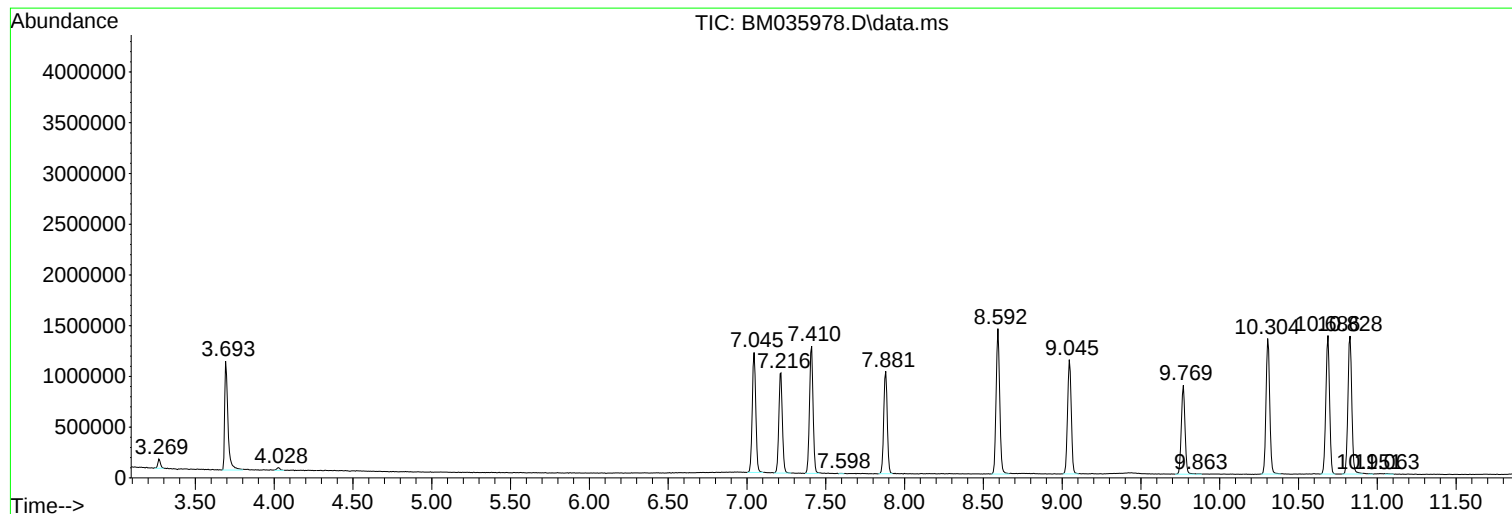

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035978.D
Acq On : 28 Jul 2022 08:56
Operator : CG/JU
Sample : PB146485BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK485

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072722\
Data File : BM035978.D
Acq On : 28 Jul 2022 08:56
Operator : CG/JU
Sample : PB146485BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK485

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc