
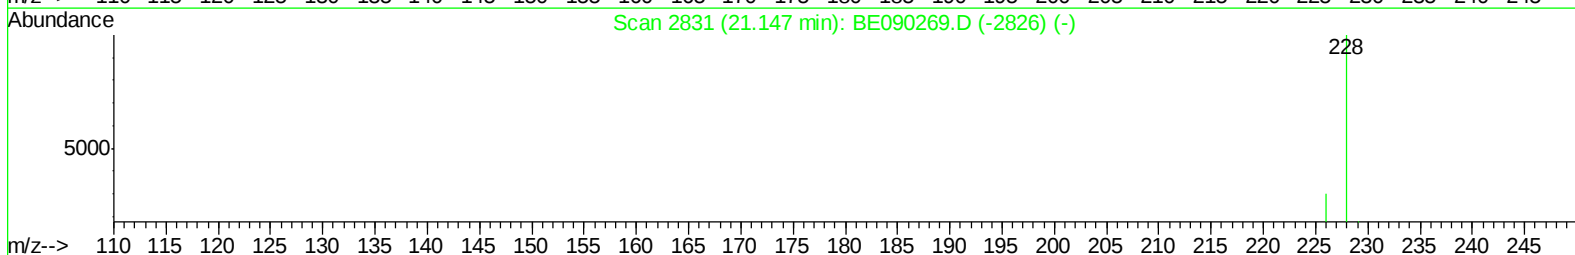
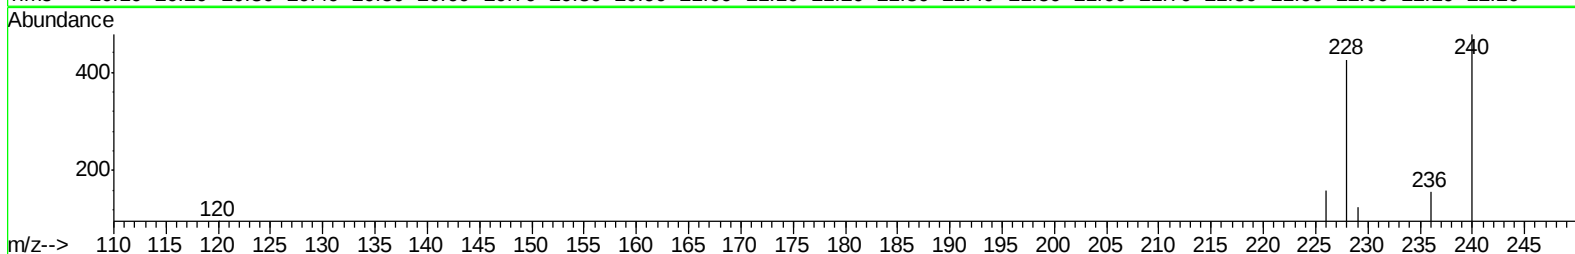


Data Path : Z:\HPCHEM1\BNA\_E\DATA\BE072815\  
Data File : BE090267.D  
Acq On : 28 Jul 2015 12:29  
Operator : TP/IZ  
Sample : SST0.142  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Jul 29 04:15:57 2015  
Quant Method : Z:\HPCHEM1\BNA\_E\METHODS\SOM02.2-EPA-SIM-BE072815.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jul 29 04:02:27 2015  
Response via : Initial Calibration

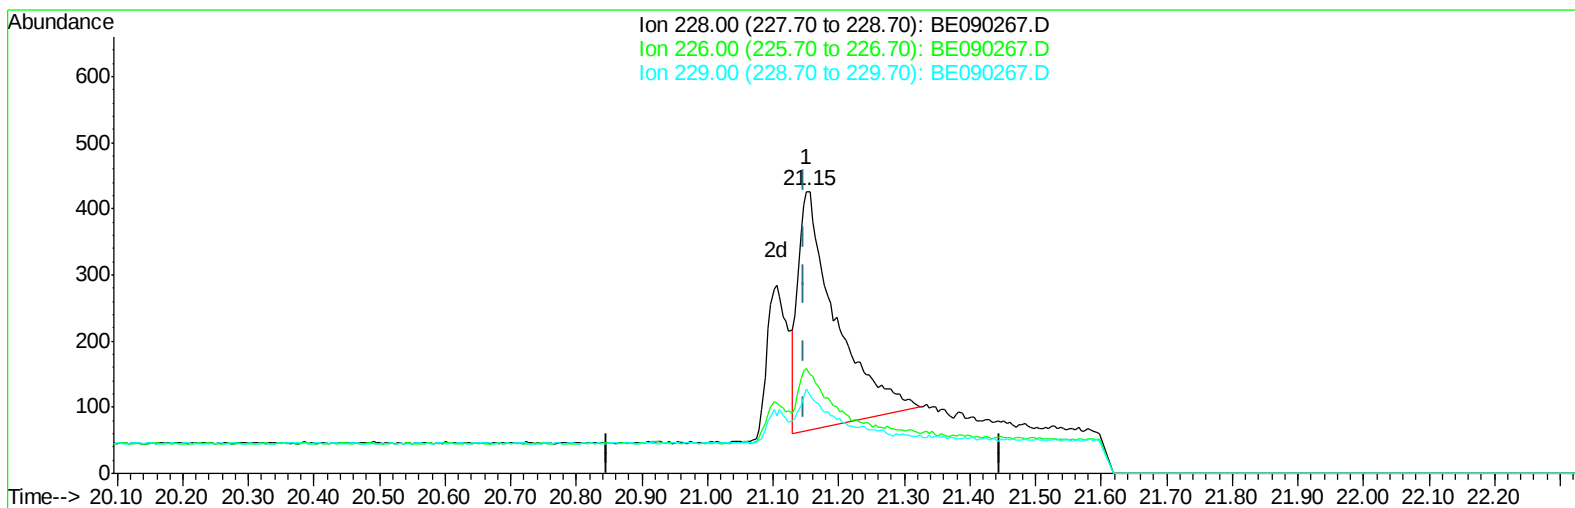

TIC: BE090267.D

(19) Chrysene

21.151min (+0.004) 0.09ng/ul

response 1457

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 228.00 | 100   | 100    |
| 226.00 | 31.20 | 37.32  |
| 229.00 | 20.70 | 29.81# |
| 0.00   | 0.00  | 0.00   |