
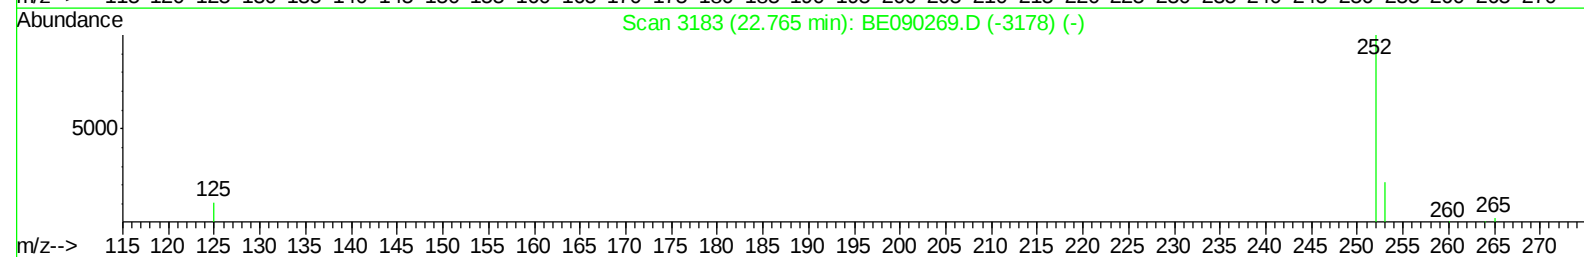
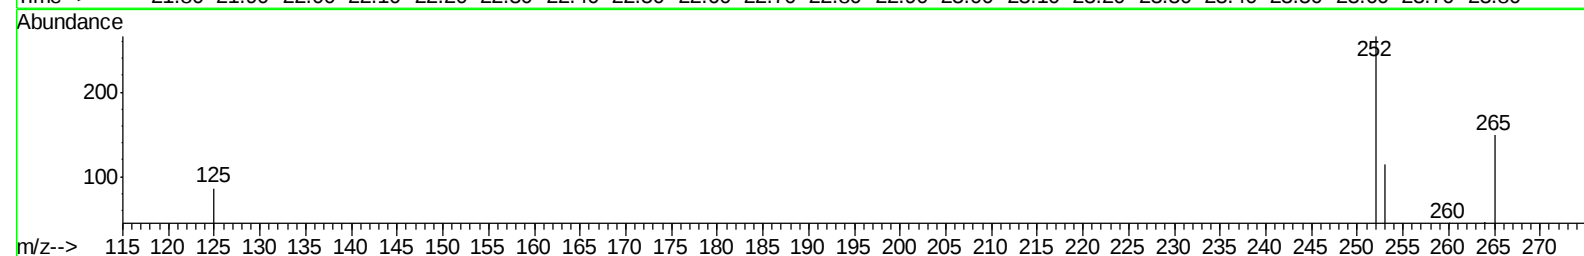


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE072815\
Data File : BE090267.D
Acq On : 28 Jul 2015 12:29
Operator : TP/IZ
Sample : SST00.142
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Jul 29 04:15:57 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE072815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 29 04:02:27 2015
Response via : Initial Calibration

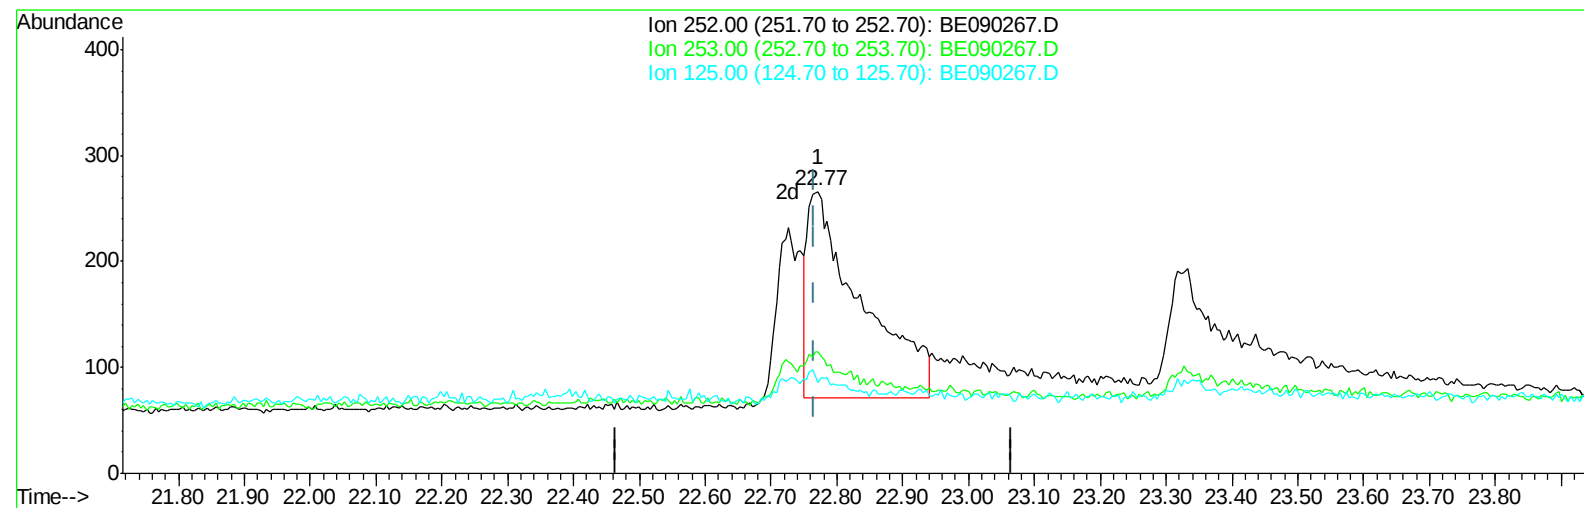

TIC: BE090267.D

(22) Benzo(k)fluoranthene

22.772min (+0.006) 0.09ng/ul m

response 1116

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	43.23#
125.00	16.60	32.33#
0.00	0.00	0.00