
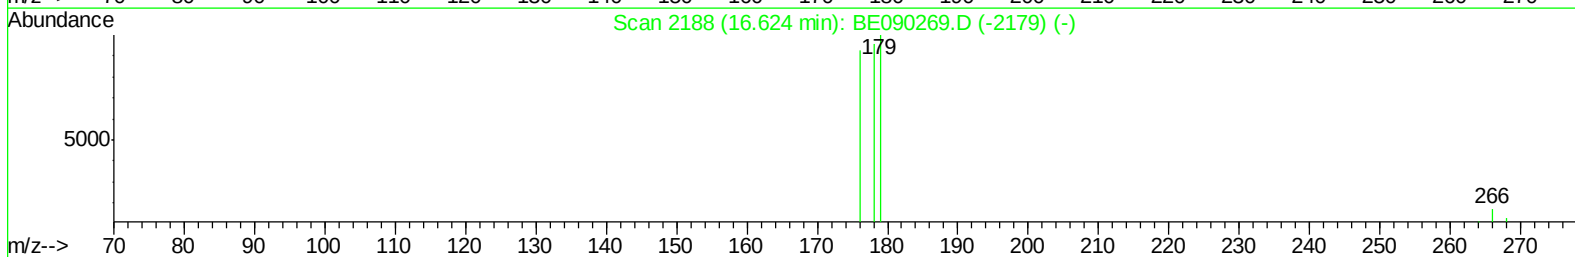
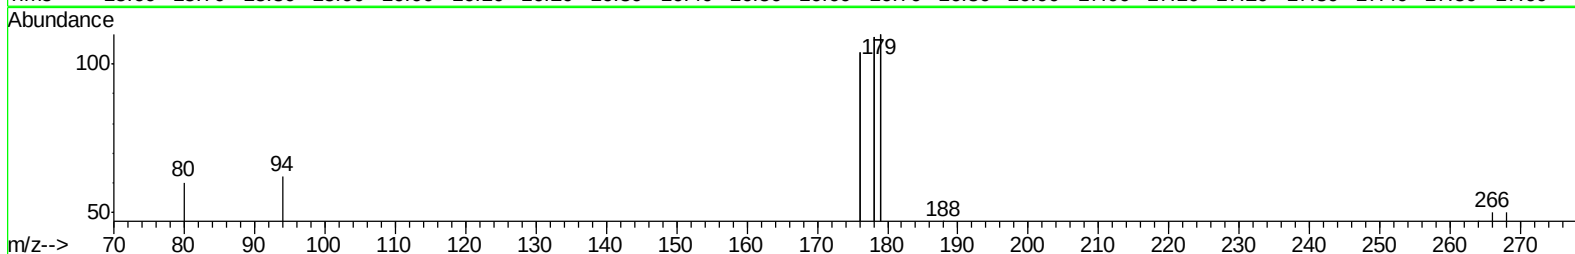


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE072815\
Data File : BE090268.D
Acq On : 28 Jul 2015 13:05
Operator : TP/IZ
Sample : SST0.243
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jul 29 04:18:19 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE072815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 29 04:02:27 2015
Response via : Initial Calibration

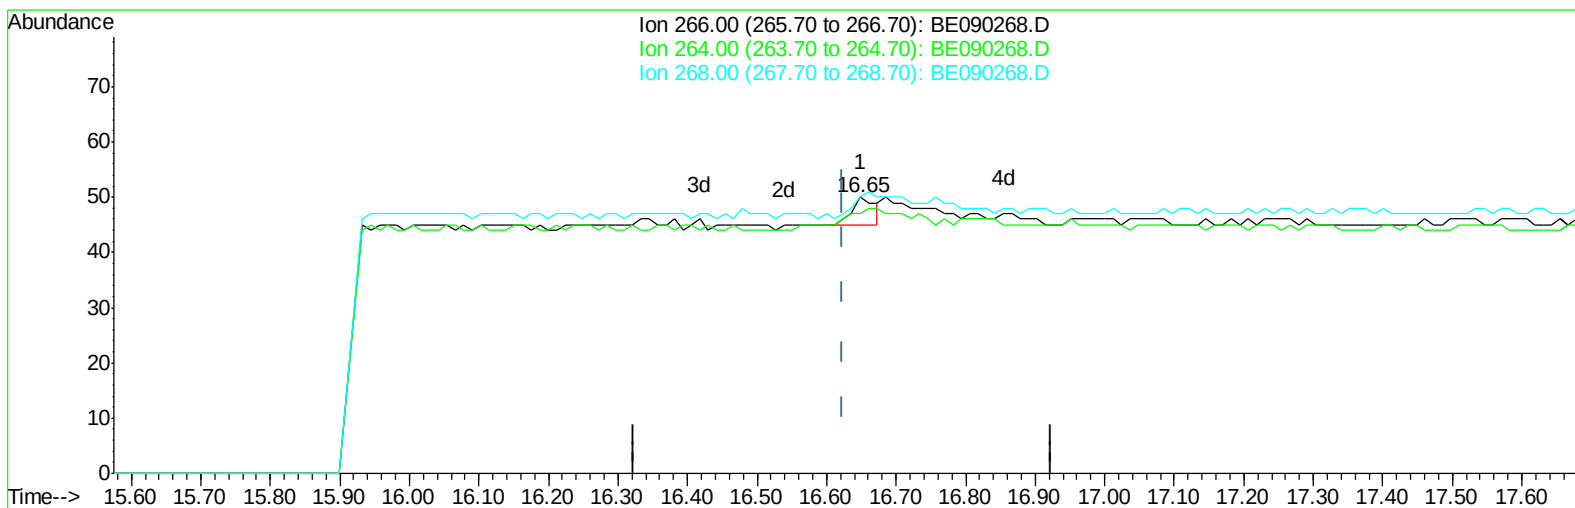

TIC: BE090268.D

(11) Pentachlorophenol

16.648min (+0.025) 0.03ng/ul

response 12

Ion	Exp%	Act%
266.00	100	100
264.00	54.20	125.00#
268.00	55.70	208.33#
0.00	0.00	0.00