
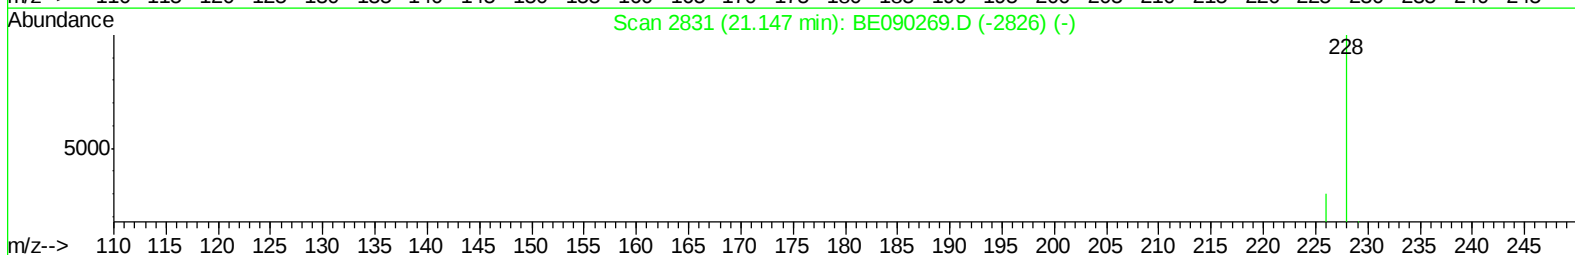
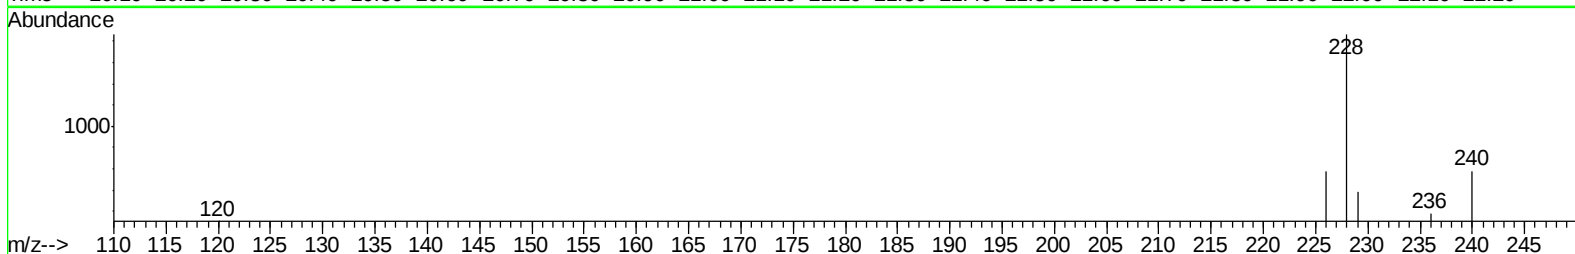


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE072815\
Data File : BE090269.D
Acq On : 28 Jul 2015 13:40
Operator : TP/IZ
Sample : SST0.444
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Jul 29 04:20:31 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE072815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 29 04:02:27 2015
Response via : Initial Calibration

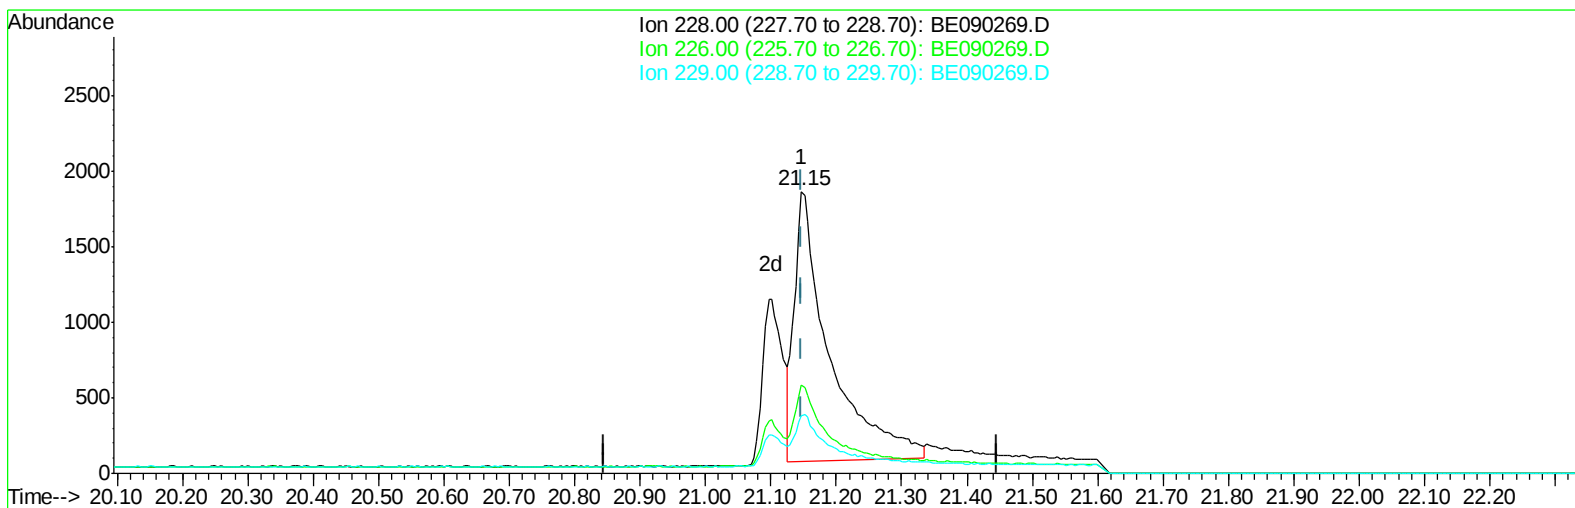

TIC: BE090269.D

(19) Chrysene

21.147min (0.000) 0.36ng/ul m

response 6682

Ion	Exp%	Act%
228.00	100	100
226.00	31.20	31.20
229.00	20.70	20.68
0.00	0.00	0.00