
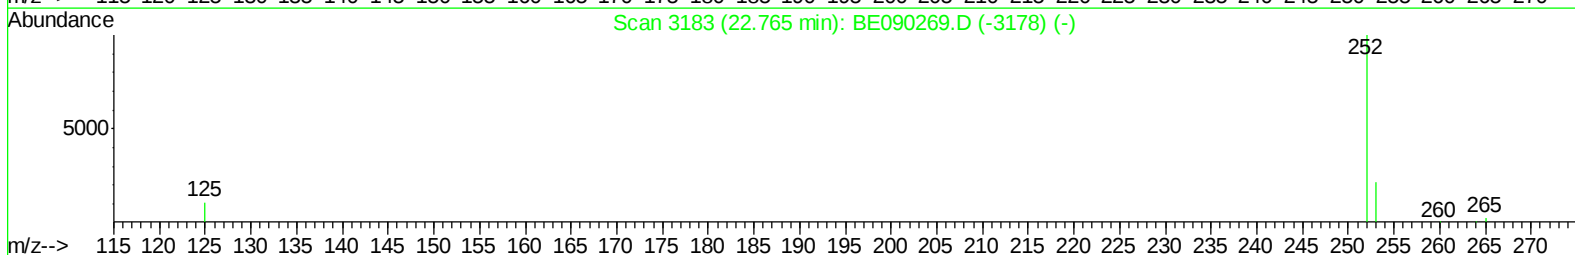
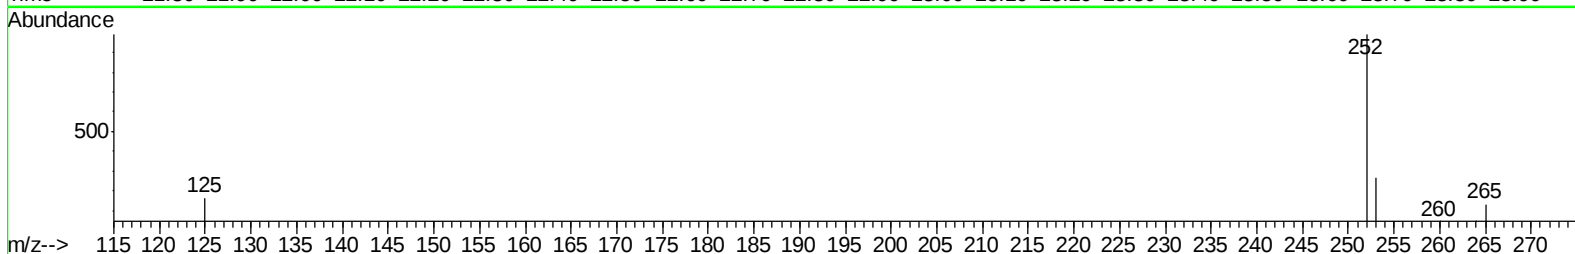


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE072815\
Data File : BE090269.D
Acq On : 28 Jul 2015 13:40
Operator : TP/IZ
Sample : SST0.444
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Jul 29 04:20:31 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE072815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 29 04:02:27 2015
Response via : Initial Calibration

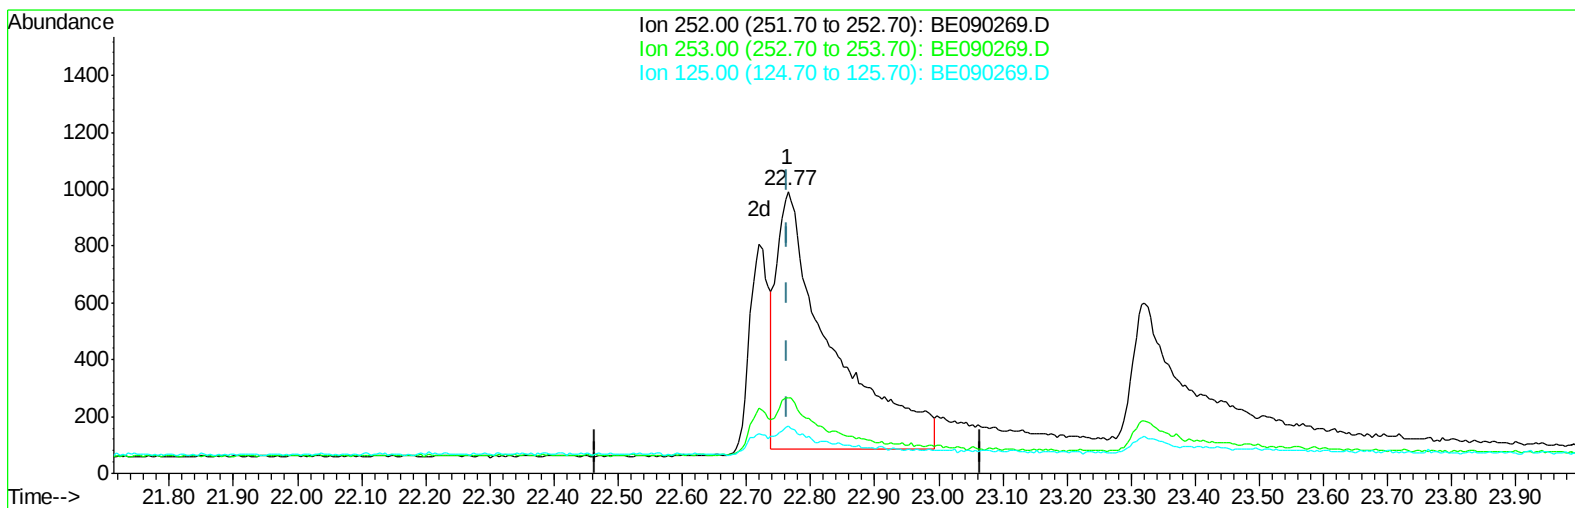

TIC: BE090269.D

(22) Benzo(k)fluoranthene

22.765min (0.000) 0.34ng/ul m

response 5330

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	26.64
125.00	16.60	16.65
0.00	0.00	0.00