


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072816\
Data File : BM006718.D
Acq On : 28 Jul 2016 10:34
Operator : UM/SJ
Sample : DFTPP60
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP60

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Title : SVOA CALIBRATION
Last Update : Wed Jul 20 04:22:37 2016

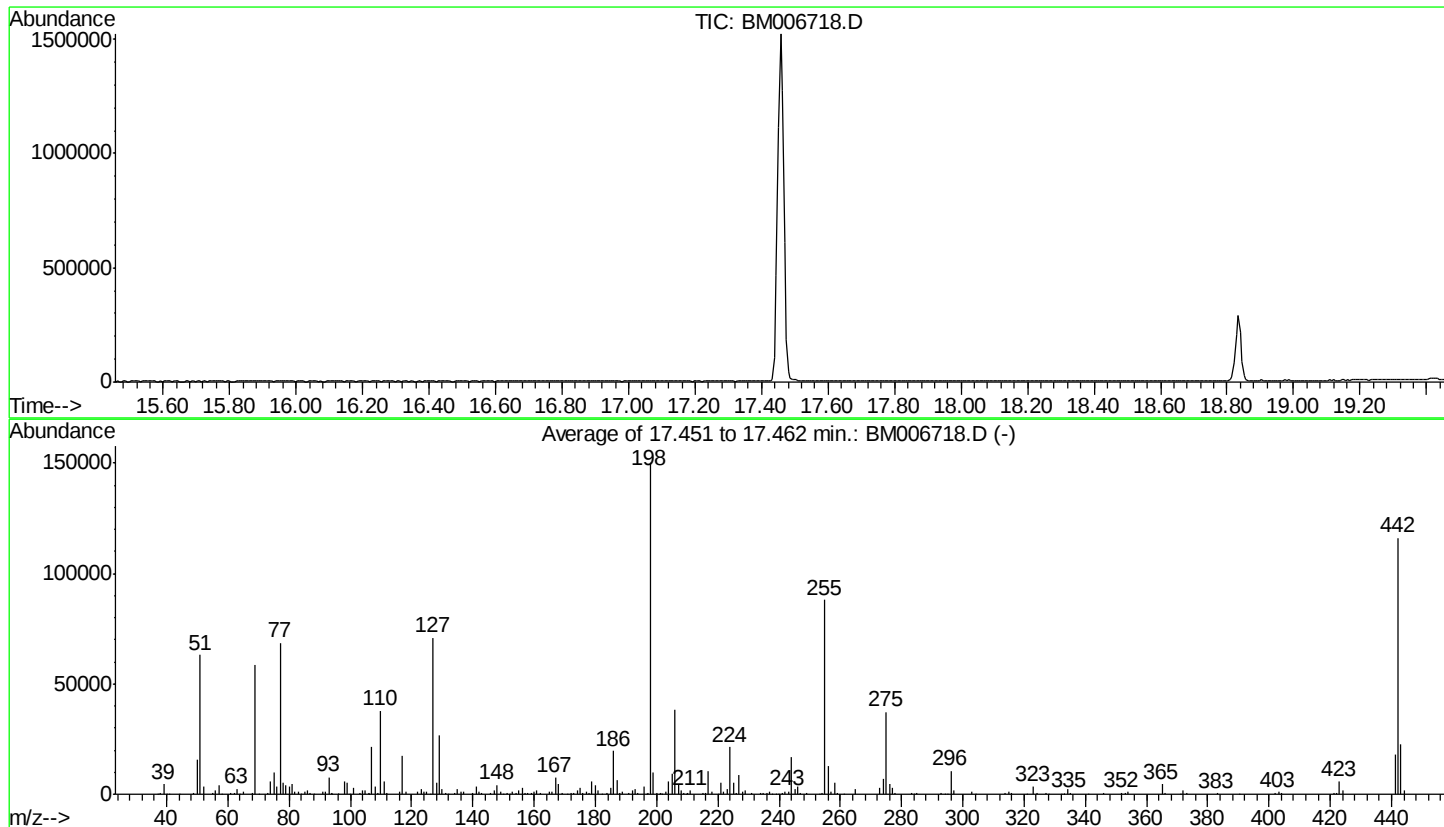

AutoFind: Scans 2527, 2528, 2529; Background Corrected with Scan 2522

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	63058	PASS
68	69	0.00	2	1.5	881	PASS
69	198	0.00	100	39.2	58810	PASS
70	69	0.00	2	0.2	126	PASS
127	198	10	80	47.1	70768	PASS
197	198	0.00	2	0.3	497	PASS
198	198	100	100	100.0	150197	PASS
199	198	5	9	6.6	9955	PASS
275	198	10	60	24.8	37218	PASS
365	198	1	100	3.0	4478	PASS
441	443	0.01	100	78.1	17803	PASS
442	198	50	100	77.3	116053	PASS
443	442	15	24	19.7	22807	PASS

m/z	Abundance
38.00	731.0
39.10	4690.0
39.90	1109.0
44.00	1276.0
48.90	761.0
50.00	14948.0
51.00	61648.0
52.00	3579.0
55.00	495.0
56.00	2024.0
57.00	3835.0
61.00	615.0
62.10	903.0
63.00	2451.0
64.00	352.0
65.00	1255.0
68.10	965.0
69.00	55848.0
73.00	919.0
74.00	6020.0
75.00	9700.0
76.00	3730.0
77.10	65368.0
78.10	5037.0
79.00	3897.0
80.00	3334.0
81.00	4942.0
82.00	1360.0
83.00	1125.0
84.00	507.0
85.00	738.0
86.00	1503.0
87.00	515.0
91.00	1174.0
91.90	1110.0
93.00	6553.0
93.80	497.0
96.00	445.0
98.00	5715.0
99.00	5558.0
100.00	321.0
101.00	2919.0
103.00	845.0
104.00	1609.0
105.00	1456.0
105.90	652.0
107.00	19696.0
108.00	3142.0
108.90	541.0
110.00	34392.0
111.00	5325.0
112.00	501.0
115.90	1010.0
117.00	15431.0
118.00	1243.0
122.00	1096.0
123.00	2132.0
123.90	843.0
125.00	925.0
126.10	314.0
127.00	62864.0
128.00	5051.0
129.00	23992.0
129.90	2274.0
131.10	320.0
133.90	834.0
135.00	2274.0
136.00	794.0
137.00	1343.0
139.90	320.0
141.00	3210.0
142.00	1028.0
142.90	517.0
146.00	476.0
147.00	1804.0
148.00	3658.0
149.00	990.0
151.10	419.0
153.00	938.0
153.90	668.0
155.00	1524.0
156.00	2837.0
157.00	612.0
157.90	648.0
158.90	491.0
160.00	1098.0
161.00	1507.0
162.00	513.0
164.90	826.0
165.90	845.0
167.00	5741.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

168.00	4755.0
169.00	879.0
171.90	557.0
173.00	891.0
174.00	1341.0
175.00	2753.0
176.00	647.0
176.90	1357.0
178.10	515.0
178.90	4691.0
180.00	3217.0
180.90	1765.0
182.00	311.0
183.90	515.0
185.10	2538.0
186.00	16512.0
187.00	5362.0
188.10	524.0
188.90	911.0
190.90	581.0
192.00	1651.0
193.00	2047.0
194.00	375.0
196.00	3110.0
196.90	609.0
198.00	127776.0
199.00	9021.0
200.00	526.0
201.50	481.0
202.90	1051.0
204.00	4555.0
205.00	7297.0
206.10	32424.0
207.10	5206.0
208.00	1231.0
208.90	516.0
209.90	403.0
211.00	1198.0
215.00	375.0
216.00	851.0
217.00	8591.0
218.00	1045.0
221.00	4545.0
221.90	1123.0
223.00	1938.0
224.00	17808.0
225.00	4477.0
226.00	492.0
227.00	7158.0
227.90	1176.0
229.00	1449.0
231.00	732.0
234.00	688.0
235.00	693.0
235.90	471.0
237.00	996.0
239.00	324.0
241.00	483.0
242.00	1141.0
243.00	940.0
244.10	13259.0
245.00	1805.0
246.00	2391.0
247.00	482.0
249.00	414.0
254.10	405.0
255.00	72256.0
256.00	11156.0
257.10	1299.0
258.00	4121.0
259.00	592.0
265.00	1678.0
273.00	2172.0
274.00	5853.0
275.00	29248.0
276.00	4531.0
277.00	2217.0
278.00	627.0
285.00	315.0
293.10	698.0
296.00	8057.0
296.90	1158.0
303.00	749.0
315.00	962.0
316.00	632.0
321.00	333.0
323.10	2492.0
324.00	504.0
327.00	704.0
328.00	362.0
334.00	2052.0
335.00	464.0
346.00	690.0
352.00	666.0
353.10	653.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

354.10	923.0
365.00	3274.0
365.90	380.0
372.00	1418.0
373.00	370.0
401.90	399.0
403.10	679.0
404.00	336.0
421.00	786.0
422.00	560.0
423.10	3829.0
424.10	1706.0
441.10	11737.0
442.10	74944.0
443.10	16142.0
444.00	1603.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

m/z	Abundance
36.90	338.0
38.00	1022.0
39.10	5437.0
40.00	962.0
41.00	389.0
44.00	1338.0
49.00	774.0
50.00	18648.0
51.10	73840.0
52.00	3586.0
54.90	432.0
55.90	2060.0
57.00	4982.0
58.00	307.0
61.00	1038.0
62.00	866.0
63.00	2939.0
64.00	394.0
65.00	1460.0
68.00	928.0
69.00	68520.0
70.00	380.0
73.00	751.0
74.00	6745.0
75.00	11917.0
76.00	3854.0
77.10	79744.0
78.10	5966.0
79.00	5040.0
80.00	3602.0
81.00	5248.0
82.00	1243.0
83.00	1366.0
83.90	409.0
84.90	1240.0
86.00	1708.0
87.00	806.0
88.00	381.0
91.00	1172.0
92.00	1721.0
93.00	9788.0
94.00	757.0
95.90	359.0
96.20	353.0
98.00	6796.0
99.00	5777.0
99.90	475.0
101.00	3124.0
103.00	881.0
104.00	1595.0
105.00	2015.0
105.90	926.0
107.00	24264.0
108.00	3699.0
109.00	859.0
110.00	43440.0
111.00	7318.0
112.00	1162.0
116.00	1112.0
117.00	20904.0
118.10	1490.0
122.00	1208.0
123.00	2558.0
123.90	1054.0
125.00	1237.0
126.10	374.0
127.00	83752.0
128.00	6452.0
129.00	31664.0
129.90	2149.0
130.90	552.0
131.90	301.0
133.90	921.0
135.00	2598.0
136.00	1080.0
137.00	1380.0
139.90	420.0
141.00	3841.0
142.00	1603.0
143.00	1146.0
145.90	645.0
147.00	2171.0
148.00	5031.0
149.00	1018.0
150.10	303.0
151.00	443.0
153.00	1259.0
154.00	905.0
155.00	2274.0
156.00	3593.0
156.80	305.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

157.90	592.0
159.00	614.0
160.00	1141.0
161.00	1737.0
162.00	433.0
165.00	1832.0
166.00	1211.0
167.00	8346.0
168.00	5222.0
169.00	885.0
171.90	731.0
173.00	928.0
174.00	1873.0
175.00	3309.0
176.00	1004.0
176.90	1359.0
178.00	452.0
179.00	6458.0
180.00	5592.0
181.00	1641.0
184.00	713.0
185.00	3113.0
186.10	23208.0
187.00	7836.0
188.00	785.0
189.00	1467.0
191.00	871.0
191.90	1941.0
193.00	2578.0
194.00	417.0
196.00	4517.0
197.00	883.0
198.00	176384.0
199.00	11237.0
200.00	950.0
200.90	448.0
201.50	478.0
203.00	1175.0
204.00	7310.0
205.00	11044.0
206.00	45016.0
207.10	7024.0
208.00	1857.0
209.00	514.0
210.30	661.0
211.00	1945.0
214.90	512.0
216.00	947.0
217.00	11961.0
218.00	1648.0
220.20	328.0
221.00	6089.0
221.80	1797.0
223.00	2408.0
224.00	24624.0
225.10	5422.0
226.00	852.0
227.00	10269.0
228.00	1533.0
229.00	2339.0
231.00	991.0
234.00	737.0
234.90	518.0
235.80	474.0
237.00	1021.0
237.90	355.0
238.90	441.0
239.90	517.0
241.00	549.0
242.00	1224.0
243.00	1619.0
244.00	19760.0
245.10	2519.0
246.00	4266.0
247.00	1047.0
249.00	808.0
253.10	361.0
254.10	676.0
255.00	104152.0
256.00	15165.0
257.10	1226.0
258.00	5713.0
259.00	759.0
260.90	318.0
264.90	2455.0
273.00	3328.0
274.00	7897.0
275.00	42200.0
276.00	5728.0
277.00	3367.0
277.90	835.0
283.00	478.0
283.90	365.0
285.00	637.0
293.00	1066.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

295.00	315.0
296.00	12864.0
297.00	1964.0
303.00	1575.0
304.00	471.0
313.90	533.0
315.00	1599.0
316.00	840.0
320.90	339.0
323.10	3618.0
324.10	740.0
327.00	915.0
328.00	453.0
332.00	302.0
332.90	484.0
334.10	2339.0
335.10	776.0
340.90	483.0
346.10	732.0
352.00	944.0
353.00	877.0
354.00	1457.0
365.00	5417.0
365.90	616.0
371.00	313.0
372.00	1925.0
373.10	484.0
383.00	499.0
390.10	391.0
402.00	883.0
403.10	1205.0
403.90	564.0
421.00	924.0
422.00	678.0
423.00	6614.0
424.00	1586.0
441.00	20752.0
442.10	130752.0
443.10	26104.0
444.00	2017.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

m/z	Abundance
38.00	776.0
39.00	3649.0
40.00	846.0
44.00	1433.0
49.00	922.0
50.00	13352.0
51.00	53688.0
52.10	2721.0
55.00	351.0
56.00	1418.0
57.00	3386.0
61.00	881.0
61.90	590.0
63.00	1775.0
65.00	1078.0
67.90	751.0
69.00	52064.0
73.00	601.0
74.00	5363.0
75.00	8719.0
76.00	2849.0
77.10	60160.0
78.00	4024.0
79.00	3776.0
79.90	3068.0
81.00	4207.0
82.00	1293.0
83.00	866.0
83.80	325.0
85.00	884.0
86.00	1294.0
87.00	631.0
91.00	907.0
92.00	1032.0
93.00	6695.0
93.90	559.0
96.10	397.0
98.00	5114.0
99.00	4820.0
100.90	2554.0
102.90	678.0
104.00	1321.0
104.90	1359.0
106.10	423.0
107.00	20376.0
108.00	2849.0
109.00	493.0
110.00	35448.0
111.00	5466.0
112.00	636.0
116.00	871.0
117.00	15947.0
118.00	1361.0
122.00	1229.0
123.00	1837.0
124.00	876.0
125.00	773.0
127.00	65688.0
128.00	4618.0
129.00	25264.0
130.00	2252.0
131.00	436.0
134.00	730.0
134.90	2116.0
136.00	862.0
137.00	1465.0
139.80	339.0
141.00	3031.0
142.10	1078.0
143.00	519.0
146.00	651.0
147.00	1836.0
148.00	4251.0
149.00	1243.0
151.10	474.0
151.90	422.0
153.00	1045.0
154.00	792.0
155.00	1806.0
156.00	2430.0
156.90	664.0
157.90	544.0
159.10	455.0
160.00	742.0
161.00	1530.0
161.90	469.0
165.00	1091.0
165.90	1022.0
167.00	7750.0
168.00	4446.0
168.90	501.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

171.00	381.0
172.00	632.0
173.00	800.0
174.00	1764.0
175.10	2338.0
176.00	572.0
176.90	1176.0
177.90	442.0
179.00	5683.0
180.00	4170.0
181.00	1765.0
183.90	368.0
185.00	2425.0
186.00	19248.0
187.00	5456.0
187.90	691.0
189.00	1467.0
191.00	556.0
192.00	1680.0
193.00	1941.0
194.00	688.0
196.00	3612.0
196.70	788.0
198.00	146432.0
198.90	9607.0
199.90	646.0
201.80	677.0
203.00	1114.0
204.00	5710.0
205.00	9786.0
206.10	37888.0
207.10	5653.0
208.00	1398.0
209.00	525.0
210.30	662.0
211.00	1333.0
214.90	355.0
215.90	559.0
217.00	11128.0
218.00	1137.0
221.00	4566.0
222.00	1150.0
223.00	1927.0
224.00	21744.0
225.00	5078.0
226.00	634.0
227.00	9410.0
228.00	1492.0
229.00	1973.0
231.00	796.0
234.00	698.0
234.90	572.0
236.00	310.0
237.00	965.0
240.00	351.0
240.90	381.0
242.00	884.0
243.00	1194.0
244.00	16760.0
245.00	2222.0
246.00	2985.0
247.00	614.0
248.90	675.0
253.00	307.0
254.10	652.0
255.00	87664.0
256.00	12337.0
256.90	869.0
258.00	5224.0
259.00	895.0
265.00	2239.0
273.00	2788.0
274.00	7487.0
275.00	40208.0
276.10	4551.0
277.00	3630.0
278.00	451.0
283.10	477.0
285.00	812.0
293.00	578.0
294.00	315.0
296.00	11289.0
297.00	1679.0
303.00	1435.0
314.00	629.0
315.00	941.0
315.80	521.0
323.00	4106.0
324.10	740.0
326.90	605.0
333.10	359.0
334.00	2520.0
335.00	718.0
341.00	340.0
346.00	629.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

352.00	940.0
353.00	841.0
354.00	1106.0
365.00	4744.0
365.90	653.0
371.00	336.0
372.00	1942.0
373.00	505.0
383.00	656.0
390.00	399.0
402.00	839.0
403.00	1109.0
403.90	422.0
421.00	819.0
422.00	1141.0
423.10	6680.0
424.10	1631.0
441.10	20920.0
442.10	142464.0
443.10	26176.0
444.00	2263.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

Scan 2522 (17.421 min): BM006718.D
DFTPP60

m/z	Abundance
39.90	850.0
44.00	1345.0
73.00	391.0
83.90	369.0
207.00	1222.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60