
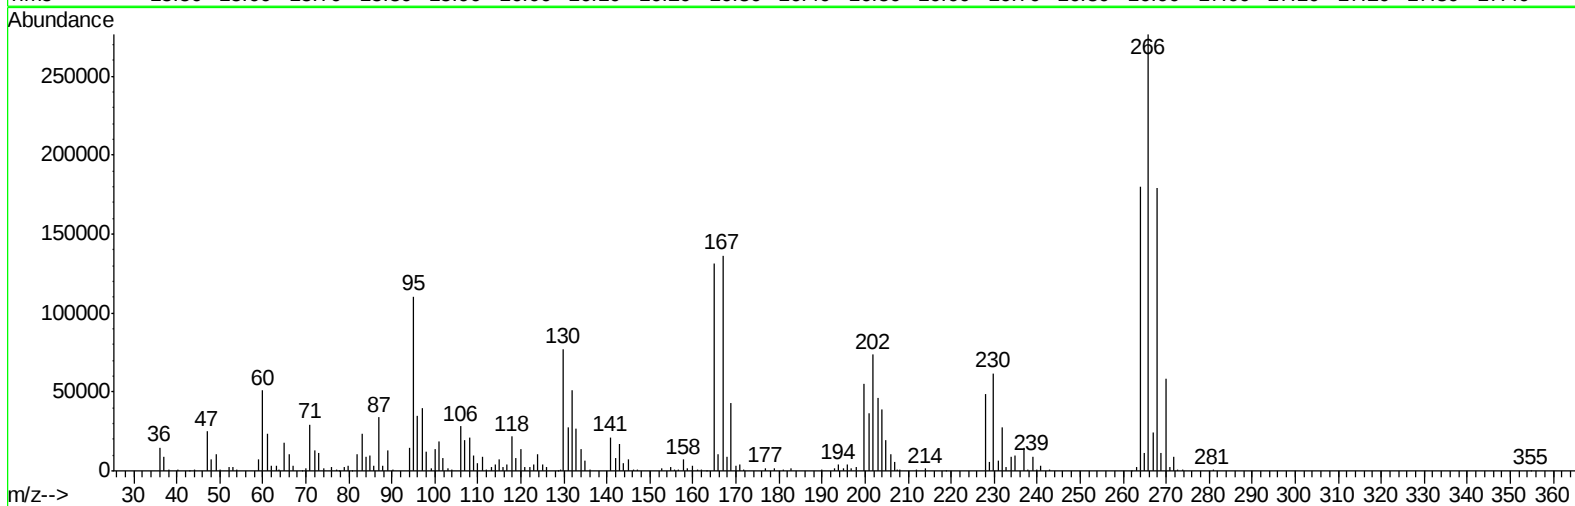


Data Path : Z:\HPCHEM1\BNA M\DATA\BM072817\
Data File : BM011031.D
Acq On : 28 Jul 2017 08:24
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 04:38:23 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 17:29:06 2017
Response via : Initial Calibration

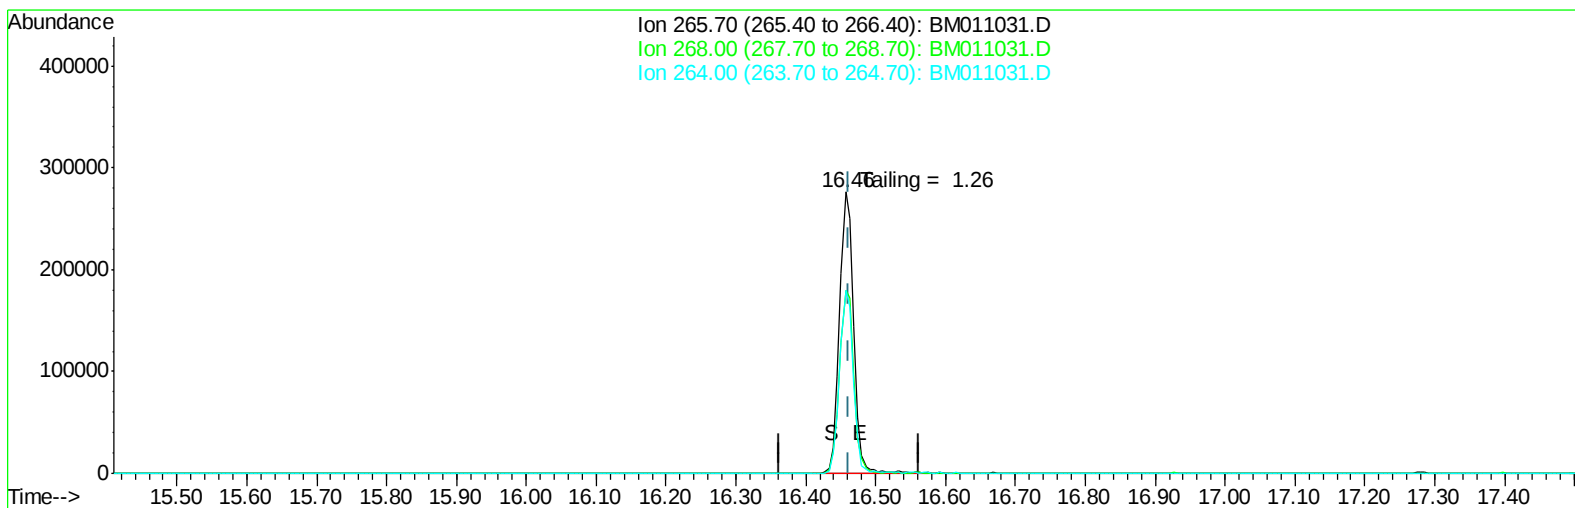

TIC: BM011031.D

(69) Pentachlorophenol (C)



16.457min (-0.006) 77068.08ng

response 382391

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	64.79
264.00	61.20	65.02
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM072817\
Data File : BM011031.D
Acq On : 28 Jul 2017 08:24
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 04:38:23 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 17:29:06 2017
Response via : Initial Calibration

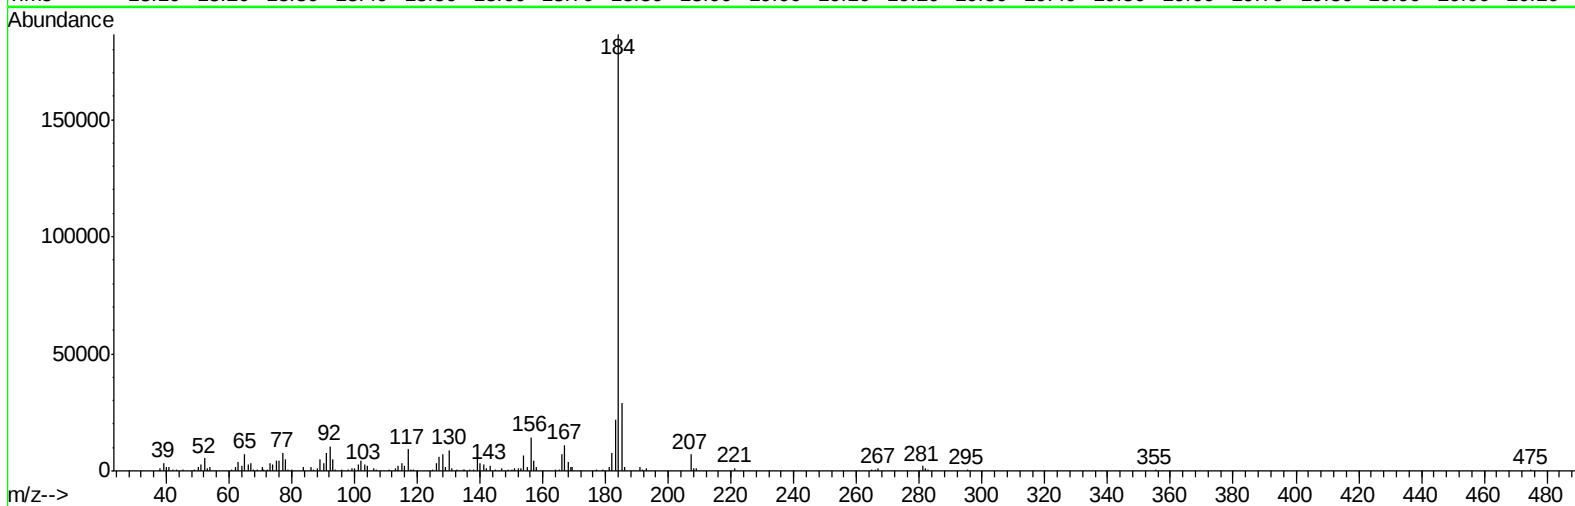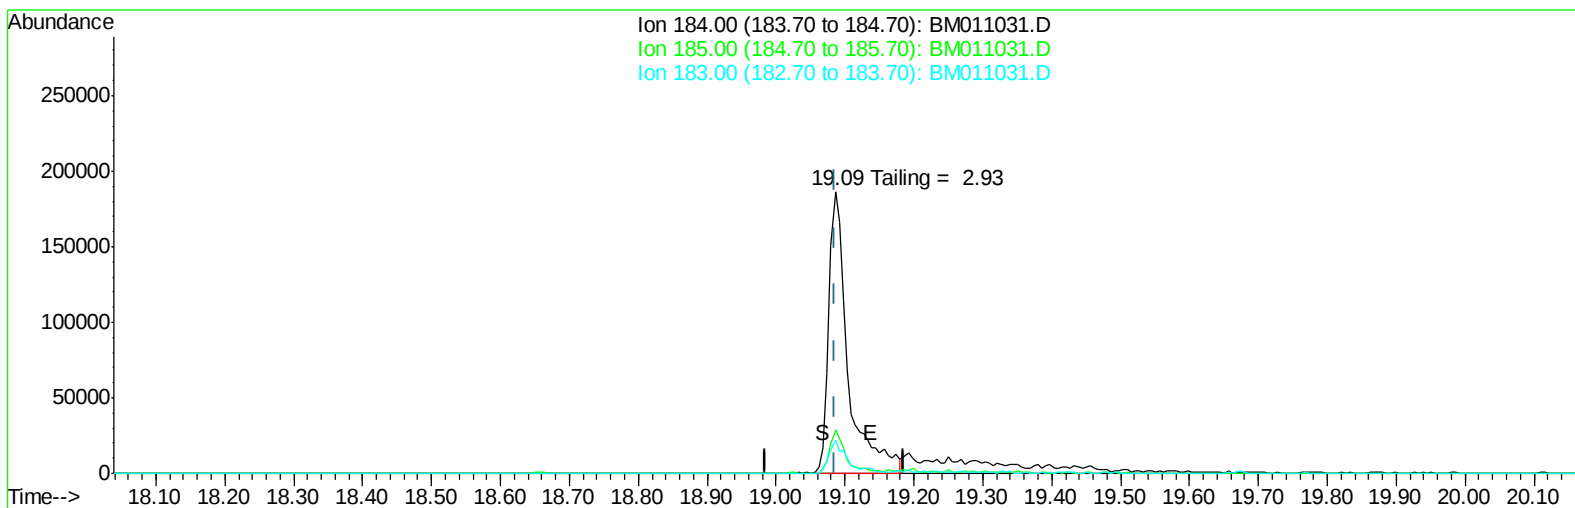

TIC: BM011031.D

(76) Benzidine

19.086min (-0.000) 2218.80ng

response 351760

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	15.41
183.00	11.10	11.85
0.00	0.00	0.00