

Data Path : Z:\HPCHEM1\BNA M\DATA\BM072817\
 Data File : BM011044.D
 Acq On : 28 Jul 2017 16:30
 Operator : SJ/JU
 Sample : I4432-09
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MW-4

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.022	373	380	390	rBV	738602	1034353	10.67%	2.181%
2	6.575	637	644	656	rBV	451293	774335	7.99%	1.633%
3	6.922	697	703	713	rBV	1319273	1993440	20.57%	4.203%
4	7.387	774	782	790	rBV	977109	1522337	15.70%	3.210%
5	7.699	828	835	843	rVB	1611511	2498865	25.78%	5.269%
6	8.528	969	976	989	rBV	1501563	2358061	24.33%	4.972%
7	10.145	1242	1251	1259	rBV	1253724	2068361	21.34%	4.361%
8	12.651	1670	1677	1684	rBV	3822469	5474353	56.48%	11.543%
9	13.516	1817	1824	1830	rBV	125369	177132	1.83%	0.373%
10	14.045	1907	1914	1922	rBV2	1929771	3011931	31.07%	6.351%
11	15.545	2162	2169	2179	rBV	2731631	3743433	38.62%	7.893%
12	16.657	2352	2358	2363	rBV2	228682	316186	3.26%	0.667%
13	16.798	2376	2382	2389	rBV2	2879128	4014805	41.42%	8.465%
14	17.727	2535	2540	2548	rBV3	173010	273280	2.82%	0.576%
15	19.027	2756	2761	2768	rBV5	164281	226108	2.33%	0.477%
16	19.462	2829	2835	2842	rBV	8089808	9693358	100.00%	20.439%
17	21.021	3095	3100	3106	rBV	3974444	4638139	47.85%	9.780%
18	23.133	3453	3459	3469	rVB	2060368	3608473	37.23%	7.608%


Sum of corrected areas: 47426950

Data Path : Z:\HPCHEM1\BNA M\DATA\BM072817\
Data File : BM011044.D
Acq On : 28 Jul 2017 16:30
Operator : SJ/JU
Sample : I4432-09
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MW-4

Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

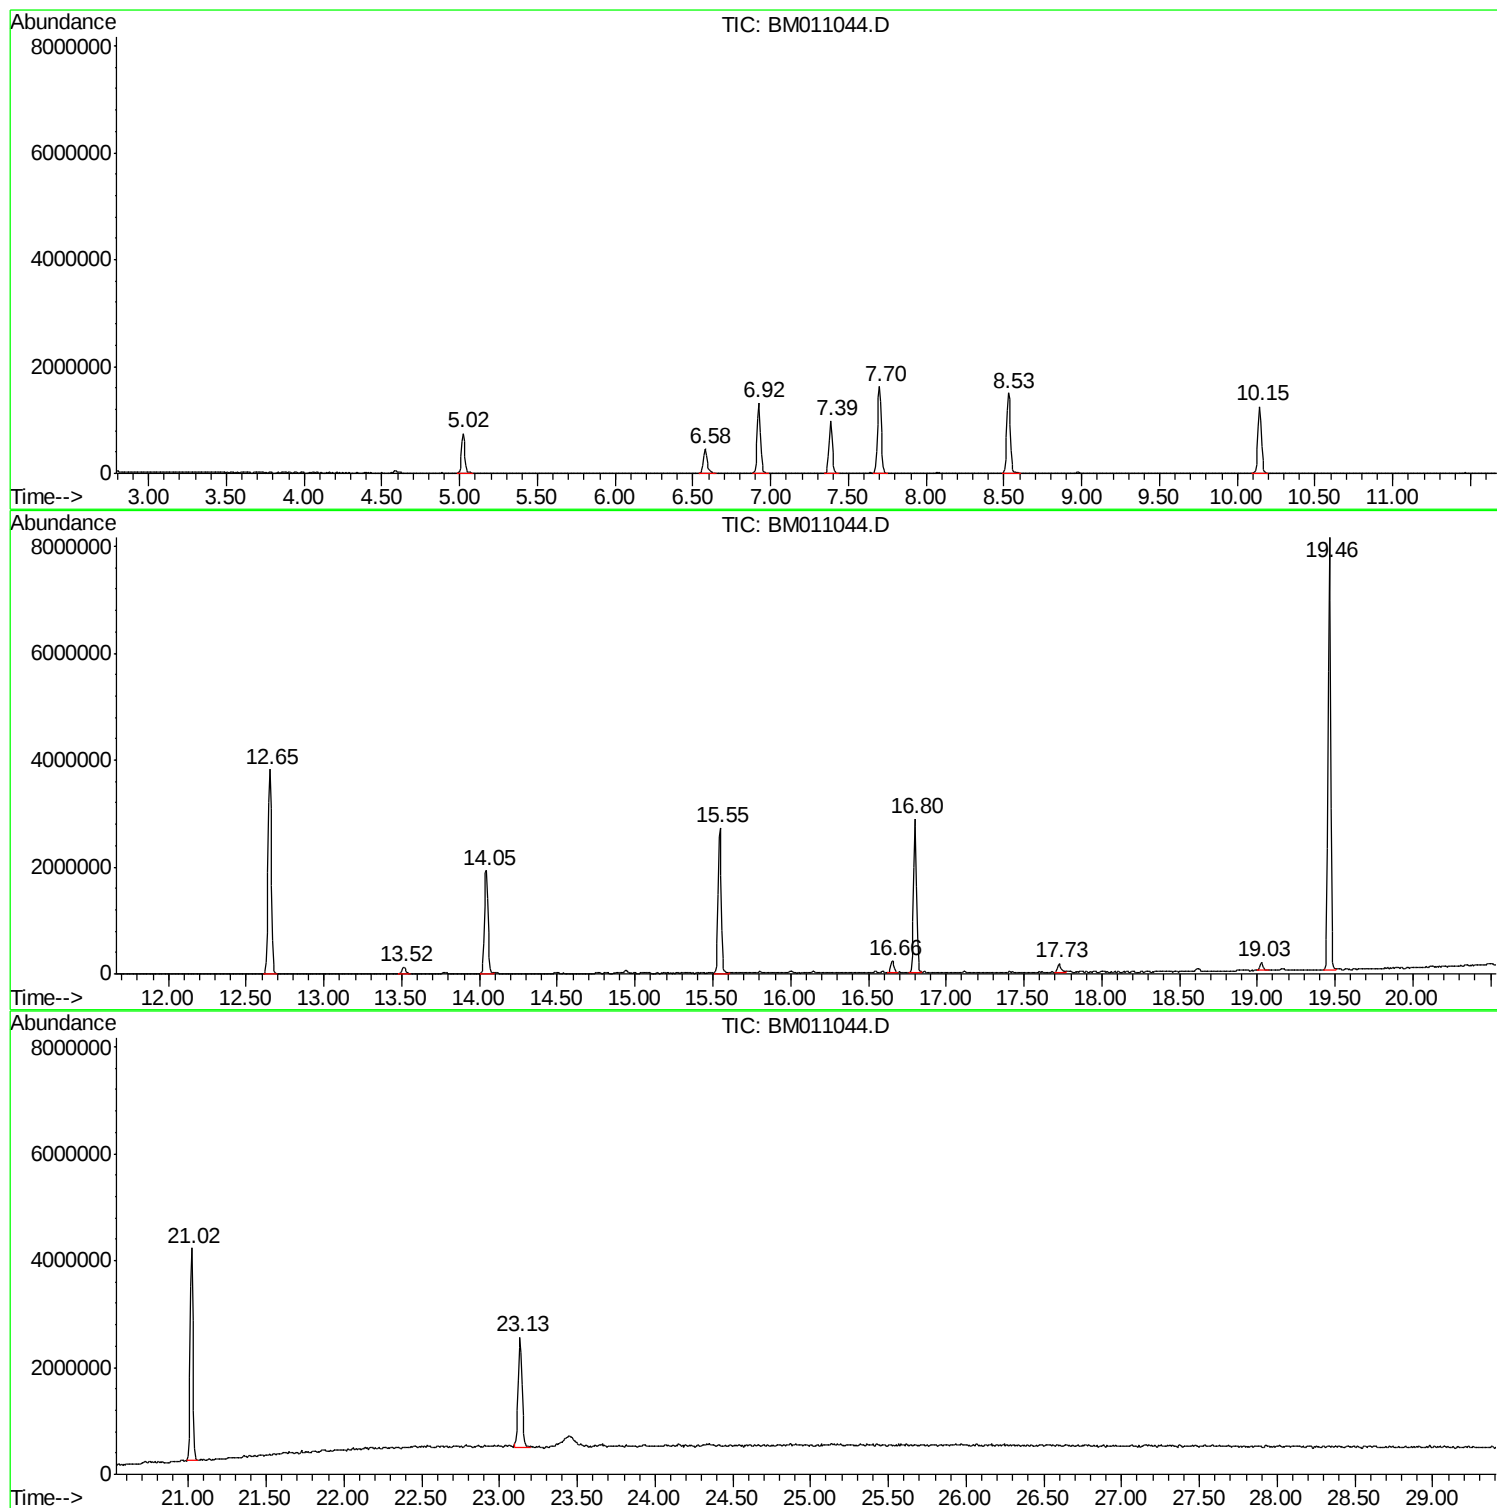

Data Path : Z:\HPCHEM1\BNA M\DATA\BM072817\
Data File : BM011044.D
Acq On : 28 Jul 2017 16:30
Operator : SJ/JU
Sample : I4432-09
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MW-4










Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.92 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.92	26.19 ng	1993440	1,4-Dichlorobenzene-d4	7.39

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Silane, bicvclo[2.2.1]hept-5-en-...	226	C7H9Cl3Si	014319-64-3	35
2		1-Penten-3-yne	66	C5H6	000646-05-9	35
3		2,4-Hexadienenitrile	93	C6H7N	001516-01-4	25
4		3-Penten-1-yne, (E)-	66	C5H6	002004-69-5	25
5		Bicyclo[2.2.1]hept-5-ene-2-aceti...	180	C11H16O2	074876-17-8	25

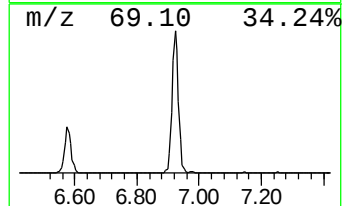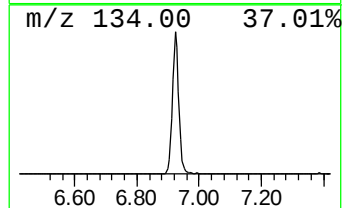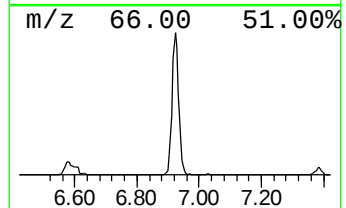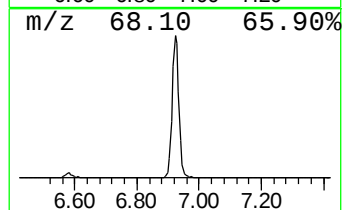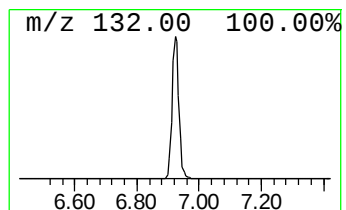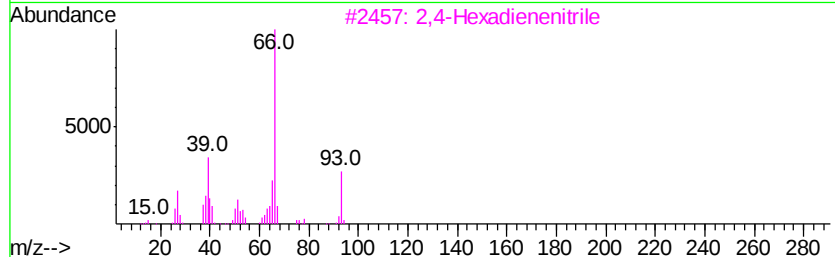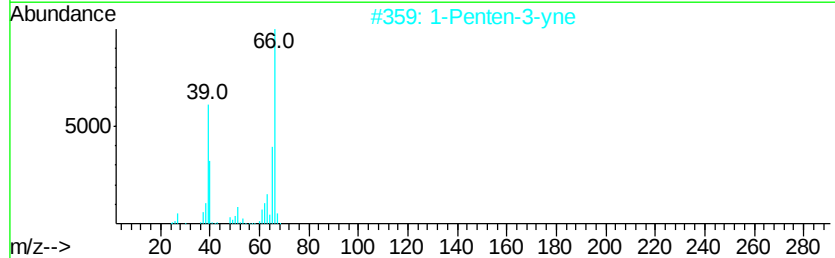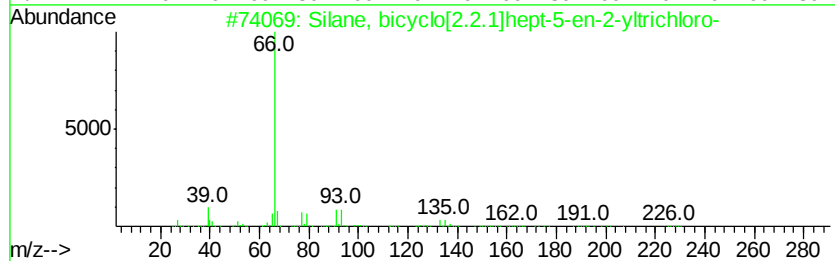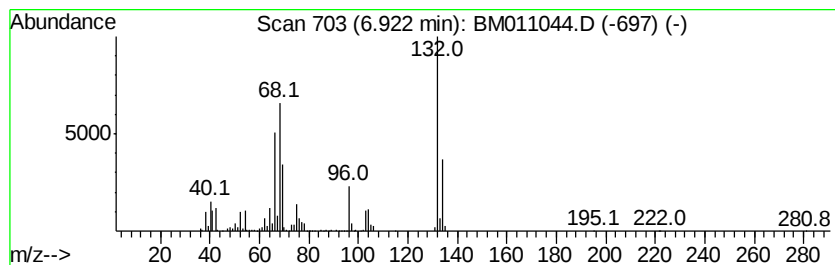

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072817\
Data File : BM011044.D
Acq On : 28 Jul 2017 16:30
Operator : SJ/JU
Sample : I4432-09
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MW-4

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.92	6.92	26.2	ng	1993440	1	7.39	1522340	20.0