




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072919\
 Data File : BM021714.D
 Acq On : 30 Jul 2019 03:40
 Operator : HP/JU
 Sample : K3863-13
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52F3

Manual Integrations
 APPROVED

mohammad
 7/30/2019 4:51:47 PM

Quant Time: Jul 30 04:44:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 26 18:42:09 2019
 Response via : Initial Calibration

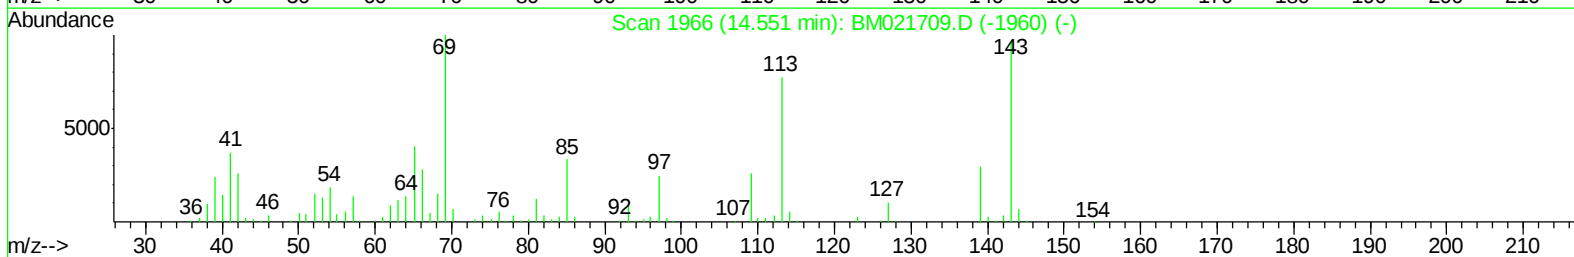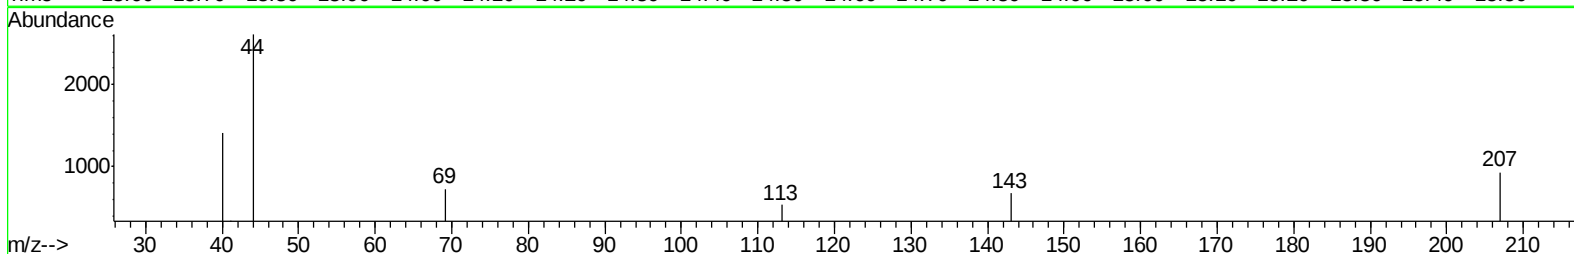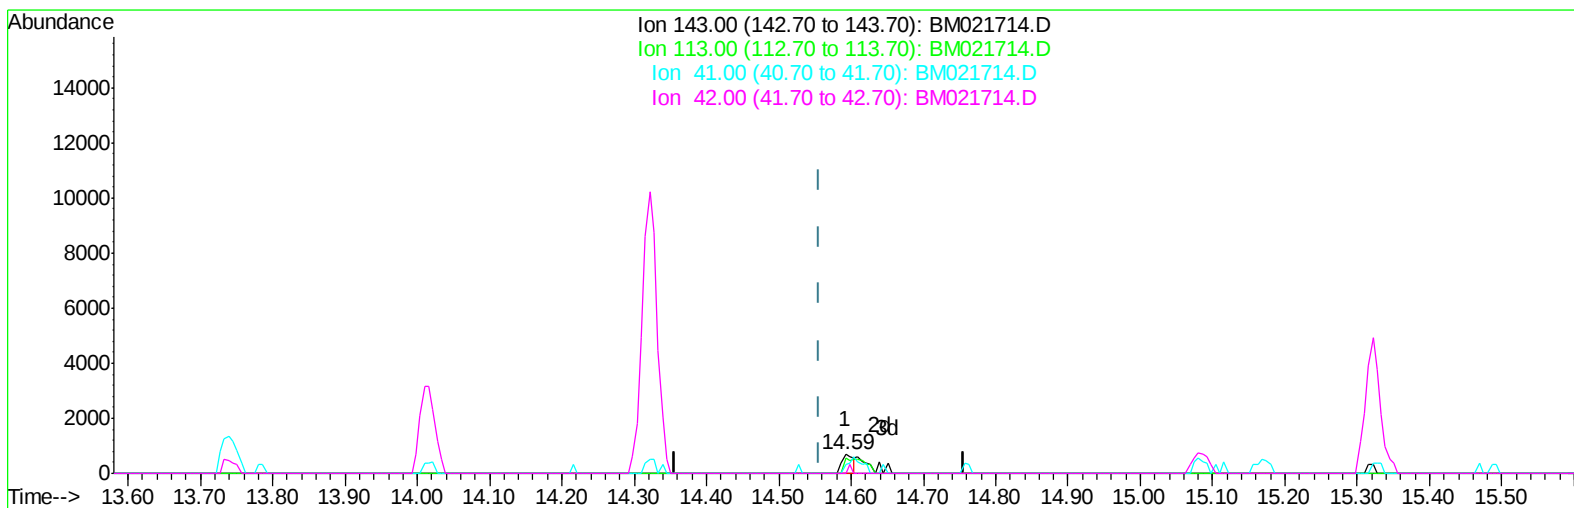

TIC: BM021714.D

(51) 4-Nitrophenol-d4 (S)
 14.592min (+0.035) 0.14ng/ul

response 781

Ion	Exp%	Act%
143.00	100	100
113.00	78.90	79.06
41.00	40.00	49.41#
42.00	27.20	0.00#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072919\
Data File : BM021714.D
Acq On : 30 Jul 2019 03:40
Operator : HP/JU
Sample : K3863-13
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52F3

Quant Time: Jul 30 04:44:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 26 18:42:09 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
7/30/2019 4:51:47 PM

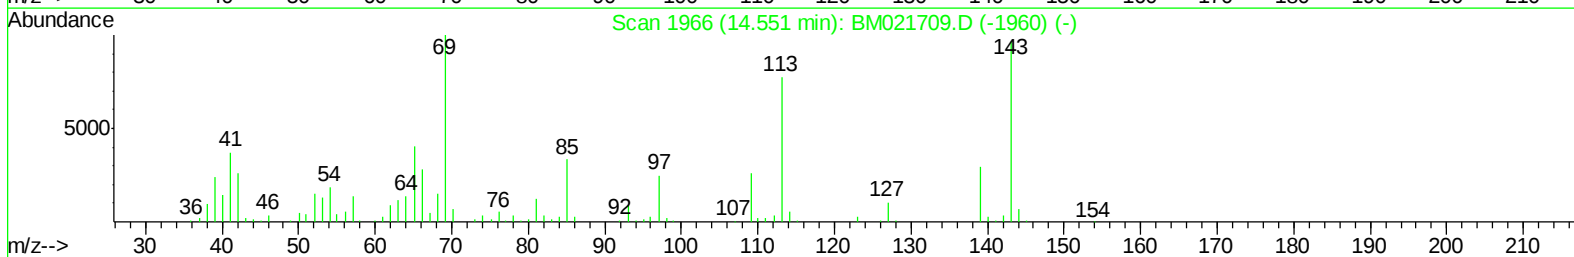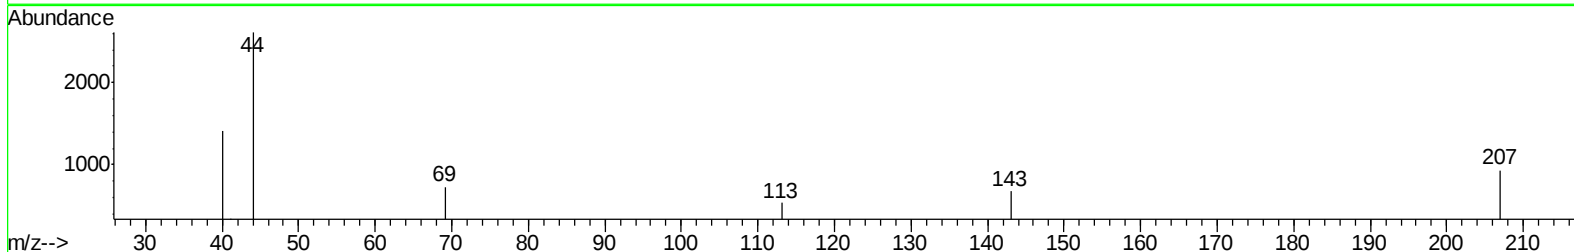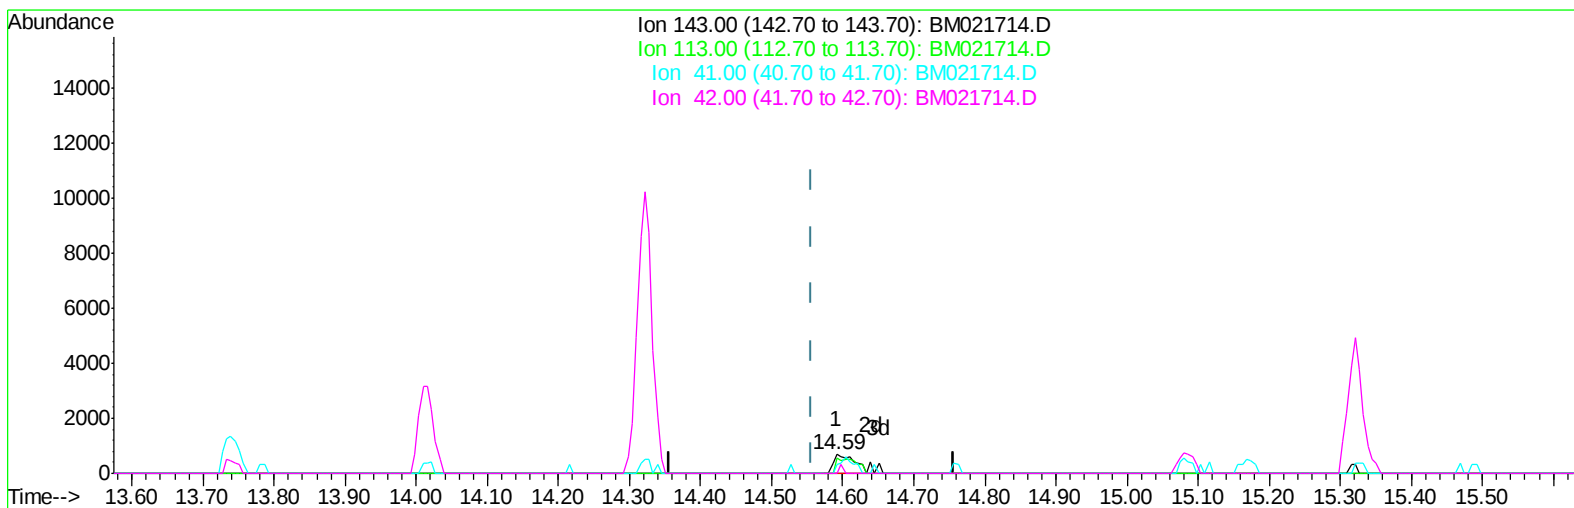

TIC: BM021714.D

(51) 4-Nitrophenol-d4 (S)

14.592min (+0.035) 0.26ng/ul m

response 1385

Ion	Exp%	Act%
143.00	100	100
113.00	78.90	79.06
41.00	40.00	49.41#
42.00	27.20	0.00#