

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072919\
 Data File : BM021703.D
 Acq On : 29 Jul 2019 19:47
 Operator : HP/JU
 Sample : K3863-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52F7

Quant Time: Jul 30 04:42:50 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 26 18:42:09 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	153024	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	642257	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	428084	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.08	188	913937	20.00	ng/ul	0.00
77) Chrysene-d12	21.27	240	686632	20.00	ng/ul	0.00
85) Perylene-d12	23.51	264	708604	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	11345	3.57	ng/uL	0.00
5) Phenol-d5	6.86	99	225111	19.55	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	137090	20.80	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	193129	20.22	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	179447	18.58	ng/ul	0.00
19) Nitrobenzene-d5	8.85	128	97431	20.29	ng/ul	0.00
22) 2-Nitrophenol-d4	9.56	143	106971	20.22	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	223932	19.77	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	254106	23.72	ng/ul	0.00
43) Dimethylphthalate-d6	13.75	166	764559	23.14	ng/ul	0.00
46) Acenaphthylene-d8	14.02	160	859868	21.90	ng/ul	0.00
51) 4-Nitrophenol-d4	14.56	143	48027	9.58	ng/ul	0.00
57) Fluorene-d10	15.32	176	679246	23.43	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.46	200	49779	8.76	ng/ul	0.00
70) Anthracene-d10	17.17	188	1008263	21.92	ng/ul	0.00
78) Pyrene-d10	19.48	212	1071117	27.81	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.36	264	854432	22.79	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.79	163	220745	6.437	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072919\
Data File : BM021703.D
Acq On : 29 Jul 2019 19:47
Operator : HP/JU
Sample : K3863-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52F7

Quant Time: Jul 30 04:42:50 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 26 18:42:09 2019
Response via : Initial Calibration

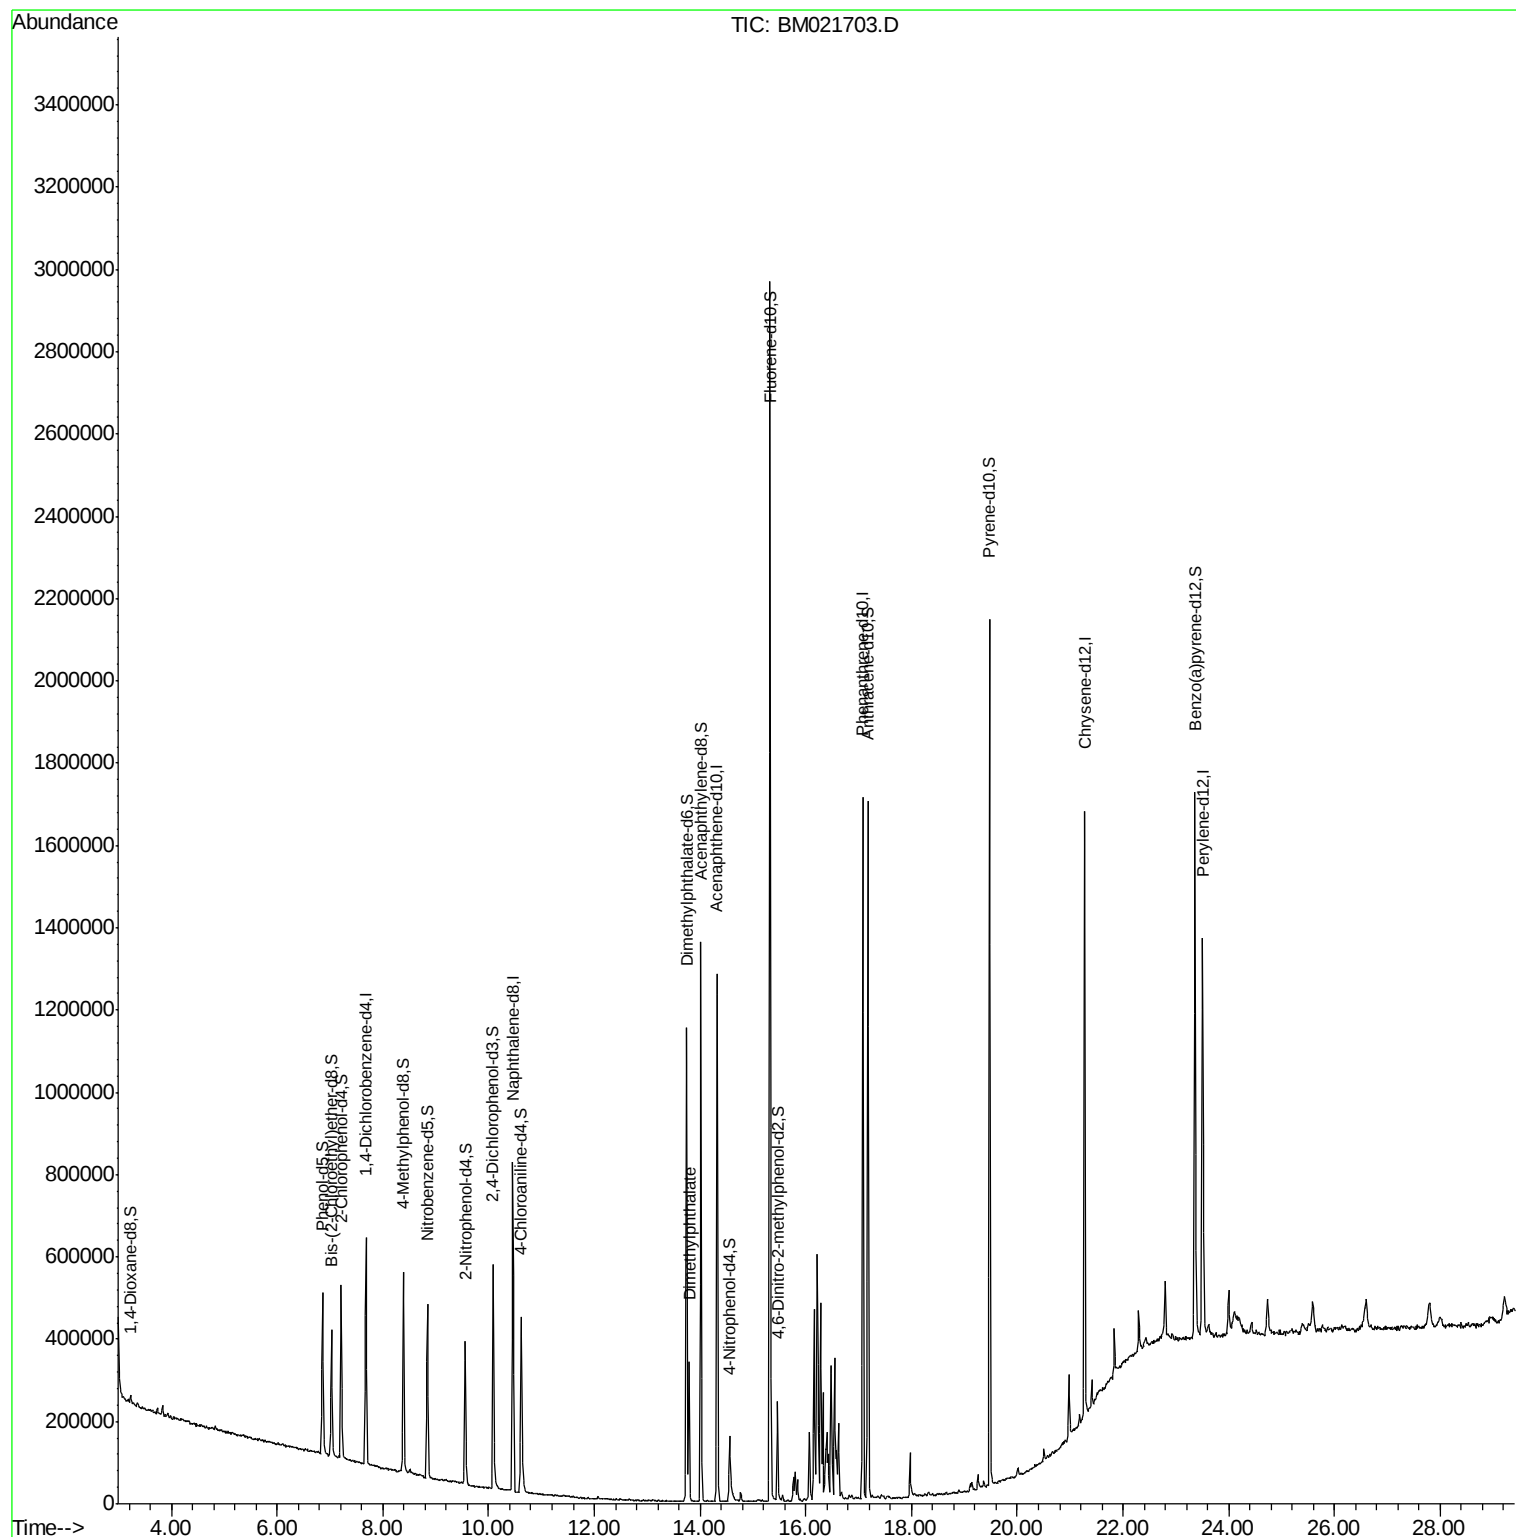

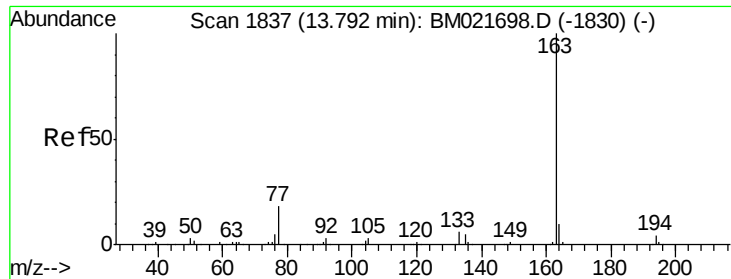

#44

Dimethylphthalate

Concen: 6.437 ng/ul

RT: 13.79 min Scan# 1837

Delta R.T. 0.00 min

Lab File: BM021703.D

Acq: 29 Jul 2019 19:47

Instrument :

BNA_M

ClientSampleId :

A52F7

Tot Ion:163 Resp: 220745

Ion Ratio Lower Upper

163 100

194 4.0 3.5 5.3

164 9.7 8.1 12.1

