

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072919\
 Data File : BM021704.D
 Acq On : 29 Jul 2019 20:24
 Operator : HP/JU
 Sample : K3863-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52F8

Quant Time: Jul 30 04:42:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 26 18:42:09 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	165465	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	685561	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.33	164	448656	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.08	188	918269	20.00	ng/ul	0.00
77) Chrysene-d12	21.27	240	689592	20.00	ng/ul	0.00
85) Perylene-d12	23.50	264	751553	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	15353	4.46	ng/uL	0.00
5) Phenol-d5	6.86	99	307812	24.73	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	183260	25.72	ng/ul	0.00
9) 2-Chlorophenol-d4	7.21	132	266041	25.76	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	270756	25.92	ng/ul	0.00
19) Nitrobenzene-d5	8.85	128	137272	26.77	ng/ul	0.00
22) 2-Nitrophenol-d4	9.56	143	150742	26.69	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	305092	25.23	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	357728	31.28	ng/ul	0.00
43) Dimethylphthalate-d6	13.74	166	967210	27.93	ng/ul	0.00
46) Acenaphthylene-d8	14.02	160	1127905	27.40	ng/ul	0.00
51) 4-Nitrophenol-d4	14.56	143	65957	12.55	ng/ul	0.00
57) Fluorene-d10	15.32	176	860449	28.33	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.47	200	68215	11.95	ng/ul	0.00
70) Anthracene-d10	17.18	188	1257671	27.22	ng/ul	0.00
78) Pyrene-d10	19.48	212	1252256	32.37	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.36	264	1102574	27.73	ng/ul	0.00


Target Compounds					Ovalue
44) Dimethylphthalate	13.79	163	235320	6.547	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072919\
Data File : BM021704.D
Acq On : 29 Jul 2019 20:24
Operator : HP/JU
Sample : K3863-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52F8

Quant Time: Jul 30 04:42:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 26 18:42:09 2019
Response via : Initial Calibration

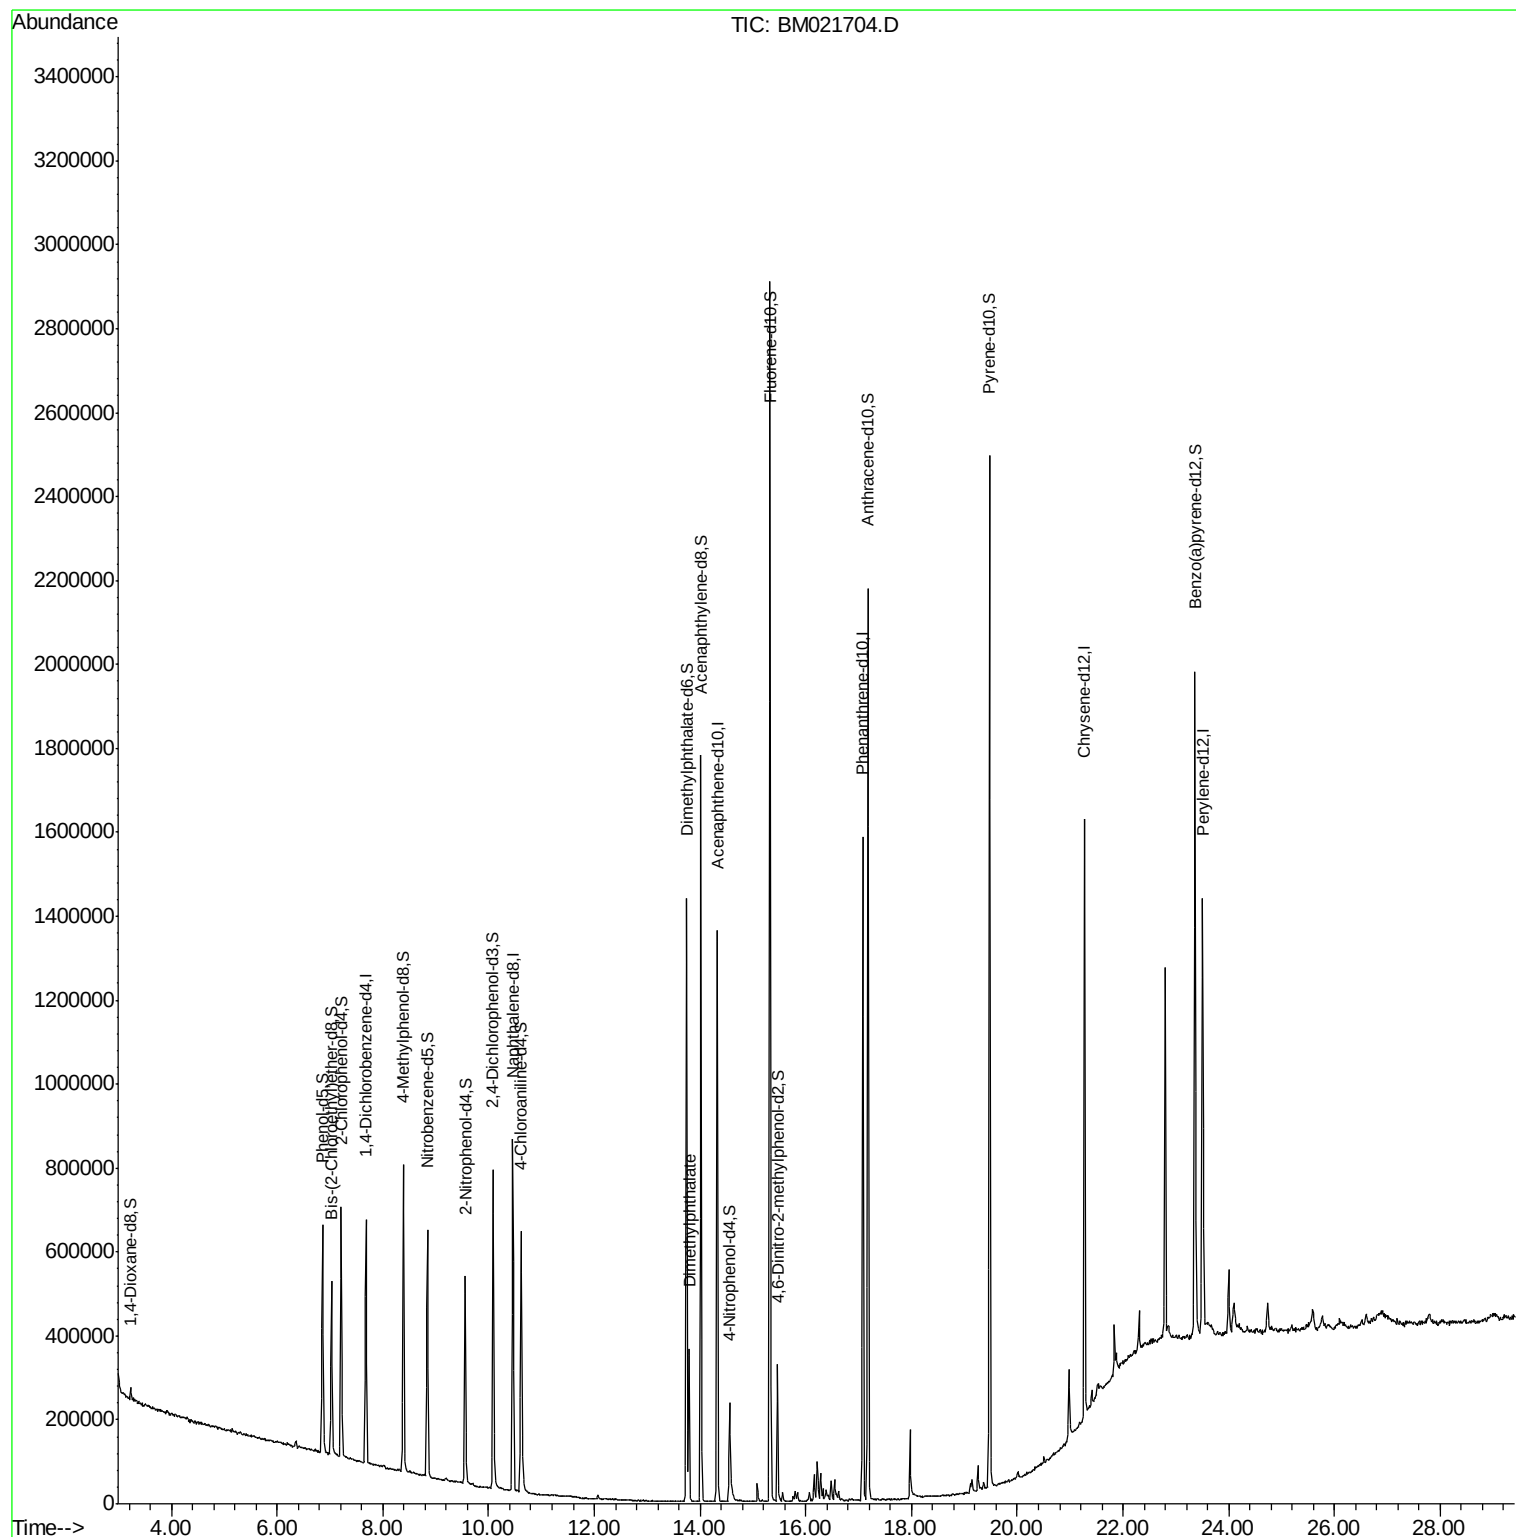

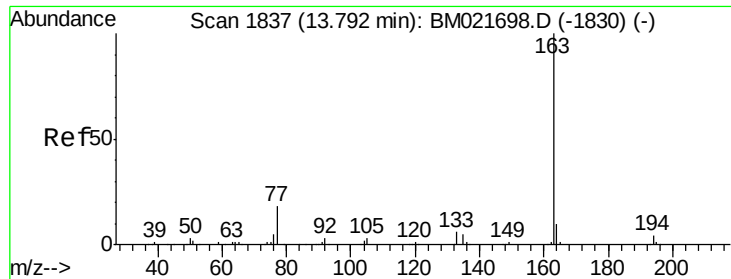

#44

Dimethylphthalate

Concen: 6.547 ng/ul

RT: 13.79 min Scan# 1837

Delta R.T. 0.00 min

Lab File: BM021704.D

Acq: 29 Jul 2019 20:24

Instrument :

BNA_M

ClientSampleId :

A52F8


Tot Ion:163 Resp: 235320

Ion Ratio Lower Upper

163 100

194 4.1 3.5 5.3

164 9.8 8.1 12.1

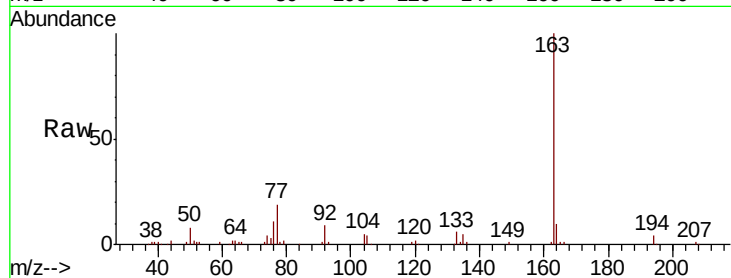

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

