

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072919\
 Data File : BM021707.D
 Acq On : 29 Jul 2019 22:13
 Operator : HP/JU
 Sample : K3863-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52G3

Quant Time: Jul 30 04:43:20 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 26 18:42:09 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	176482	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	739098	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	487886	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	1032476	20.00	ng/ul	0.00
77) Chrysene-d12	21.27	240	768621	20.00	ng/ul	0.00
85) Perylene-d12	23.50	264	790799	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	8330	2.27	ng/uL	0.00
5) Phenol-d5	6.86	99	170206	12.82	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	100725	13.25	ng/ul	0.00
9) 2-Chlorophenol-d4	7.21	132	144897	13.15	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	133908	12.02	ng/ul	0.00
19) Nitrobenzene-d5	8.85	128	72896	13.19	ng/ul	0.00
22) 2-Nitrophenol-d4	9.56	143	76463	12.56	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	162319	12.45	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	185356	15.03	ng/ul	0.00
43) Dimethylphthalate-d6	13.75	166	562585	14.94	ng/ul	0.00
46) Acenaphthylene-d8	14.02	160	631745	14.12	ng/ul	0.00
51) 4-Nitrophenol-d4	14.56	143	20135	3.52	ng/ul	0.00
57) Fluorene-d10	15.32	176	494729	14.98	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.47	200	27159	4.23	ng/ul	0.00
70) Anthracene-d10	17.17	188	739419	14.23	ng/ul	0.00
78) Pyrene-d10	19.47	212	782178	18.14	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.36	264	636473	15.21	ng/ul	0.00


Target Compounds				Ovalue	
44) Dimethylphthalate	13.79	163	160584	4.108	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072919\
Data File : BM021707.D
Acq On : 29 Jul 2019 22:13
Operator : HP/JU
Sample : K3863-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52G3

Quant Time: Jul 30 04:43:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 26 18:42:09 2019
Response via : Initial Calibration

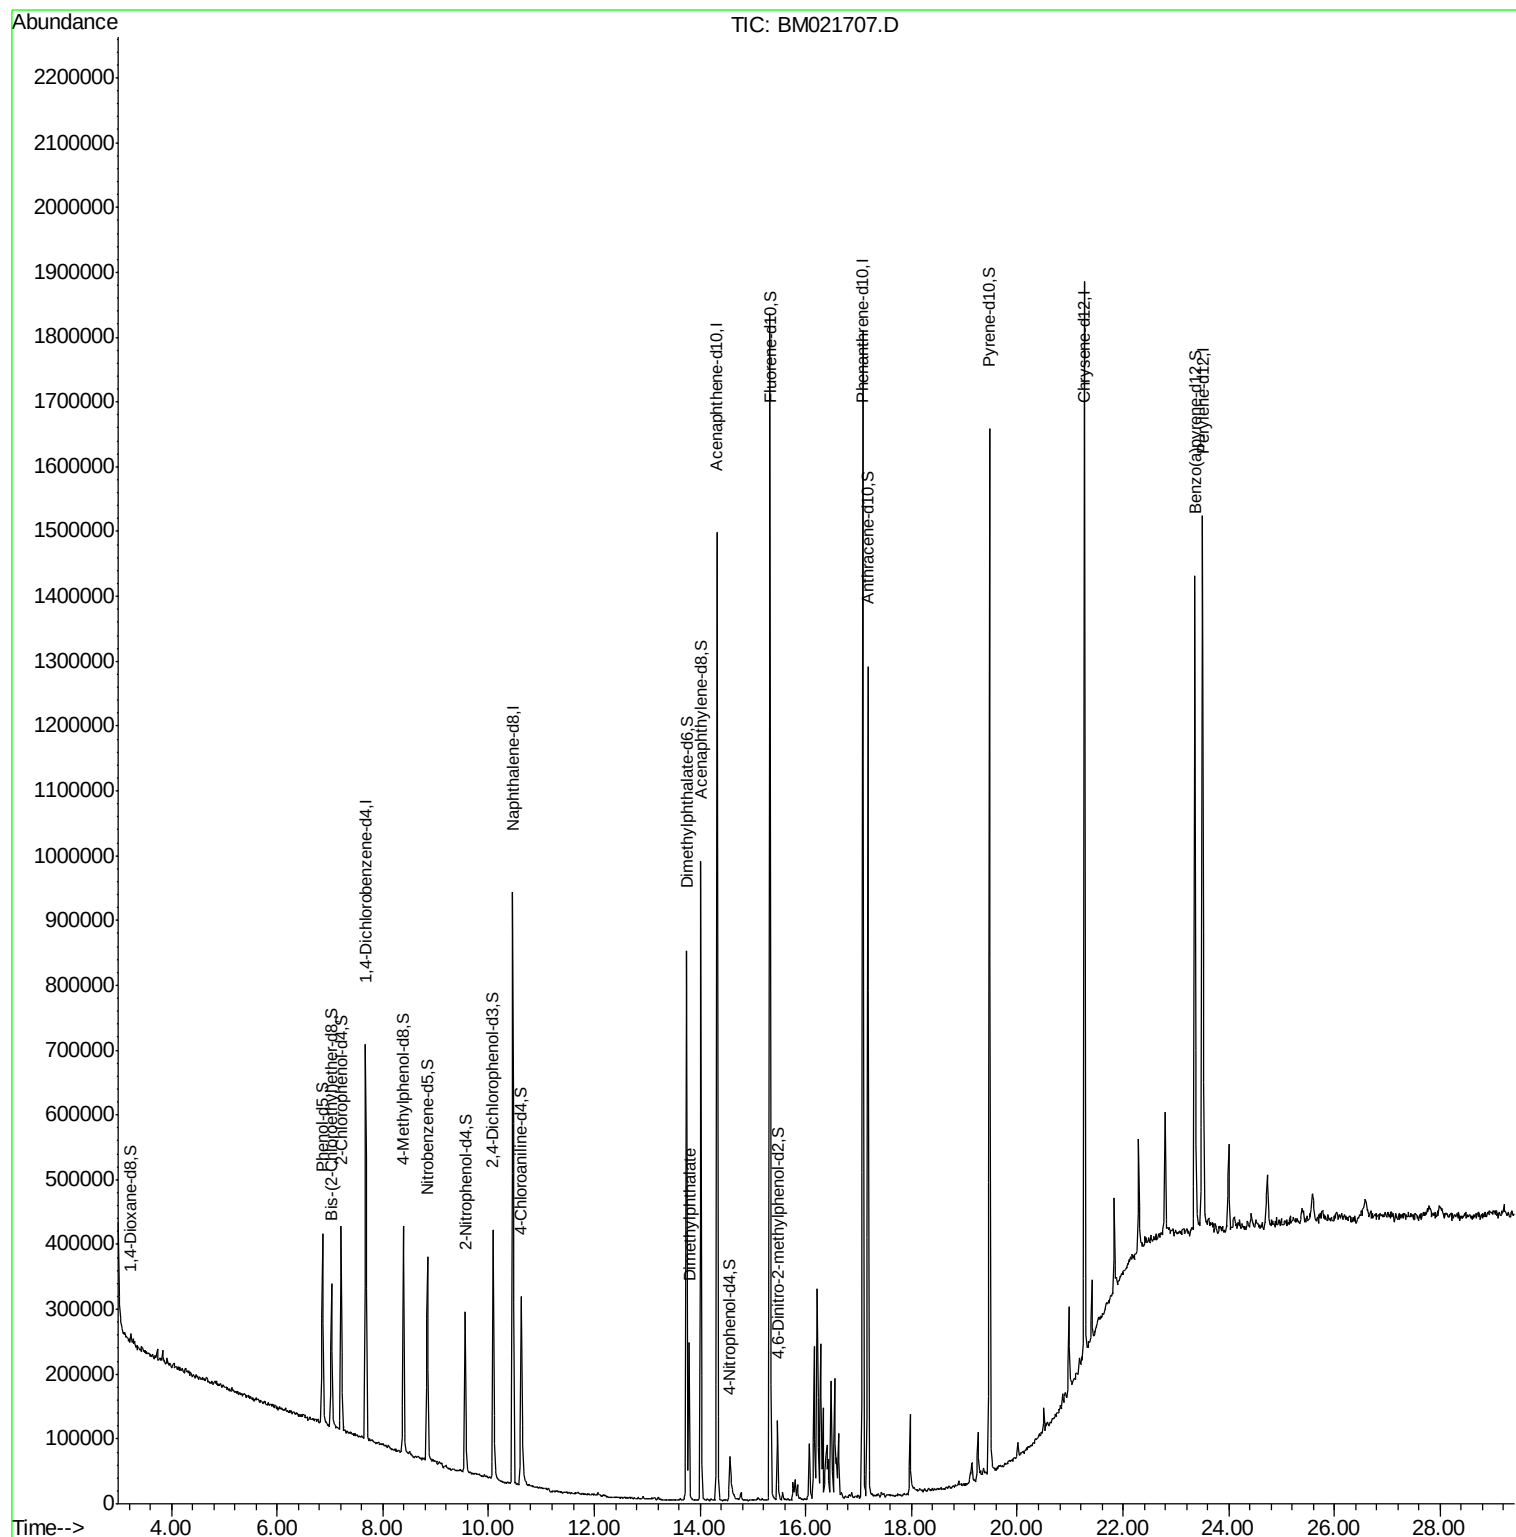

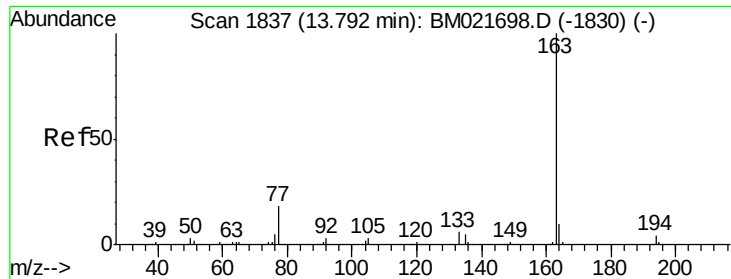

#44

Dimethylphthalate

Concen: 4.108 ng/ul

RT: 13.79 min Scan# 1837

Delta R.T. 0.00 min

Lab File: BM021707.D

Acq: 29 Jul 2019 22:13

Instrument :

BNA_M

ClientSampleId :

A52G3


Tot Ion:163 Resp: 160584

Ion Ratio Lower Upper

163 100

194 3.9 3.5 5.3

164 10.0 8.1 12.1

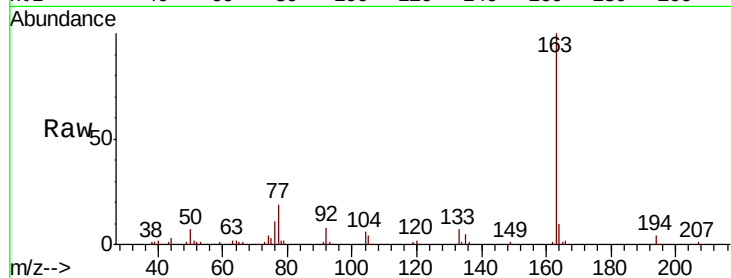

Abundance Ion 163.00 (162.70 to 163.70): E

150000 Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

