

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072919\
 Data File : BM021719.D
 Acq On : 30 Jul 2019 06:41
 Operator : HP/JU
 Sample : K3863-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52F6

Quant Time: Jul 30 07:18:52 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 30 05:24:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	182291	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	747331	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	497871	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	1048078	20.00	ng/ul	0.00
77) Chrysene-d12	21.27	240	816013	20.00	ng/ul	0.00
85) Perylene-d12	23.50	264	905992	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	17588	4.64	ng/uL	0.00
5) Phenol-d5	6.85	99	324194	23.64	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	193587	24.66	ng/ul	0.00
9) 2-Chlorophenol-d4	7.21	132	283892	24.95	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	271273	23.58	ng/ul	0.00
19) Nitrobenzene-d5	8.84	128	142665	25.53	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	155656	25.29	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	319480	24.24	ng/ul	0.00
29) 4-Chloroaniline-d4	10.61	131	337832	27.10	ng/ul	0.00
43) Dimethylphthalate-d6	13.74	166	1025313	26.68	ng/ul	0.00
46) Acenaphthylene-d8	14.02	160	1181406	25.87	ng/ul	0.00
51) 4-Nitrophenol-d4	14.56	143	66872	11.46	ng/ul	0.00
57) Fluorene-d10	15.32	176	904286	26.83	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.46	200	78130	11.99	ng/ul	0.00
70) Anthracene-d10	17.17	188	1362882	25.84	ng/ul	0.00
78) Pyrene-d10	19.47	212	1449022	31.65	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.36	264	1325451	27.65	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.79	163	259275	6.500	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072919\
Data File : BM021719.D
Acq On : 30 Jul 2019 06:41
Operator : HP/JU
Sample : K3863-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52F6

Quant Time: Jul 30 07:18:52 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 30 05:24:20 2019
Response via : Initial Calibration

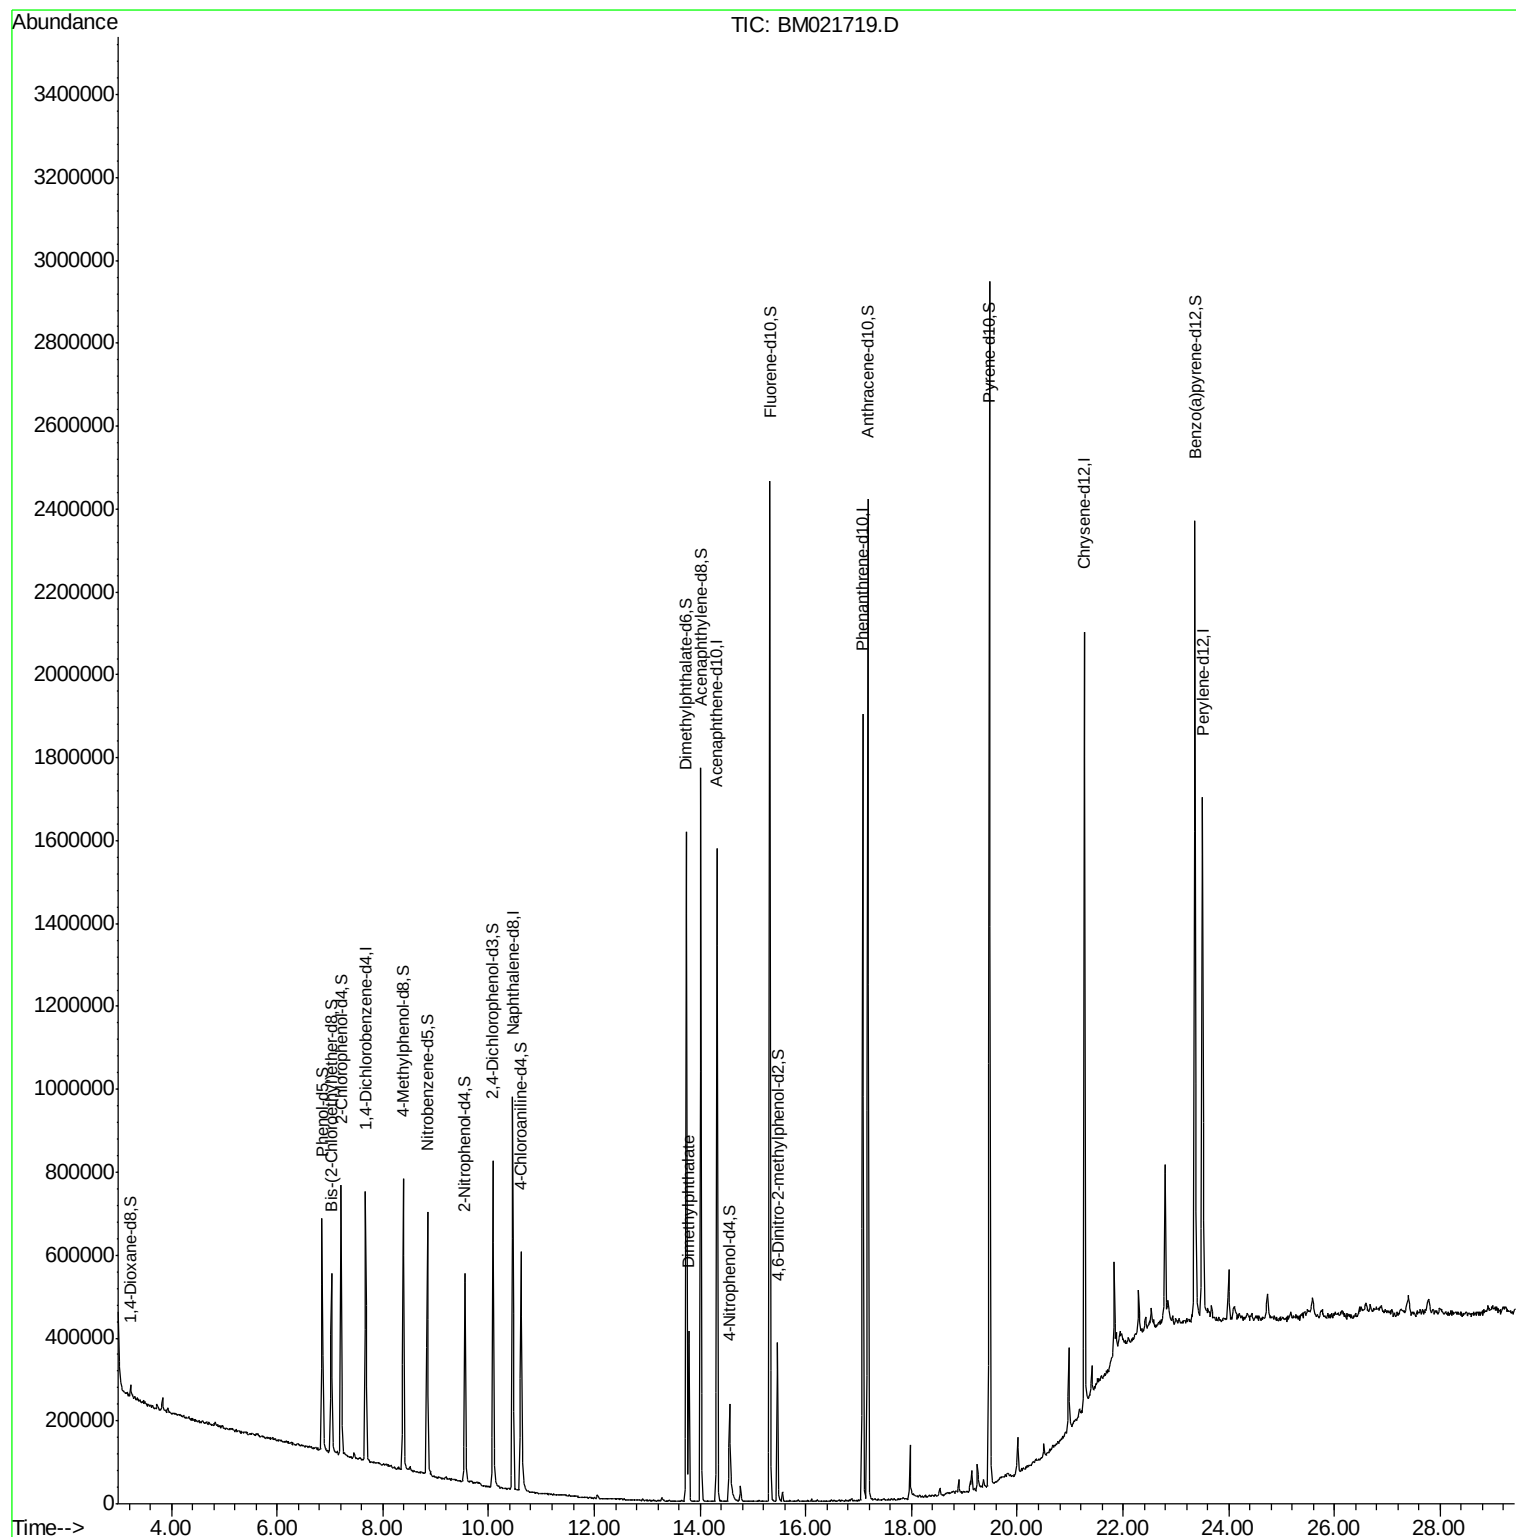

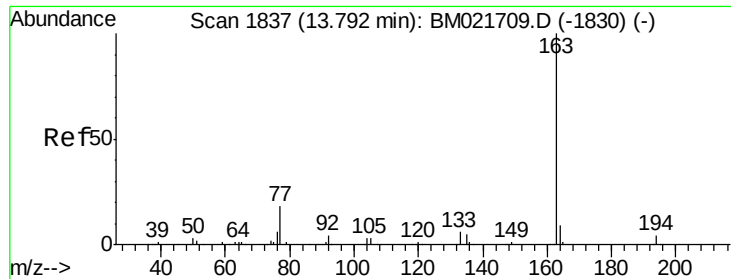

#44

Dimethylphthalate

Concen: 6.500 ng/ul

RT: 13.79 min Scan# 1836

Delta R.T. -0.01 min

Lab File: BM021719.D

Acq: 30 Jul 2019 06:41

Instrument :

BNA_M

ClientSampleId :

A52F6


Tot Ion:163 Resp: 259275

Ion Ratio Lower Upper

163 100

194 4.0 3.5 5.3

164 10.6 8.1 12.1

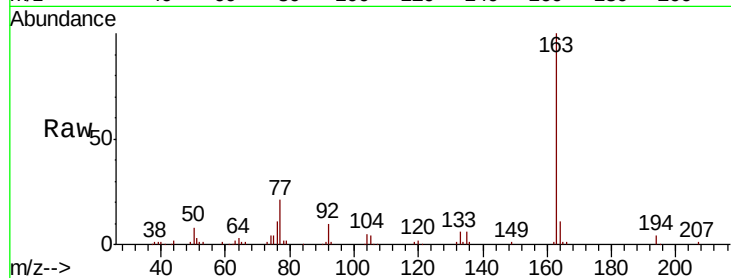

Abundance Ion 163.00 (162.70 to 163.70): E

250000 Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

