

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072919\
 Data File : BM021692.D
 Acq On : 29 Jul 2019 09:42
 Operator : HP/JU
 Sample : PB121643BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK43

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072619MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.858	653	658	669	rVB	570996	948016	23.11%	2.361%
2	7.028	682	687	704	rVB	452963	745580	18.18%	1.857%
3	7.216	713	719	729	rVB	649846	1036934	25.28%	2.583%
4	7.681	792	798	804	rBV	469547	737136	17.97%	1.836%
5	8.387	912	918	931	rVB	755844	1288445	31.42%	3.209%
6	8.846	990	996	1004	rBV	644139	1060455	25.86%	2.641%
7	9.557	1111	1117	1130	rVB	560101	935329	22.81%	2.330%
8	10.087	1201	1207	1221	rBV	816096	1456996	35.53%	3.629%
9	10.463	1264	1271	1281	rVB	691229	1136062	27.70%	2.830%
10	10.616	1290	1297	1314	rBV	759680	1410903	34.40%	3.514%
11	12.069	1539	1544	1552	rVB3	8724	17110	0.42%	0.043%
12	13.745	1822	1829	1842	rBV	1668147	2405936	58.66%	5.993%
13	14.016	1868	1875	1886	rBV	1900892	2866827	69.90%	7.141%
14	14.328	1921	1928	1937	rVB	1183503	1723146	42.01%	4.292%
15	14.557	1960	1967	1990	rBV	443163	862535	21.03%	2.148%
16	15.328	2091	2098	2108	rBV	2481944	3586511	87.45%	8.933%
17	15.469	2116	2122	2134	rBV	514581	775379	18.91%	1.931%
18	15.563	2134	2138	2143	rVB	23851	32519	0.79%	0.081%
19	16.110	2224	2231	2235	rVB3	7327	11054	0.27%	0.028%
20	16.869	2356	2360	2365	rBV3	4139	7568	0.18%	0.019%
21	17.080	2389	2396	2406	rBV2	1411060	2010166	49.01%	5.007%
22	17.180	2406	2413	2430	rVV	2798717	3867036	94.29%	9.632%
23	17.533	2468	2473	2477	rBV3	2002	4289	0.10%	0.011%
24	19.116	2738	2742	2745	rBV	22284	28859	0.70%	0.072%
25	19.369	2781	2785	2790	rBV	18559	26279	0.64%	0.065%
26	19.480	2798	2804	2817	rBV	3087140	4101321	100.00%	10.216%
27	21.274	3104	3109	3118	rBV	1374944	1826505	44.53%	4.549%
28	23.368	3458	3465	3481	rVB	1844106	3521912	85.87%	8.772%
29	23.509	3483	3489	3500	rVB	920346	1716849	41.86%	4.276%


Sum of corrected areas: 40147657

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072919\
Data File : BM021692.D
Acq On : 29 Jul 2019 09:42
Operator : HP/JU
Sample : PB121643BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK43

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

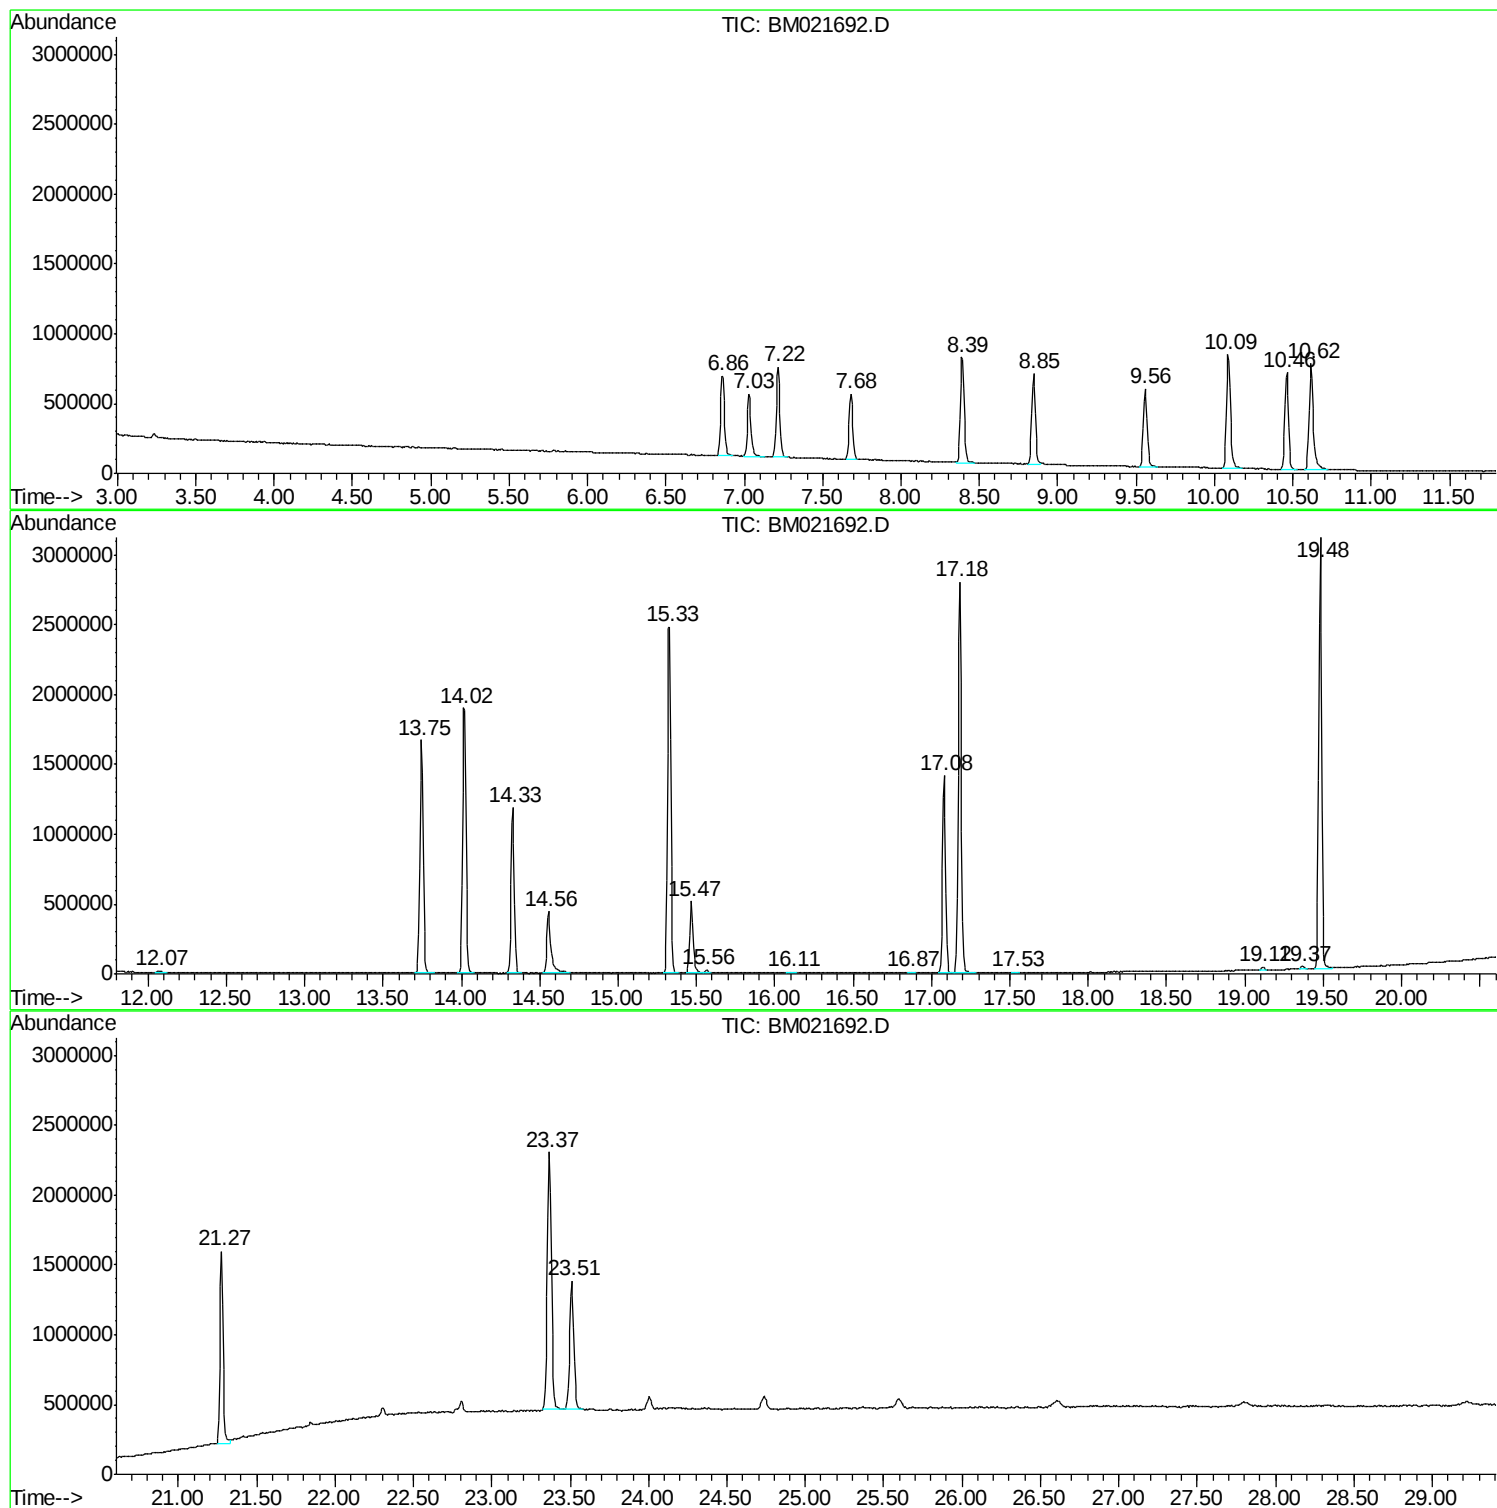

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM072919\
Data File : BM021692.D
Acq On : 29 Jul 2019 09:42
Operator : HP/JU
Sample : PB121643BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK43

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM072919\
Data File : BM021692.D
Acq On : 29 Jul 2019 09:42
Operator : HP/JU
Sample : PB121643BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK43

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc