

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072919\
 Data File : BM021710.D
 Acq On : 30 Jul 2019 01:14
 Operator : HP/JU
 Sample : K3863-12
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52F2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072619MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.857	653	658	667	rVB	309688	523652	15.55%	1.623%
2	7.028	682	687	696	rVB	230587	374180	11.11%	1.160%
3	7.210	713	718	726	rVB	338109	542669	16.12%	1.682%
4	7.675	792	797	804	rVB	621024	986728	29.31%	3.058%
5	8.386	912	918	927	rVB	373729	622700	18.50%	1.930%
6	8.839	990	995	1008	rVB	330538	564520	16.77%	1.750%
7	9.557	1111	1117	1127	rVB	265650	444047	13.19%	1.376%
8	10.086	1201	1207	1222	rBV	421285	788388	23.42%	2.443%
9	10.457	1263	1270	1282	rVB	903582	1510472	44.87%	4.681%
10	10.622	1291	1298	1315	rVB	222695	493368	14.66%	1.529%
11	12.074	1540	1545	1548	rVB	4345	6469	0.19%	0.020%
12	13.745	1822	1829	1833	rBV	798500	1161718	34.51%	3.601%
13	13.792	1833	1837	1847	rVB	150563	228881	6.80%	0.709%
14	14.016	1867	1875	1886	rBV	1037729	1513053	44.94%	4.689%
15	14.321	1921	1927	1936	rBV2	1499939	2163349	64.26%	6.705%
16	14.557	1961	1967	1989	rBV	156226	377121	11.20%	1.169%
17	14.768	1997	2003	2013	rVB4	30448	49319	1.46%	0.153%
18	15.321	2091	2097	2112	rBV	1405885	2006300	59.60%	6.218%
19	15.462	2115	2121	2134	rVV	215928	324896	9.65%	1.007%
20	15.562	2134	2138	2144	rVB	11231	13853	0.41%	0.043%
21	16.104	2227	2230	2233	rVB3	4017	4724	0.14%	0.015%
22	16.486	2291	2295	2297	rBV3	2423	3980	0.12%	0.012%
23	16.621	2314	2318	2321	rBV4	3122	4380	0.13%	0.014%
24	16.745	2335	2339	2344	rBV3	4122	6793	0.20%	0.021%
25	16.827	2349	2353	2356	rBV3	2292	4150	0.12%	0.013%
26	16.862	2356	2359	2363	rVV3	3585	6586	0.20%	0.020%
27	16.892	2363	2364	2367	rVB2	3642	3422	0.10%	0.011%
28	16.992	2376	2381	2384	rBV3	1886	3474	0.10%	0.011%
29	17.074	2389	2395	2400	rVV2	1756697	2493805	74.08%	7.729%
30	17.121	2400	2403	2407	rVV	170779	224863	6.68%	0.697%
31	17.174	2407	2412	2427	rVB2	1640513	2444553	72.61%	7.577%
32	17.462	2457	2461	2462	rBV3	3022	3430	0.10%	0.011%
33	17.498	2462	2467	2475	rVB2	16610	30721	0.91%	0.095%
34	17.668	2491	2496	2499	rBV5	4541	7311	0.22%	0.023%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072919\
 Data File : BM021710.D
 Acq On : 30 Jul 2019 01:14
 Operator : HP/JU
 Sample : K3863-12
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52F2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072619MA.M
 Title : SVOA CALIBRATION

35	17.845	2522	2526	2533	rBV7	8173	15452	0.46%	0.048%
36	17.915	2535	2538	2540	rVB4	3548	3684	0.11%	0.011%
37	17.968	2540	2547	2551	rBV2	115033	183003	5.44%	0.567%
38	18.003	2551	2553	2558	rVB	30595	37749	1.12%	0.117%
39	18.151	2574	2578	2582	rBV2	30637	46149	1.37%	0.143%
40	18.186	2582	2584	2589	rVB	10904	13166	0.39%	0.041%
41	18.315	2604	2606	2609	rBV4	3597	4293	0.13%	0.013%
42	18.462	2627	2631	2634	rBV	15589	20563	0.61%	0.064%
43	18.509	2635	2639	2648	rVB	42117	62381	1.85%	0.193%
44	18.750	2678	2680	2683	rVB3	5590	5544	0.16%	0.017%
45	18.874	2697	2701	2706	rBV3	10831	22229	0.66%	0.069%
46	19.139	2738	2746	2752	rBV	587607	782522	23.24%	2.425%
47	19.250	2762	2765	2770	rBV5	41396	64202	1.91%	0.199%
48	19.362	2781	2784	2786	rBV	19261	20891	0.62%	0.065%
49	19.474	2797	2803	2807	rBV	2310444	3366533	100.00%	10.434%
50	19.692	2837	2840	2845	rVB	15820	23374	0.69%	0.072%
51	19.821	2860	2862	2865	rBV3	15264	23250	0.69%	0.072%
52	20.003	2891	2893	2899	rVB2	46226	57576	1.71%	0.178%
53	20.103	2907	2910	2914	rBV2	24990	36249	1.08%	0.112%
54	21.268	3102	3108	3112	rBV	1786782	2515080	74.71%	7.795%
55	21.303	3112	3114	3121	rVB	239090	302562	8.99%	0.938%
56	23.362	3458	3464	3469	rBV	1413077	2455925	72.95%	7.612%
57	23.503	3482	3488	3502	rVB	1142700	2264612	67.27%	7.019%


Sum of corrected areas: 32264864

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072919\
Data File : BM021710.D
Acq On : 30 Jul 2019 01:14
Operator : HP/JU
Sample : K3863-12
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52F2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

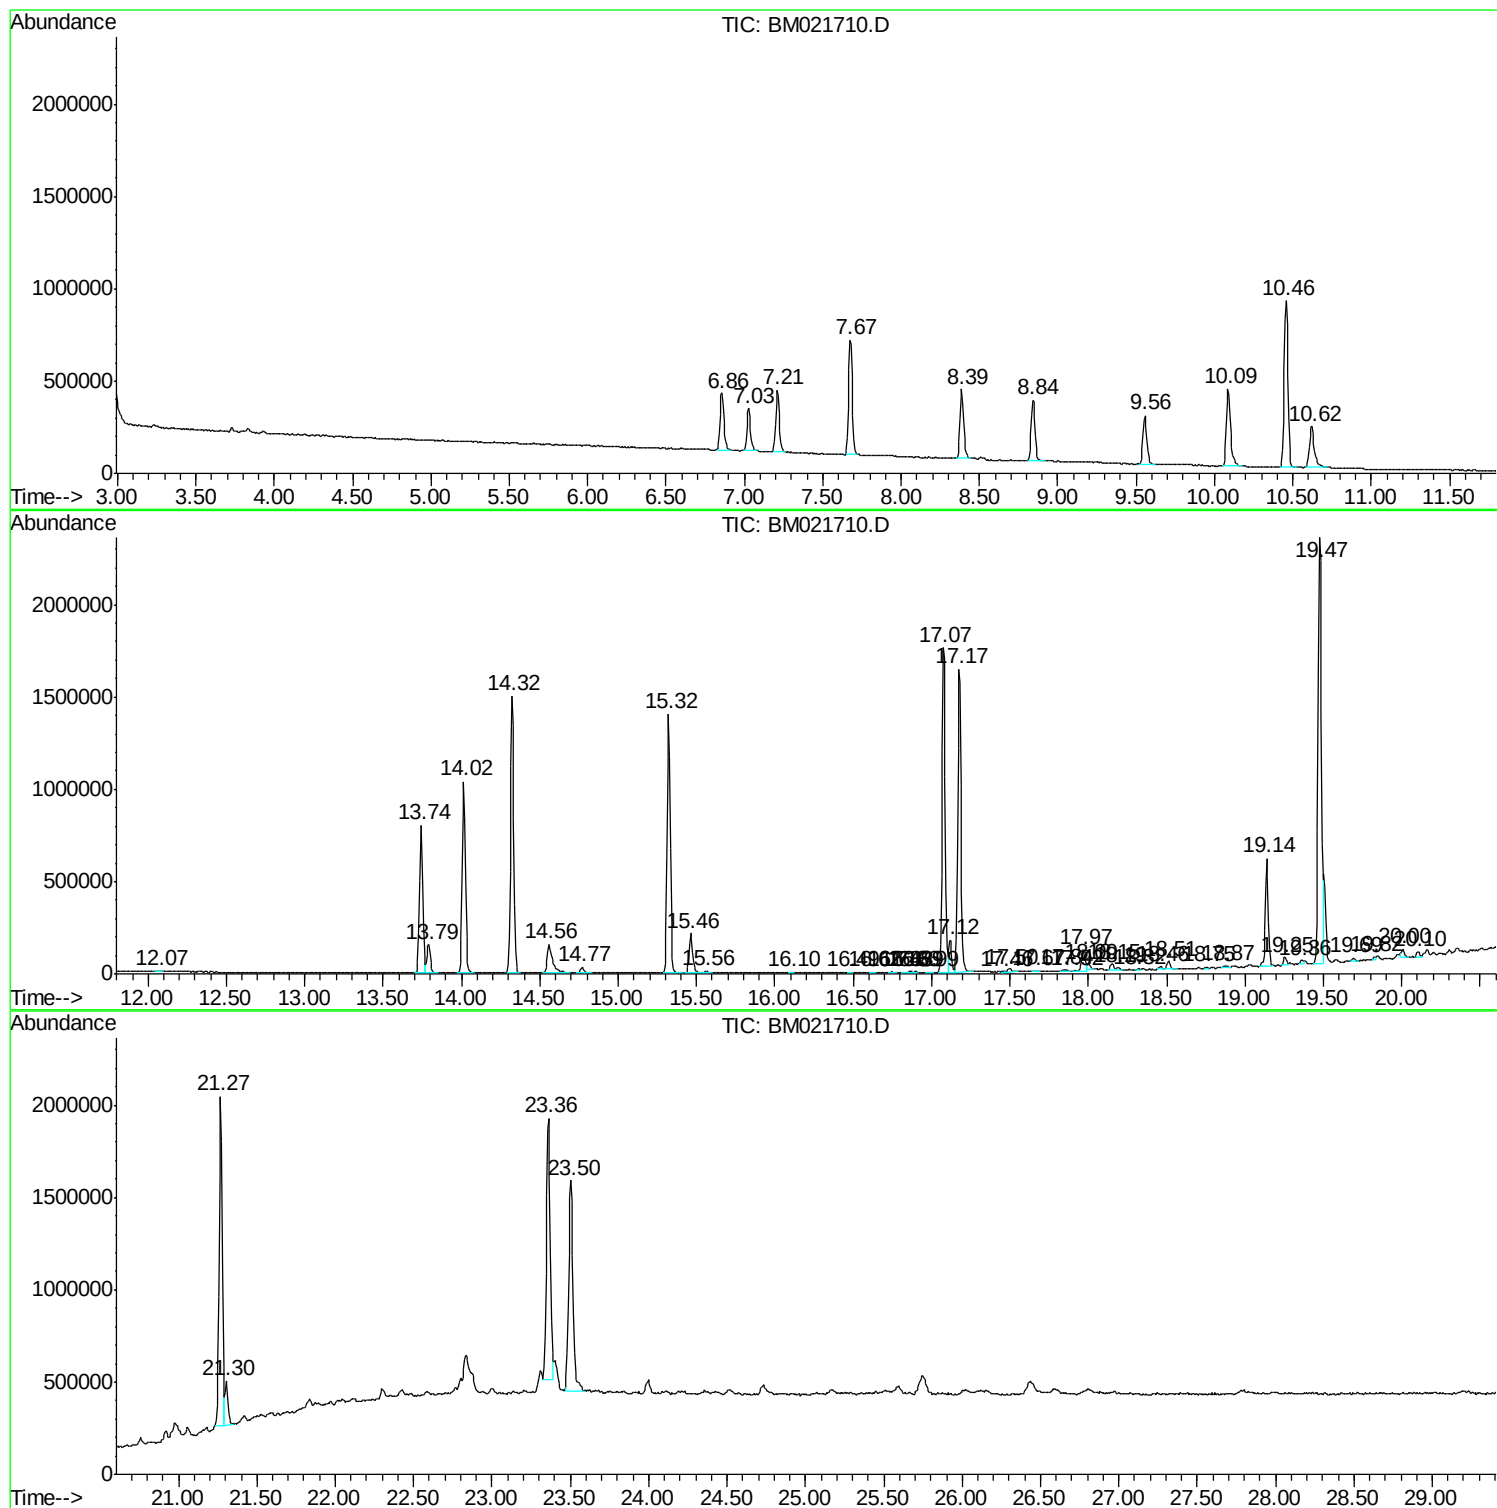

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM072919\
Data File : BM021710.D
Acq On : 30 Jul 2019 01:14
Operator : HP/JU
Sample : K3863-12
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52F2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM072919\
Data File : BM021710.D
Acq On : 30 Jul 2019 01:14
Operator : HP/JU
Sample : K3863-12
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52F2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc