

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072919\
 Data File : BM021720.D
 Acq On : 30 Jul 2019 07:17
 Operator : HP/JU
 Sample : PB121643BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK43

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072619MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.857	652	658	671	rVB	701328	1172491	25.42%	2.472%
2	7.028	681	687	704	rVB	537213	902072	19.56%	1.902%
3	7.210	712	718	730	rVB	810533	1280818	27.77%	2.700%
4	7.675	791	797	804	rVB	659756	1024568	22.22%	2.160%
5	8.387	911	918	932	rVB	912305	1544679	33.49%	3.257%
6	8.839	989	995	1006	rVB	770827	1289187	27.95%	2.718%
7	9.551	1110	1116	1127	rVB	647898	1077433	23.36%	2.272%
8	10.081	1200	1206	1223	rVB	974238	1732710	37.57%	3.653%
9	10.457	1263	1270	1281	rVB	919462	1525389	33.08%	3.216%
10	10.610	1289	1296	1316	rBV	867921	1636928	35.49%	3.451%
11	12.063	1538	1543	1551	rVB2	10367	17723	0.38%	0.037%
12	13.739	1822	1828	1843	rBV	1896813	2720450	58.99%	5.736%
13	14.016	1867	1875	1886	rBV	2228223	3267022	70.84%	6.888%
14	14.321	1920	1927	1936	rBV	1531086	2194185	47.58%	4.626%
15	14.551	1959	1966	1988	rBV	520399	989649	21.46%	2.087%
16	15.321	2090	2097	2108	rBV	2925022	4013258	87.02%	8.461%
17	15.463	2115	2121	2134	rBV	622605	895025	19.41%	1.887%
18	15.563	2134	2138	2142	rVB	28825	38206	0.83%	0.081%
19	16.104	2226	2230	2234	rBV3	8526	10852	0.24%	0.023%
20	16.862	2354	2359	2363	rBV5	3386	6053	0.13%	0.013%
21	17.074	2389	2395	2406	rBV2	1794690	2508360	54.39%	5.289%
22	17.174	2406	2412	2427	rVV	3092840	4288407	92.99%	9.042%
23	19.109	2737	2741	2748	rBV	23802	30698	0.67%	0.065%
24	19.362	2780	2784	2788	rBV	18920	26943	0.58%	0.057%
25	19.474	2797	2803	2812	rBV	3361502	4611748	100.00%	9.723%
26	21.268	3103	3108	3116	rBV	1766092	2308973	50.07%	4.868%
27	23.362	3457	3464	3477	rBV	2266260	4065635	88.16%	8.572%
28	23.503	3482	3488	3497	rVB	1193377	2250250	48.79%	4.744%


Sum of corrected areas: 47429712

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072919\
Data File : BM021720.D
Acq On : 30 Jul 2019 07:17
Operator : HP/JU
Sample : PB121643BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK43

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

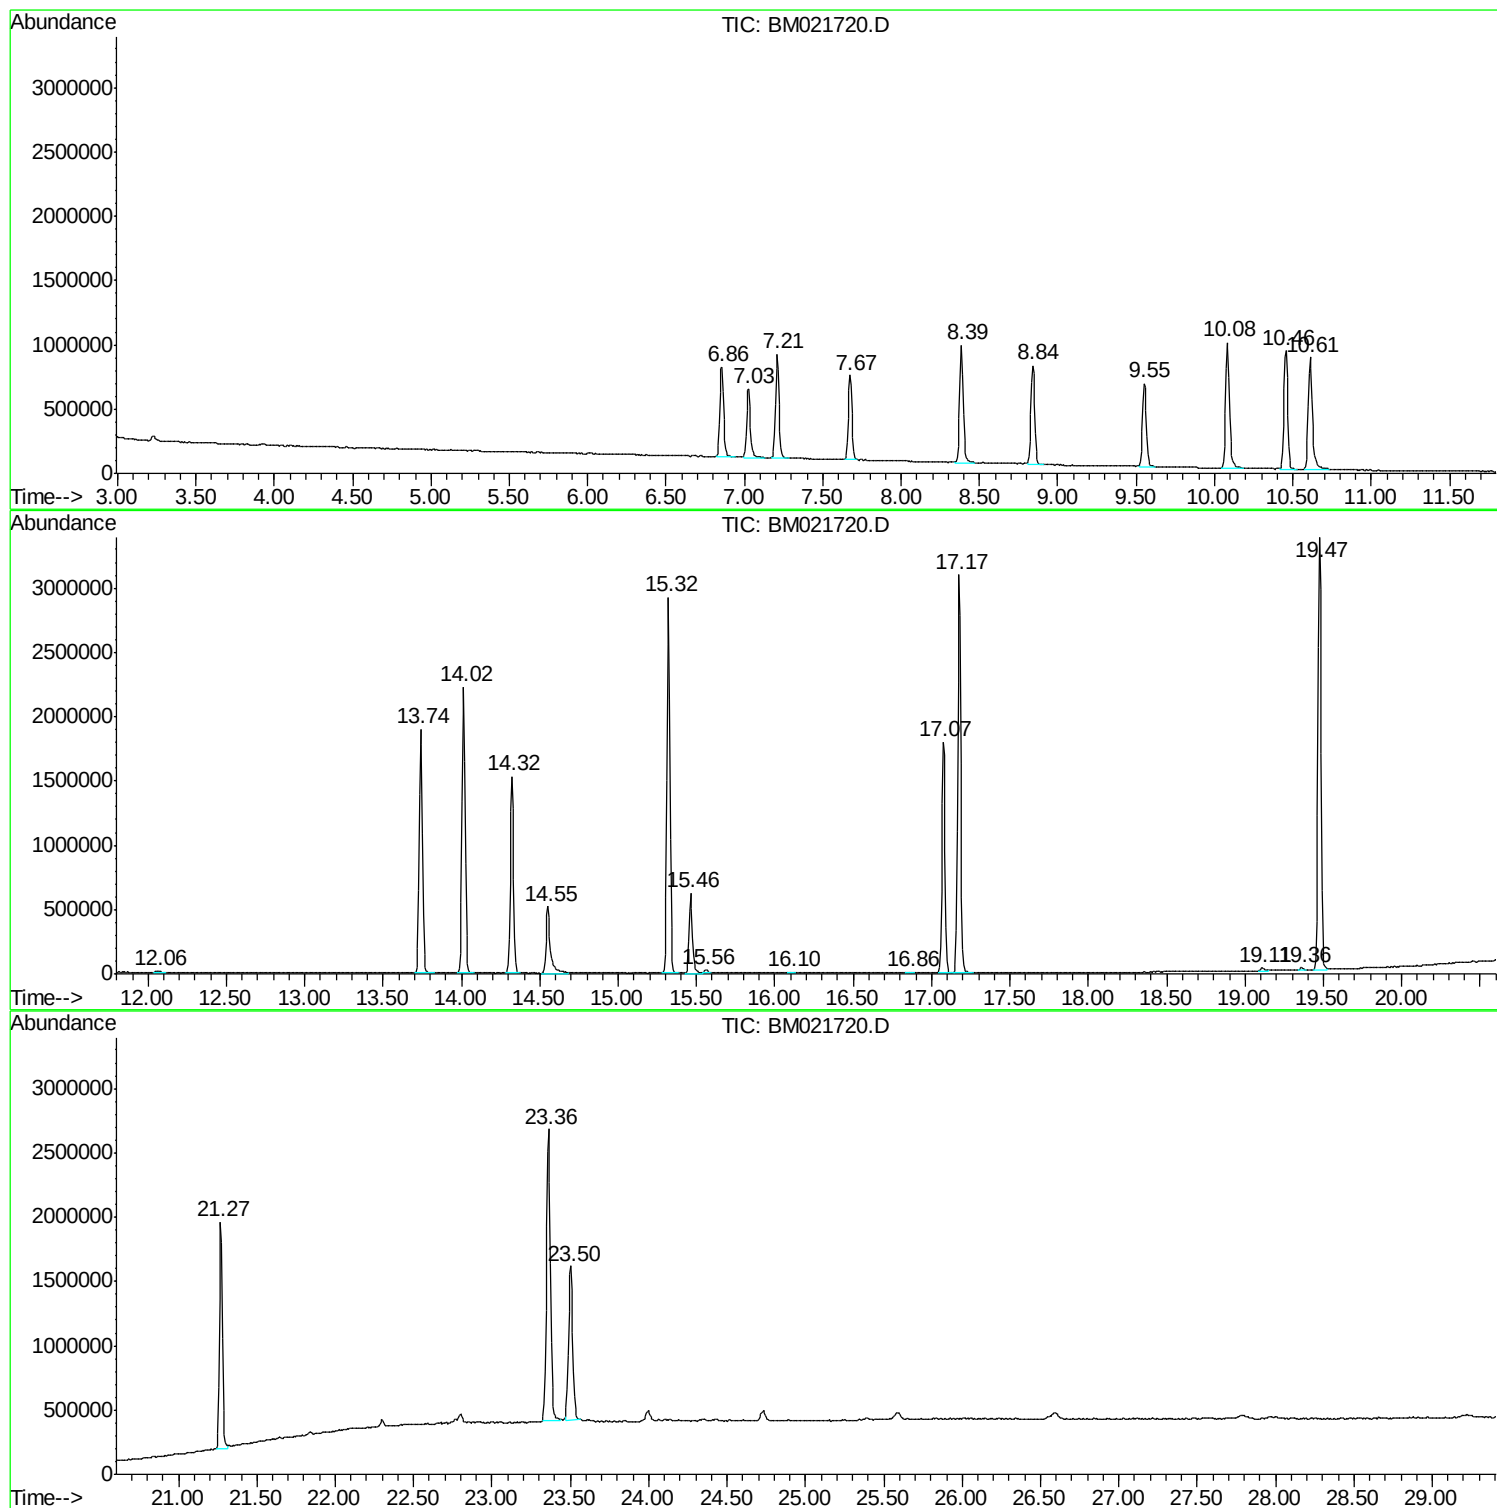

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM072919\
Data File : BM021720.D
Acq On : 30 Jul 2019 07:17
Operator : HP/JU
Sample : PB121643BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK43

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM072919\
Data File : BM021720.D
Acq On : 30 Jul 2019 07:17
Operator : HP/JU
Sample : PB121643BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK43

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc