

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072921\
 Data File : BM031265.D
 Acq On : 30 Jul 2021 01:19
 Operator : CG/JU
 Sample : M3084-16
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0034

Quant Time: Jul 30 03:42:53 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 28 15:20:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.611	152	1592	0.400	ng/ul	0.00
4) Naphthalene-d8	10.374	136	6021	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.243	164	3694	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.989	188	7013	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.178	240	5330	0.400	ng/ul	0.00
23) Perylene-d12	23.341	264	5418	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.200	96	7137	4.037	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.971	152	2590	0.255	ng/ul	0.00
18) Fluoranthene-d10	19.020	212	4775	0.268	ng/ul	0.00
Target Compounds						
15) Phenanthrene	17.030	178	580	0.026	ng/ul#	Qvalue 75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072921\
Data File : BM031265.D
Acq On : 30 Jul 2021 01:19
Operator : CG/JU
Sample : M3084-16
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0034


Quant Time: Jul 30 03:42:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 28 15:20:04 2021
Response via : Initial Calibration

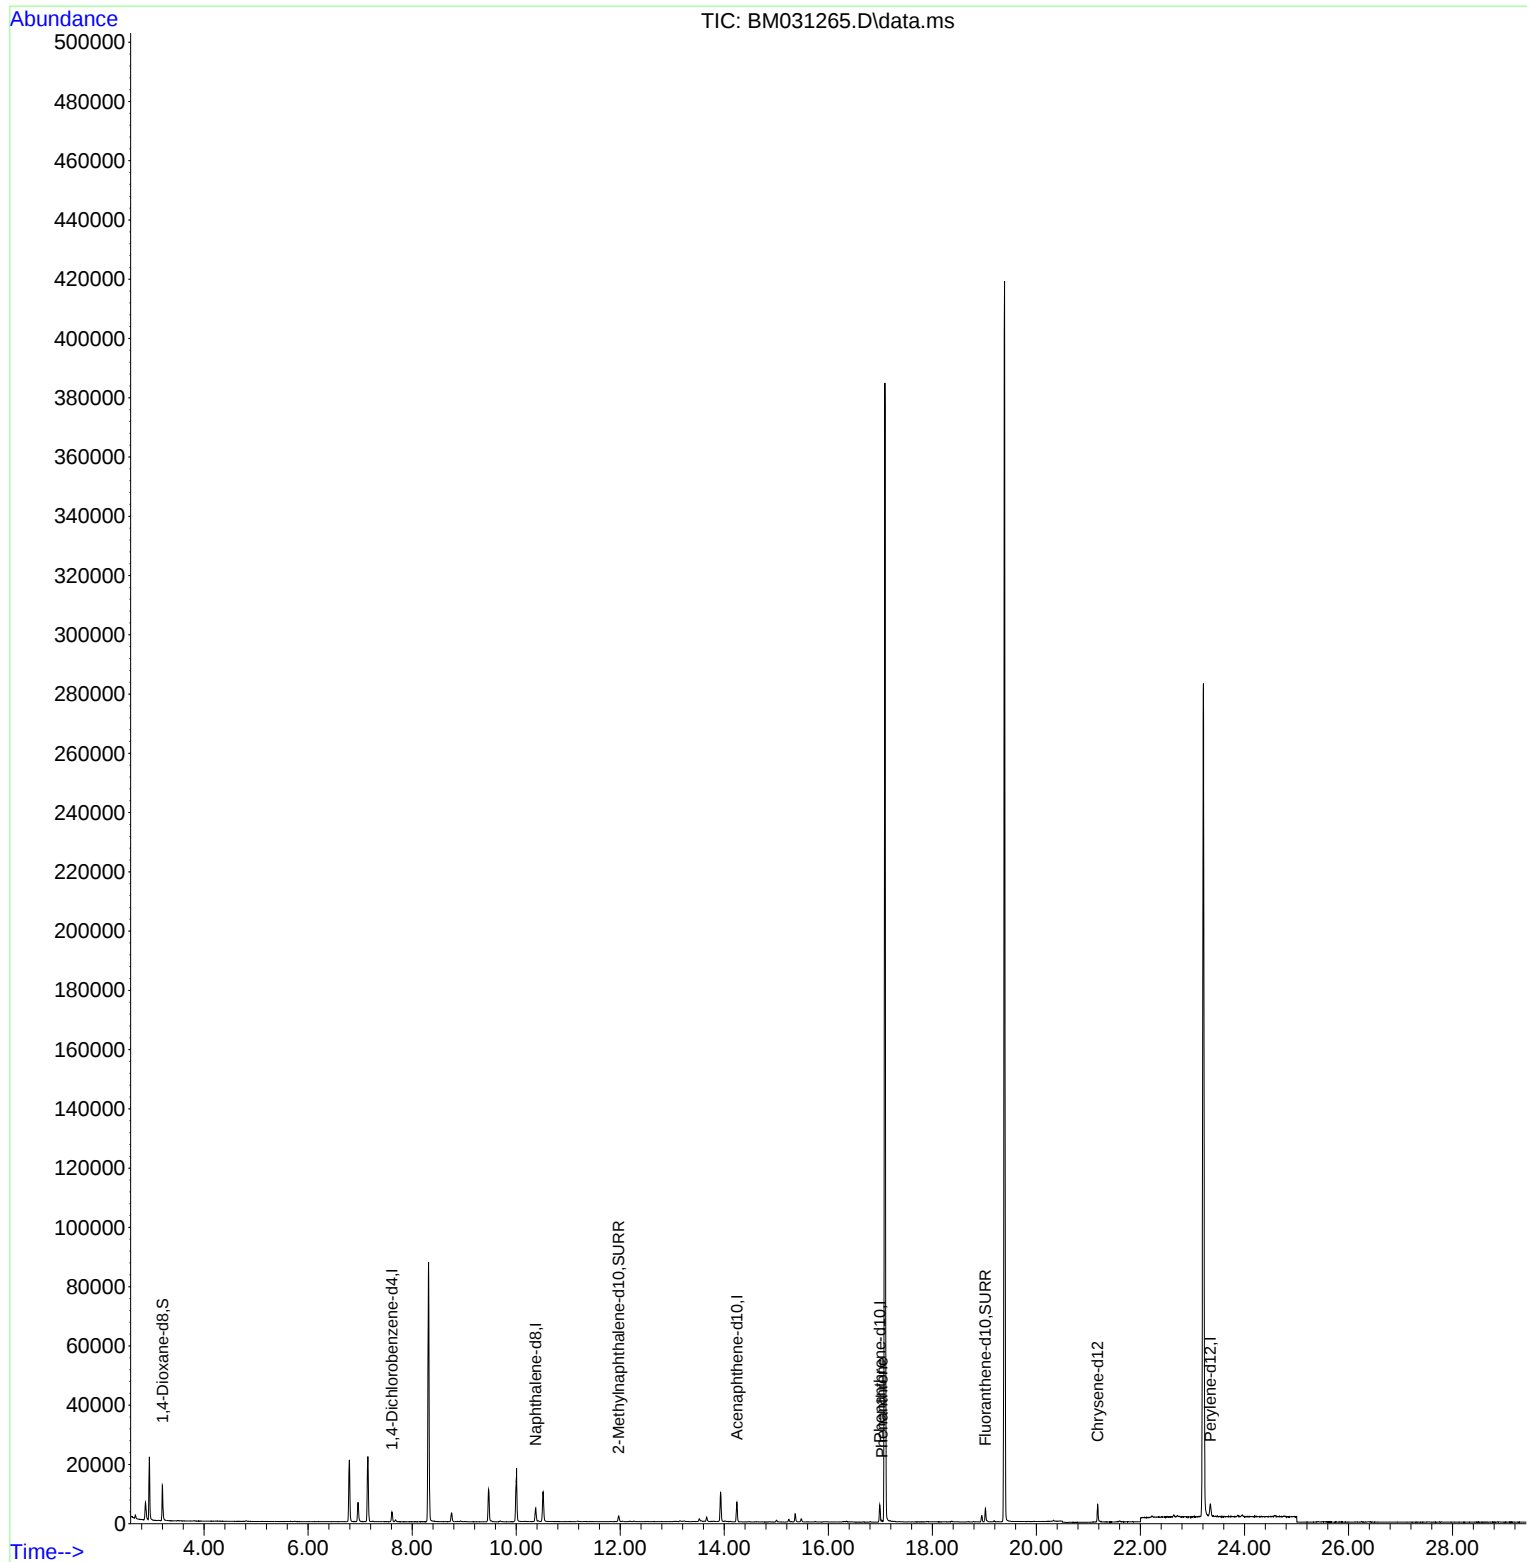

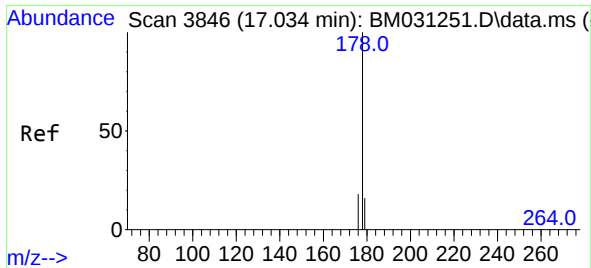

#15
Phenanthrene
Concen: 0.026 ng/ul
RT: 17.030 min Scan# 3845
Delta R.T. -0.003 min
Lab File: BM031265.D
Acq: 30 Jul 2021 01:19

Instrument :
BNA_M
ClientSampleId :
C0034

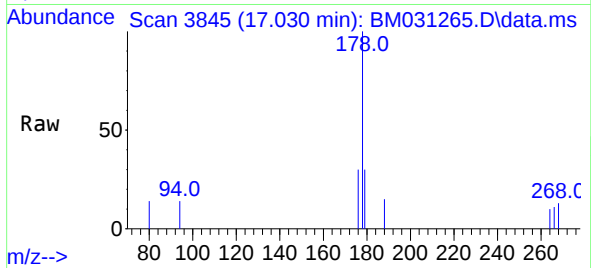

Tgt Ion:178 Resp: 580
Ion Ratio Lower Upper
178 100
179 29.8 13.3 19.9#
176 30.0 16.2 24.4#

