
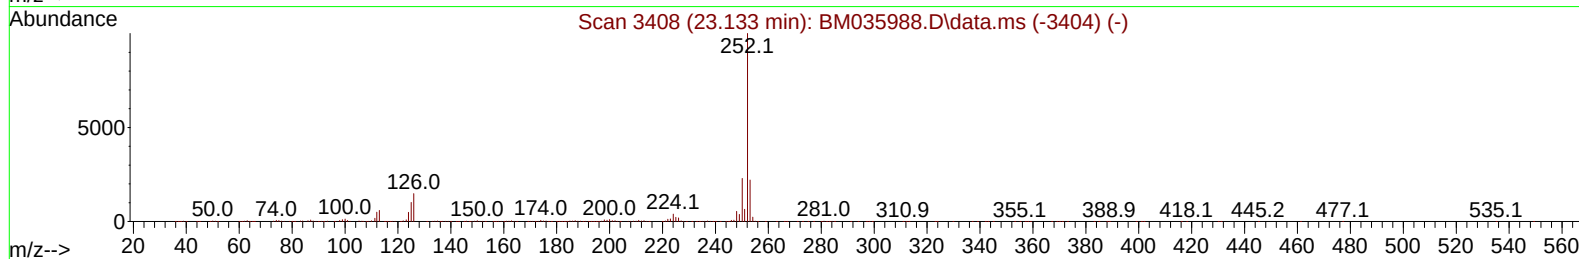
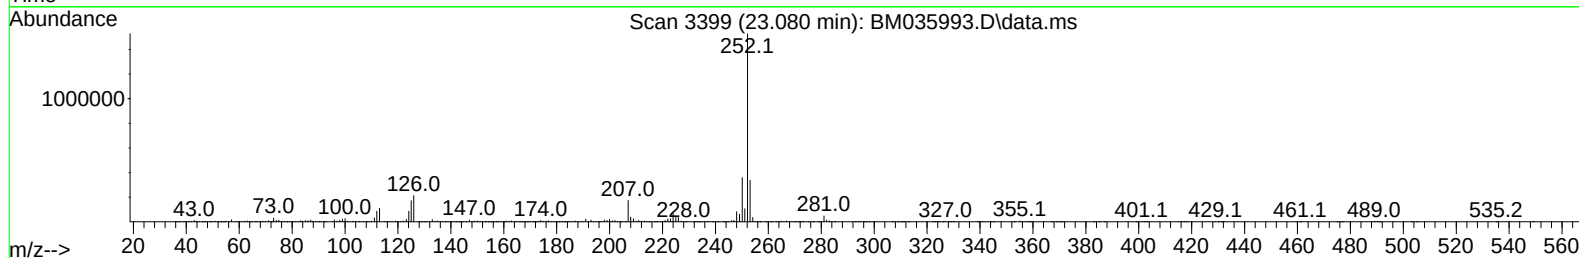


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM035993.D
Acq On : 29 Jul 2022 15:26
Operator : CG/JU
Sample : PB146474BS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Jul 30 00:23:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 30 00:20:59 2022
Response via : Initial Calibration

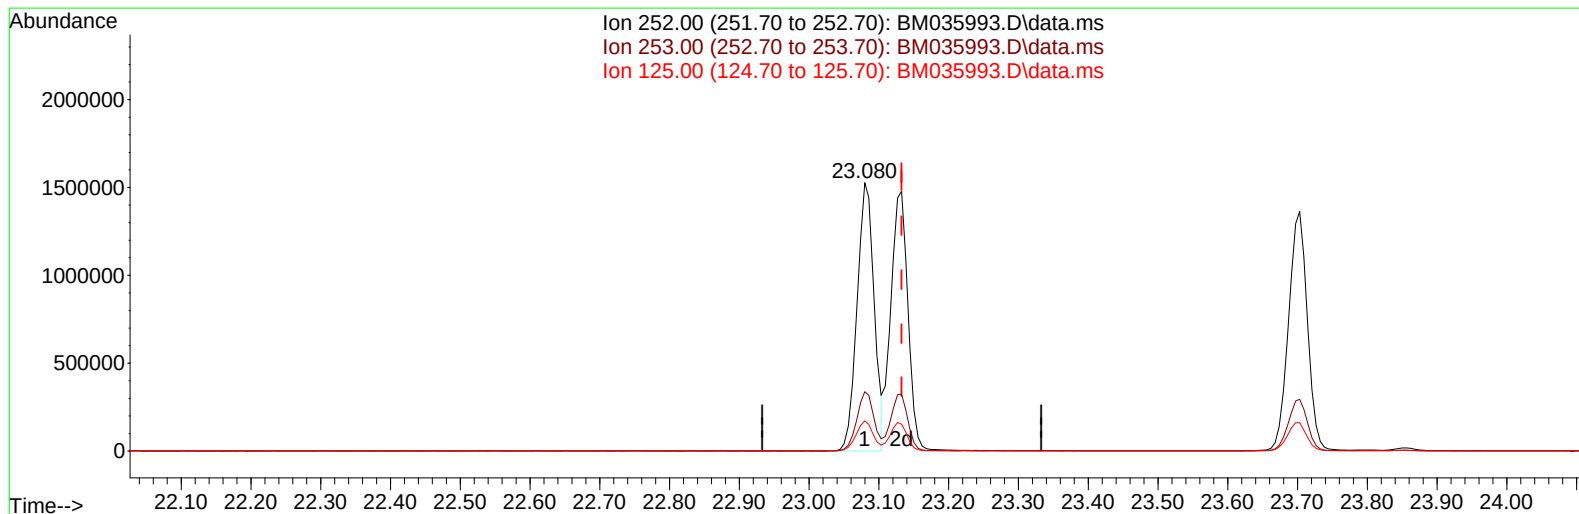

TIC: BM035993.D\data.ms

(91) Benzo(k)fluoranthene

23.080min (-0.053) 35.40 ng/u1

response 2602769

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.70	22.12
125.00	13.20	11.27
0.00	0.00	0.00