

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
 Data File : BM035998.D
 Acq On : 29 Jul 2022 18:30
 Operator : CG/JU
 Sample : N3890-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YBEA3

Quant Time: Jul 30 00:24:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 30 00:20:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	291043	20.000	ng/u1	0.00
20) Naphthalene-d8	10.681	136	1187154	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.516	164	647996	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.251	188	1215825	20.000	ng/u1	0.00
79) Chrysene-d12	21.433	240	1158531	20.000	ng/u1	0.00
88) Perylene-d12	23.797	264	1193482	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	33189	4.291	ng/uL	0.00
4) Pyridine-d5	3.699	84	199431	9.412	ng/u1	0.00
7) Phenol-d5	7.040	99	121488	4.978	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.210	67	439643	27.021	ng/u1	0.00
11) 2-Chlorophenol-d4	7.404	132	425629	21.010	ng/u1	0.00
15) 4-Methylphenol-d8	8.587	113	229659	11.615	ng/u1	0.00
21) Nitrobenzene-d5	9.045	128	281382	29.912	ng/u1	0.00
24) 2-Nitrophenol-d4	9.769	143	262281	28.617	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.304	165	428699	25.862	ng/u1	0.00
31) 4-Chloroaniline-d4	10.822	131	625382	22.286	ng/u1	0.00
46) Dimethylphthalate-d6	13.927	166	1476042	33.440	ng/u1	0.00
49) Acenaphthylene-d8	14.210	160	1747706	31.033	ng/u1	0.00
54) 4-Nitrophenol-d4	14.716	143	44661	4.927	ng/u1	0.00
60) Fluorene-d10	15.504	176	1331712	33.387	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.621	200	180718	27.652	ng/u1	0.00
73) Anthracene-d10	17.351	188	2235090	40.662	ng/u1	0.00
81) Pyrene-d10	19.645	212	2526948	39.356	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.650	264	2513893	41.489	ng/u1	0.00


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.310	88	8463	1.056	ng/uL#	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM035998.D
Acq On : 29 Jul 2022 18:30
Operator : CG/JU
Sample : N3890-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YBEA3

Quant Time: Jul 30 00:24:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 30 00:20:59 2022
Response via : Initial Calibration

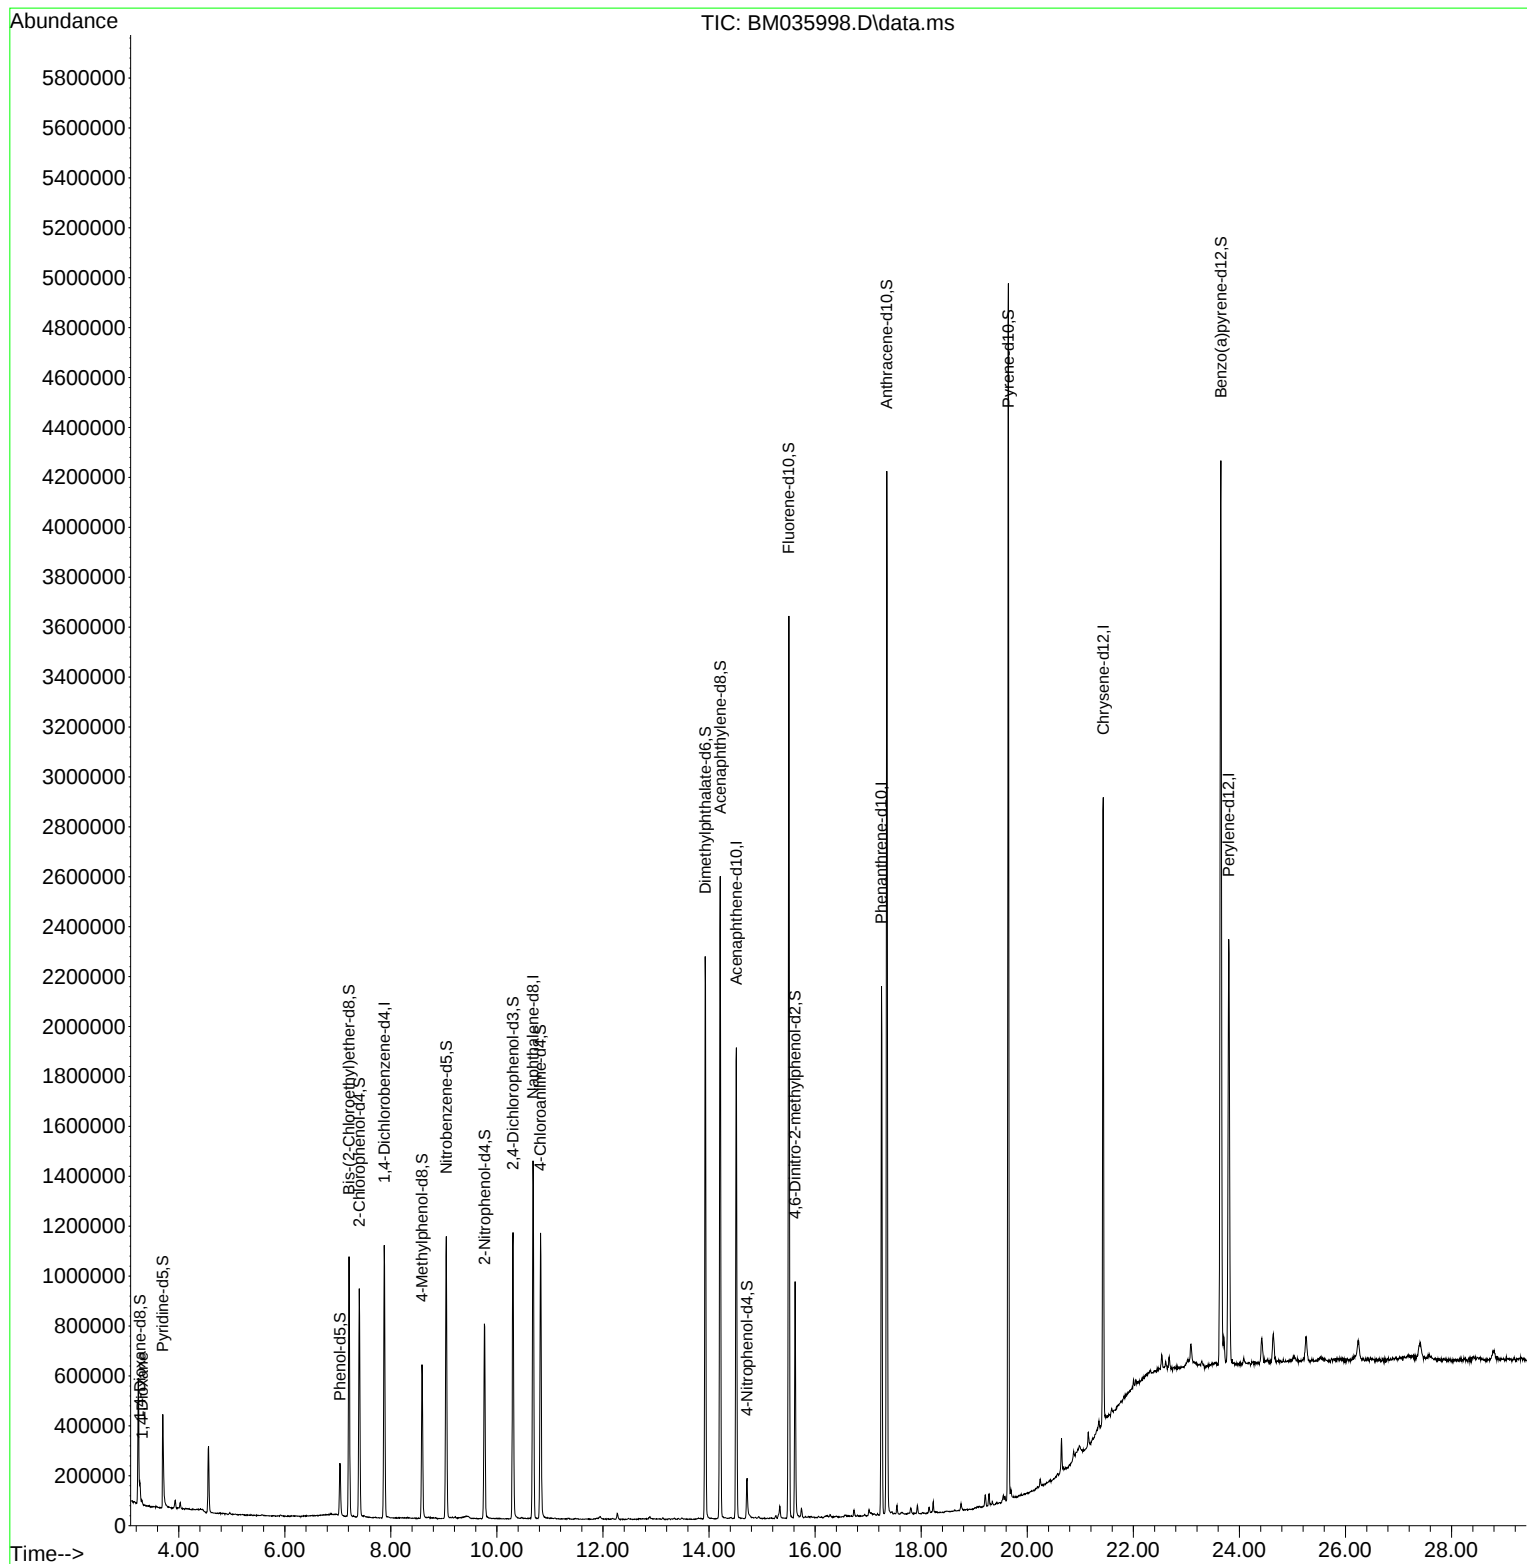

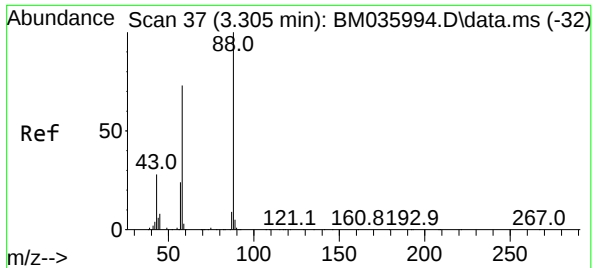

#2
 1,4-Dioxane
 Concen: 1.056 ng/uL
 RT: 3.310 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: BM035998.D
 Acq: 29 Jul 2022 18:30

Instrument :
 BNA_M
 ClientSampleId :
 YBEA3

Tgt Ion:	88	Resp:	8463
Ion	Ratio	Lower	Upper
88	100		
43	31.7	27.8	41.8
58	61.3	61.8	92.8#

