

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM072922\  
 Data File : BM036007.D  
 Acq On : 29 Jul 2022 23:59  
 Operator : CG/JU  
 Sample : N3790-07  
 Misc :  
 ALS Vial : 20 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DBUK3

Quant Time: Jul 30 00:57:31 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM072522.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Sat Jul 30 00:20:59 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|-------------------------------|--------|------|----------|--------|-------|----------|
| -----                         |        |      |          |        |       |          |
| Internal Standards            |        |      |          |        |       |          |
| 1) 1,4-Dichlorobenzene-d4     | 7.875  | 152  | 344824   | 20.000 | ng/ul | 0.00     |
| 20) Naphthalene-d8            | 10.680 | 136  | 1434446  | 20.000 | ng/ul | 0.00     |
| 38) Acenaphthene-d10          | 14.510 | 164  | 777503   | 20.000 | ng/ul | 0.00     |
| 64) Phenanthrene-d10          | 17.251 | 188  | 1446584  | 20.000 | ng/ul | 0.00     |
| 79) Chrysene-d12              | 21.427 | 240  | 1251756  | 20.000 | ng/ul | 0.00     |
| 88) Perylene-d12              | 23.791 | 264  | 1297377  | 20.000 | ng/ul | -0.02    |
| System Monitoring Compounds   |        |      |          |        |       |          |
| 3) 1,4-Dioxane-d8             | 3.269  | 96   | 34153    | 3.727  | ng/uL | 0.00     |
| 4) Pyridine-d5                | 3.699  | 84   | 88076    | 3.508  | ng/ul | 0.00     |
| 7) Phenol-d5                  | 7.040  | 99   | 577947   | 19.987 | ng/ul | 0.00     |
| 9) Bis-(2-Chloroethyl)eth...  | 7.210  | 67   | 389164   | 20.188 | ng/ul | 0.00     |
| 11) 2-Chlorophenol-d4         | 7.404  | 132  | 508630   | 21.191 | ng/ul | 0.00     |
| 15) 4-Methylphenol-d8         | 8.586  | 113  | 452970   | 19.336 | ng/ul | 0.00     |
| 21) Nitrobenzene-d5           | 9.045  | 128  | 247260   | 21.753 | ng/ul | 0.00     |
| 24) 2-Nitrophenol-d4          | 9.763  | 143  | 246061   | 22.219 | ng/ul | 0.00     |
| 28) 2,4-Dichlorophenol-d3     | 10.298 | 165  | 419109   | 20.925 | ng/ul | 0.00     |
| 31) 4-Chloroaniline-d4        | 10.822 | 131  | 590703   | 17.421 | ng/ul | 0.00     |
| 46) Dimethylphthalate-d6      | 13.927 | 166  | 1257592  | 23.745 | ng/ul | 0.00     |
| 49) Acenaphthylene-d8         | 14.204 | 160  | 1575152  | 23.310 | ng/ul | 0.00     |
| 54) 4-Nitrophenol-d4          | 14.710 | 143  | 173445   | 15.948 | ng/ul | 0.00     |
| 60) Fluorene-d10              | 15.504 | 176  | 1090166  | 22.779 | ng/ul | 0.00     |
| 65) 4,6-Dinitro-2-methylph... | 15.621 | 200  | 121488   | 15.624 | ng/ul | 0.00     |
| 73) Anthracene-d10            | 17.351 | 188  | 1549634  | 23.694 | ng/ul | 0.00     |
| 81) Pyrene-d10                | 19.639 | 212  | 1754792  | 25.294 | ng/ul | 0.00     |
| 92) Benzo(a)pyrene-d12        | 23.638 | 264  | 1623404  | 24.647 | ng/ul | -0.01    |
| Target Compounds              |        |      |          |        |       |          |
| 86) Bis(2-ethylhexyl)phtha... | 21.344 | 149  | 59734    | 1.330  | ng/ul | 99       |
| -----                         |        |      |          |        |       |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM072922\  
Data File : BM036007.D  
Acq On : 29 Jul 2022 23:59  
Operator : CG/JU  
Sample : N3790-07  
Misc :  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DBUK3


Quant Time: Jul 30 00:57:31 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM072522.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Sat Jul 30 00:20:59 2022  
Response via : Initial Calibration

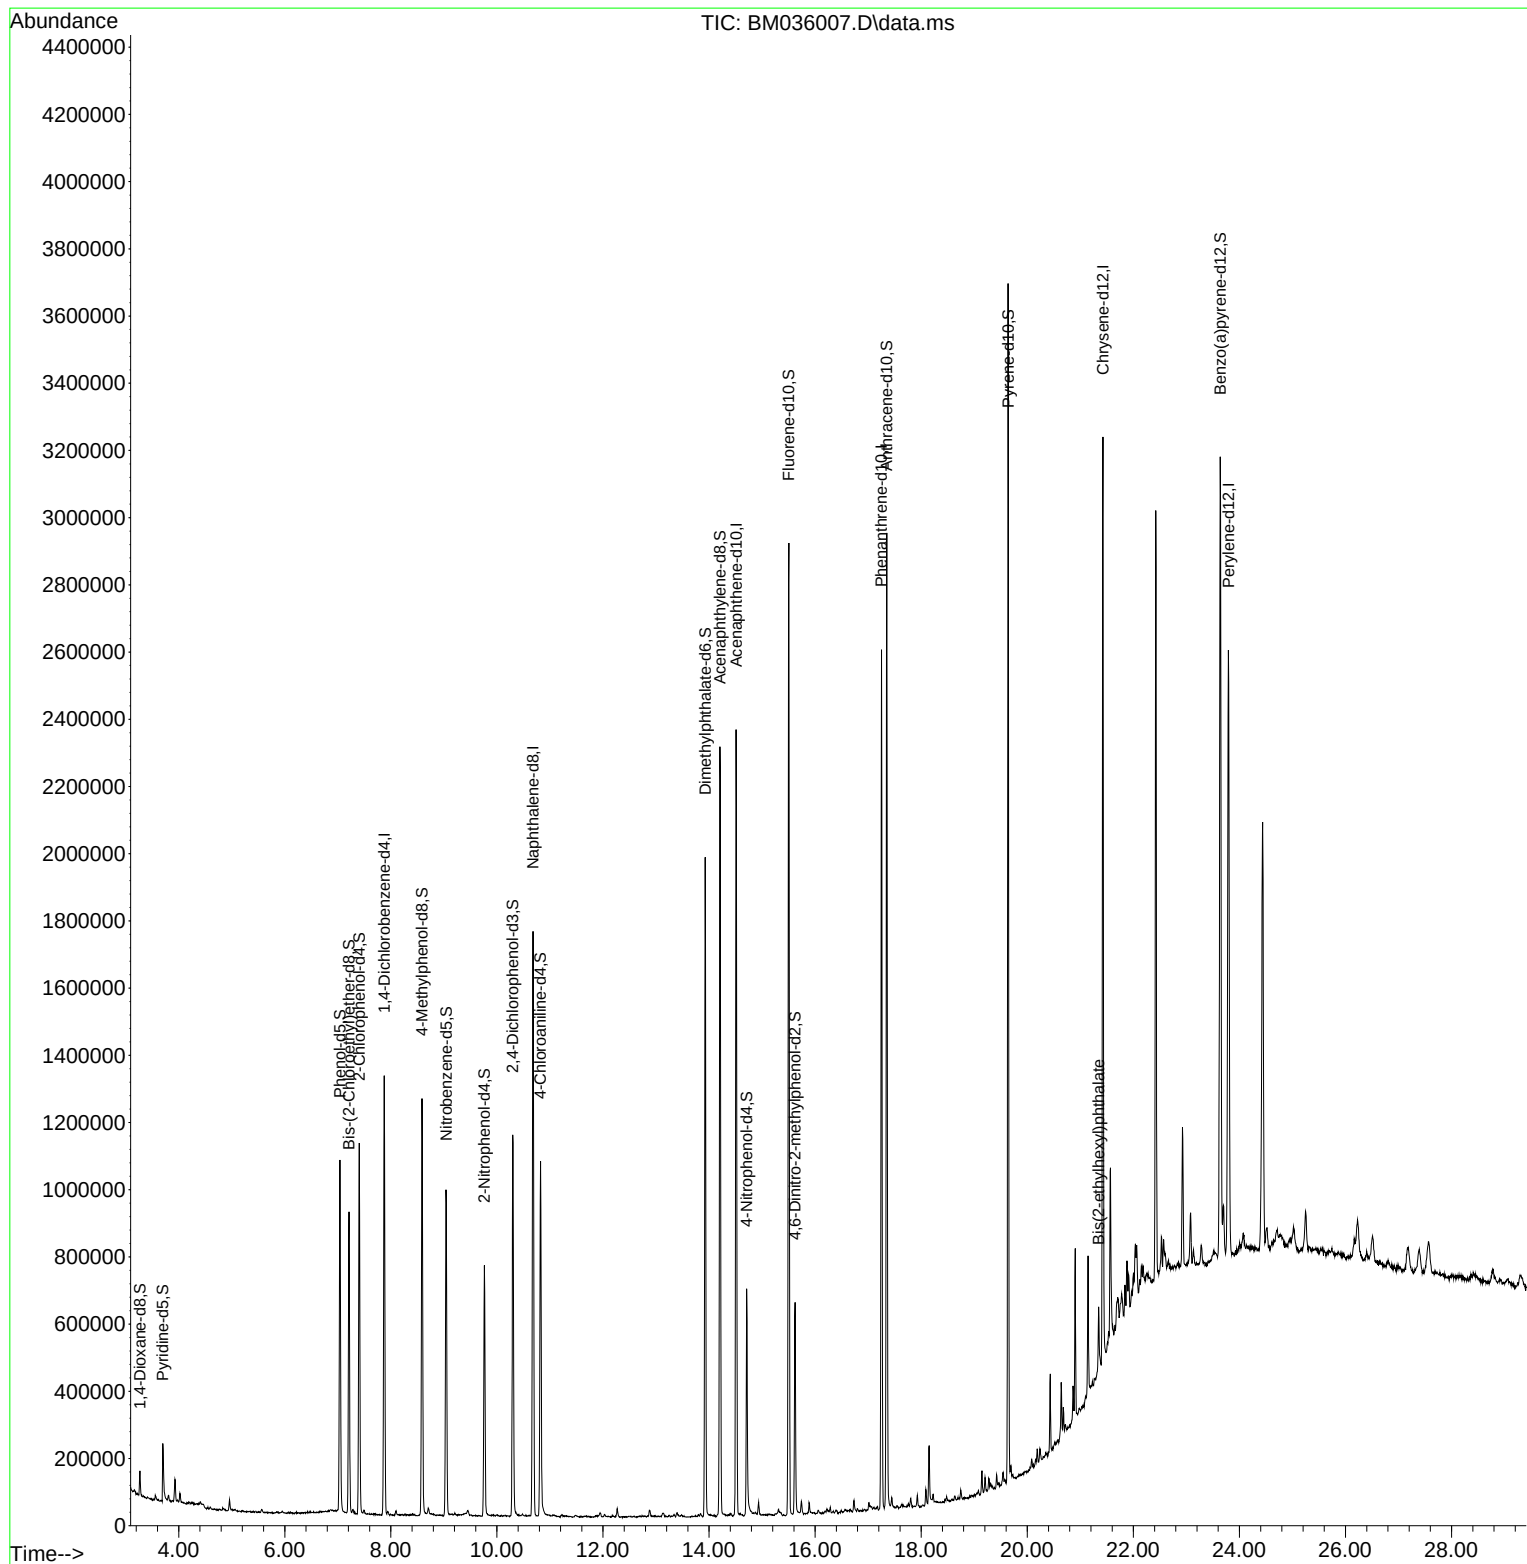

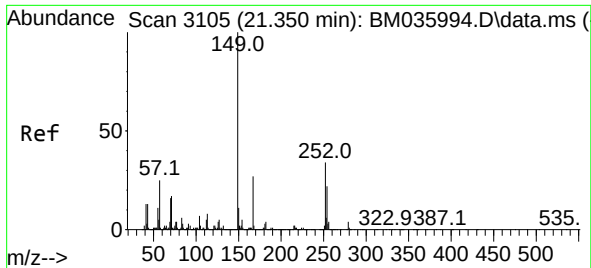

#86  
 Bis(2-ethylhexyl)phthalate  
 Concen: 1.330 ng/ul  
 RT: 21.344 min Scan# 3104  
 Delta R.T. -0.006 min  
 Lab File: BM036007.D  
 Acq: 29 Jul 2022 23:59

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DBUK3

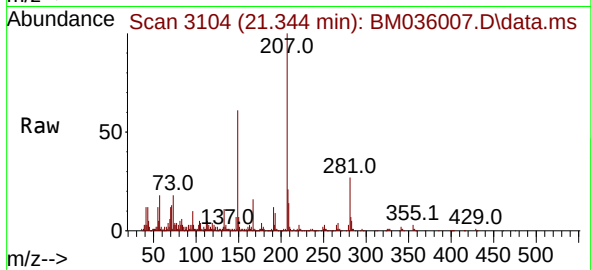

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 149   | Resp: | 59734 |
| Ion      | Ratio | Lower | Upper |
| 149      | 100   |       |       |
| 167      | 26.1  | 21.5  | 32.3  |
| 279      | 4.2   | 3.4   | 5.2   |

