

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
 Data File : BM035995.D
 Acq On : 29 Jul 2022 16:40
 Operator : CG/JU
 Sample : PB146498BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK498

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035995.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	38	rVB	85233	111117	2.01%	0.176%
2	3.693	100	103	117	rBV	978594	1433627	25.88%	2.265%
3	4.028	157	160	164	rVB	22703	24039	0.43%	0.038%
4	6.422	564	567	571	rBV6	3425	5574	0.10%	0.009%
5	7.039	666	672	685	rVB	1072151	1699310	30.67%	2.685%
6	7.210	695	701	713	rVV	946440	1451577	26.20%	2.293%
7	7.404	727	734	747	rBV	1181158	1836953	33.16%	2.902%
8	7.875	807	814	823	rBV	1037097	1632515	29.47%	2.579%
9	8.586	928	935	947	rBV	1291569	2116362	38.20%	3.343%
10	9.045	1004	1013	1021	rBV	1038728	1680634	30.34%	2.655%
11	9.686	1120	1122	1126	rVB5	4705	5984	0.11%	0.009%
12	9.763	1126	1135	1144	rBV	791666	1336143	24.12%	2.111%
13	10.304	1219	1227	1242	rBV	1238098	2076903	37.49%	3.281%
14	10.680	1284	1291	1299	rBV	1411573	2305096	41.61%	3.642%
15	10.822	1307	1315	1332	rBV	1293935	2220735	40.09%	3.508%
16	11.869	1488	1493	1495	rBV5	5805	6754	0.12%	0.011%
17	11.945	1503	1506	1517	rVB5	10034	21614	0.39%	0.034%
18	12.269	1555	1561	1569	rBV2	22607	43153	0.78%	0.068%
19	12.880	1659	1665	1670	rBV7	6778	14806	0.27%	0.023%
20	13.480	1762	1767	1772	rVB9	4061	8458	0.15%	0.013%
21	13.804	1818	1822	1824	rBV5	4870	6005	0.11%	0.009%
22	13.927	1837	1843	1857	rBV	2064088	2861155	51.65%	4.520%
23	14.210	1884	1891	1900	rBV	2529629	3617272	65.30%	5.715%
24	14.515	1936	1943	1951	rBV	1980212	2884955	52.08%	4.558%
25	14.710	1969	1976	1989	rBV	841315	1364169	24.63%	2.155%
26	15.309	2073	2078	2081	rBV6	7970	12479	0.23%	0.020%
27	15.504	2103	2111	2118	rBV	3260151	4437266	80.10%	7.010%
28	15.621	2125	2131	2143	rBV	818948	1134646	20.48%	1.793%
29	15.739	2147	2151	2158	rVB	37822	59375	1.07%	0.094%
30	15.921	2178	2182	2185	rBV6	5665	6746	0.12%	0.011%
31	16.186	2222	2227	2230	rBV7	4305	9181	0.17%	0.015%
32	16.227	2230	2234	2236	rBV5	5432	6426	0.12%	0.010%
33	16.286	2241	2244	2249	rVB7	12585	16745	0.30%	0.026%
34	16.398	2257	2263	2264	rBV6	4014	6092	0.11%	0.010%
35	16.562	2287	2291	2294	rBV5	7019	11839	0.21%	0.019%
36	16.733	2315	2320	2327	rBV2	27222	41960	0.76%	0.066%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
 Data File : BM035995.D
 Acq On : 29 Jul 2022 16:40
 Operator : CG/JU
 Sample : PB146498BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK498

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	16.933	2351	2354	2357	rBV4	6619	8402	0.15%	0.013%
38	17.021	2363	2369	2370	rBV4	15692	24960	0.45%	0.039%
39	17.251	2402	2408	2415	rBV	2324973	3312891	59.80%	5.234%
40	17.351	2418	2425	2437	rVV2	3357107	4722718	85.25%	7.461%
41	17.803	2498	2502	2508	rVB2	24052	37106	0.67%	0.059%
42	17.927	2519	2523	2528	rVB8	8332	14681	0.27%	0.023%
43	18.145	2557	2560	2563	rBV5	5800	8347	0.15%	0.013%
44	18.221	2571	2573	2575	rBV3	6991	7731	0.14%	0.012%
45	18.750	2659	2663	2666	rBV3	25646	36377	0.66%	0.057%
46	19.209	2737	2741	2748	rVB3	41736	52762	0.95%	0.083%
47	19.280	2749	2753	2758	rBV	40910	56107	1.01%	0.089%
48	19.544	2795	2798	2802	rBV4	29979	37184	0.67%	0.059%
49	19.645	2809	2815	2821	rBV	4130258	5539766	100.00%	8.752%
50	20.244	2914	2917	2921	rBV4	26616	34669	0.63%	0.055%
51	20.644	2982	2985	2992	rBV	148883	170511	3.08%	0.269%
52	21.433	3114	3119	3125	rBV	2834427	3583049	64.68%	5.661%
53	23.650	3489	3496	3503	rBV2	2856276	5466394	98.68%	8.636%
54	23.803	3515	3522	3532	rVB2	1790194	3677628	66.39%	5.810%




Sum of corrected areas: 63298948

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM035995.D
Acq On : 29 Jul 2022 16:40
Operator : CG/JU
Sample : PB146498BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK498

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

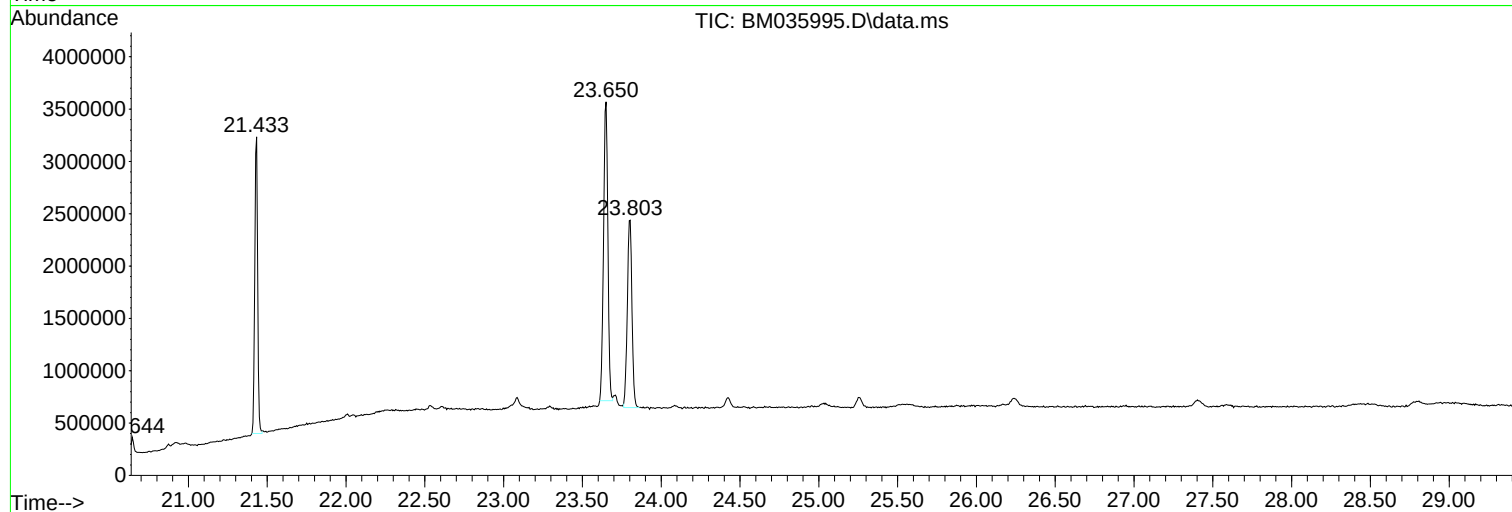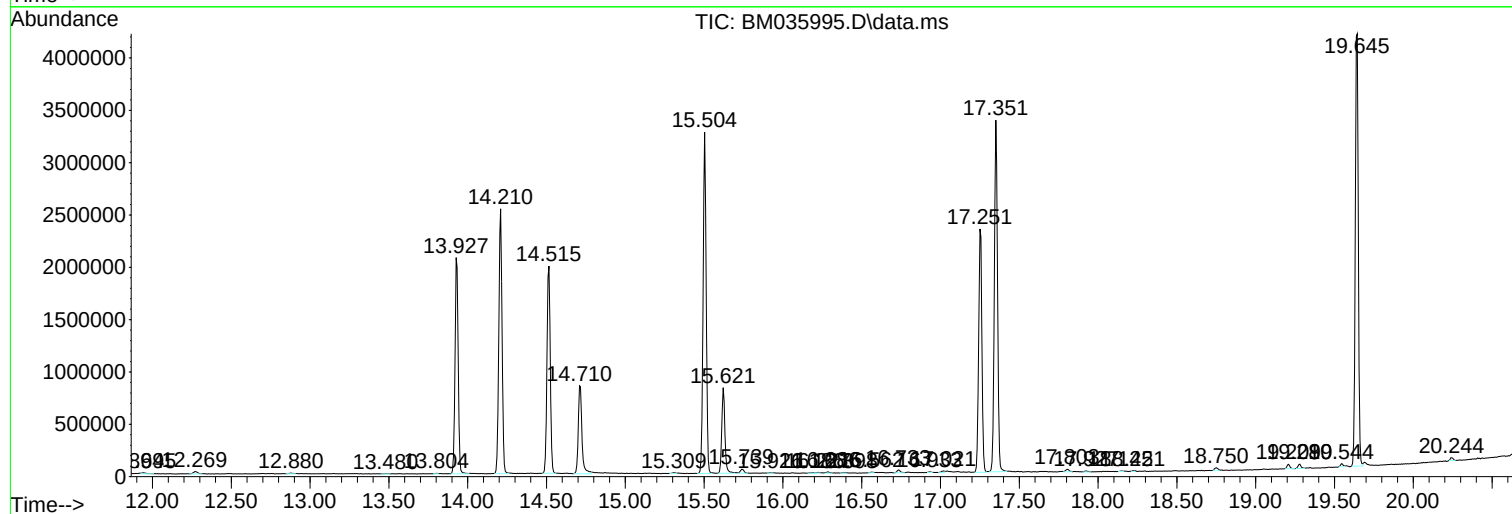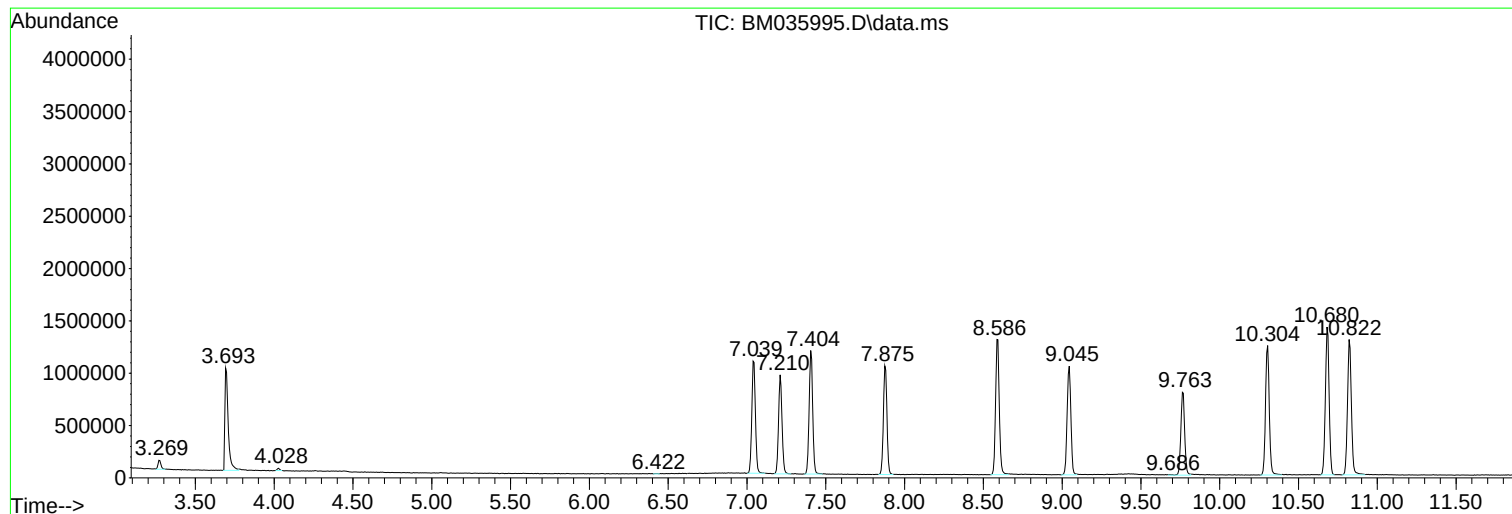

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM035995.D
Acq On : 29 Jul 2022 16:40
Operator : CG/JU
Sample : PB146498BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK498

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM035995.D
Acq On : 29 Jul 2022 16:40
Operator : CG/JU
Sample : PB146498BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK498

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------