

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
 Data File : BM035997.D
 Acq On : 29 Jul 2022 17:53
 Operator : CG/JU
 Sample : N3790-22
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBUL8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035997.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	36	rVB	52546	64073	1.46%	0.120%
2	3.699	102	104	115	rBV	184141	285158	6.50%	0.534%
3	3.928	139	143	149	rVB2	43315	67594	1.54%	0.126%
4	4.028	156	160	167	rVB2	27089	40066	0.91%	0.075%
5	4.840	295	298	302	rBV6	5839	8533	0.19%	0.016%
6	4.957	314	318	323	rBV	21745	30794	0.70%	0.058%
7	7.040	666	672	682	rVV	679077	1046730	23.87%	1.959%
8	7.210	695	701	710	rVV	582066	885183	20.18%	1.656%
9	7.287	712	714	718	rVB3	6213	8004	0.18%	0.015%
10	7.404	728	734	746	rVV	701667	1099679	25.07%	2.058%
11	7.493	746	749	755	rVB6	9734	15778	0.36%	0.030%
12	7.875	807	814	821	rBV	1146982	1779842	40.58%	3.331%
13	8.587	929	935	945	rBV	670770	1088281	24.81%	2.037%
14	9.045	1004	1013	1020	rBV	624007	1025487	23.38%	1.919%
15	9.763	1129	1135	1148	rBV	465436	781864	17.83%	1.463%
16	10.304	1219	1227	1240	rBV	714692	1224911	27.93%	2.292%
17	10.681	1284	1291	1299	rBV	1515797	2510564	57.24%	4.698%
18	10.822	1307	1315	1328	rBV	696994	1230786	28.06%	2.303%
19	11.939	1502	1505	1512	rVB7	10110	18462	0.42%	0.035%
20	12.275	1558	1562	1567	rVV3	15324	21322	0.49%	0.040%
21	12.351	1570	1575	1582	rBV5	8116	15573	0.36%	0.029%
22	12.557	1607	1610	1617	rVB7	6237	11438	0.26%	0.021%
23	12.880	1657	1665	1671	rBV10	10084	27580	0.63%	0.052%
24	13.127	1702	1707	1711	rVB7	5945	10645	0.24%	0.020%
25	13.245	1724	1727	1733	rVB6	5119	7909	0.18%	0.015%
26	13.351	1739	1745	1749	rVV9	5410	8281	0.19%	0.015%
27	13.486	1765	1768	1773	rVB7	5639	8712	0.20%	0.016%
28	13.804	1817	1822	1824	rBV6	5300	7664	0.17%	0.014%
29	13.839	1824	1828	1833	rVV8	9213	15332	0.35%	0.029%
30	13.927	1837	1843	1857	rVB	1339247	1820234	41.50%	3.406%
31	14.210	1882	1891	1899	rBV	1507824	2181384	49.74%	4.082%
32	14.510	1936	1942	1949	rVV	2030194	2987311	68.11%	5.590%
33	14.574	1949	1953	1960	rVB	56592	92151	2.10%	0.172%
34	14.710	1969	1976	1991	rBV	421415	688347	15.69%	1.288%
35	14.986	2020	2023	2027	rVB6	6526	8207	0.19%	0.015%
36	15.304	2073	2077	2080	rBV5	11524	17211	0.39%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
 Data File : BM035997.D
 Acq On : 29 Jul 2022 17:53
 Operator : CG/JU
 Sample : N3790-22
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBUL8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	15.504	2101	2111	2117	rBV	2009565	2830200	64.53%	5.296%
38	15.557	2117	2120	2126	rVV	79203	111967	2.55%	0.210%
39	15.621	2126	2131	2139	rVV	386817	552624	12.60%	1.034%
40	15.680	2139	2141	2145	rVV4	13748	18147	0.41%	0.034%
41	15.739	2145	2151	2159	rVV3	21734	50988	1.16%	0.095%
42	15.804	2160	2162	2167	rVV6	6202	8618	0.20%	0.016%
43	15.851	2167	2170	2178	rVB3	13069	22648	0.52%	0.042%
44	15.992	2187	2194	2203	rVB3	13411	32083	0.73%	0.060%
45	16.192	2222	2228	2229	rBV6	5363	7759	0.18%	0.015%
46	16.221	2230	2233	2241	rVV8	13708	28109	0.64%	0.053%
47	16.292	2241	2245	2248	rVB6	6485	10033	0.23%	0.019%
48	16.563	2281	2291	2294	rBV6	25590	49421	1.13%	0.092%
49	16.663	2304	2308	2310	rBV4	7599	8228	0.19%	0.015%
50	16.733	2313	2320	2324	rBV4	25863	39159	0.89%	0.073%
51	16.798	2327	2331	2335	rBV7	14151	20758	0.47%	0.039%
52	16.910	2344	2350	2352	rBV5	16366	21198	0.48%	0.040%
53	17.015	2359	2368	2373	rBV7	41324	83546	1.90%	0.156%
54	17.068	2373	2377	2383	rVB	35383	56981	1.30%	0.107%
55	17.180	2391	2396	2399	rVB7	8602	12639	0.29%	0.024%
56	17.251	2402	2408	2412	rVV	2242565	3174460	72.38%	5.940%
57	17.292	2412	2415	2420	rVV	718269	994532	22.68%	1.861%
58	17.351	2420	2425	2430	rVV2	2121834	3009373	68.61%	5.631%
59	17.386	2430	2431	2437	rVV	203871	178419	4.07%	0.334%
60	17.445	2437	2441	2446	rVB6	58225	86234	1.97%	0.161%
61	17.657	2470	2477	2483	rVV	108374	179325	4.09%	0.336%
62	17.757	2490	2494	2495	rBV4	8265	9429	0.21%	0.018%
63	17.774	2495	2497	2498	rVV	12257	12440	0.28%	0.023%
64	17.804	2499	2502	2516	rVB5	30611	74793	1.71%	0.140%
65	17.927	2519	2523	2527	rVB6	18679	24191	0.55%	0.045%
66	17.968	2527	2530	2535	rBV5	6602	11305	0.26%	0.021%
67	18.133	2552	2558	2559	rBV	62115	87762	2.00%	0.164%
68	18.174	2562	2565	2570	rVV	91039	134659	3.07%	0.252%
69	18.227	2572	2574	2576	rVV	14854	16476	0.38%	0.031%
70	18.257	2576	2579	2584	rVB2	28701	36836	0.84%	0.069%
71	18.327	2585	2591	2595	rVV2	112782	191784	4.37%	0.359%
72	18.362	2595	2597	2603	rVB2	42260	46032	1.05%	0.086%
73	18.439	2606	2610	2613	rBV6	12501	21158	0.48%	0.040%
74	18.480	2613	2617	2621	rBV5	26314	40544	0.92%	0.076%
75	18.633	2639	2643	2647	rBV	55465	80292	1.83%	0.150%
76	18.674	2647	2650	2654	rVB3	24897	34135	0.78%	0.064%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
 Data File : BM035997.D
 Acq On : 29 Jul 2022 17:53
 Operator : CG/JU
 Sample : N3790-22
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBUL8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

77	18.751	2660	2663	2668	rVB2	31518	40375	0.92%	0.076%
78	18.874	2681	2684	2688	rBV5	14134	18496	0.42%	0.035%
79	18.921	2690	2692	2696	rVB	12023	10895	0.25%	0.020%
80	19.045	2709	2713	2718	rBV4	37603	64769	1.48%	0.121%
81	19.209	2734	2741	2745	rVB5	39714	75099	1.71%	0.141%
82	19.309	2749	2758	2766	rBV	1223006	1580014	36.02%	2.957%
83	19.404	2772	2774	2781	rVB5	16079	23046	0.53%	0.043%
84	19.551	2795	2799	2802	rBV2	52131	69802	1.59%	0.131%
85	19.645	2809	2815	2818	rBV	2847149	4156066	94.76%	7.777%
86	19.739	2828	2831	2839	rVB2	37711	56474	1.29%	0.106%
87	19.851	2847	2850	2857	rBV2	40337	63490	1.45%	0.119%
88	19.998	2870	2875	2880	rBV4	48364	109286	2.49%	0.205%
89	20.051	2882	2884	2888	rVB2	34183	33968	0.77%	0.064%
90	20.162	2900	2903	2912	rVB	169320	219480	5.00%	0.411%
91	20.262	2917	2920	2924	rVB	143829	182635	4.16%	0.342%
92	20.362	2934	2937	2941	rVB2	42964	47259	1.08%	0.088%
93	20.645	2982	2985	2989	rVB	133591	137366	3.13%	0.257%
94	21.080	3055	3059	3062	rBV	116133	148804	3.39%	0.278%
95	21.150	3068	3071	3077	rBV3	137805	217638	4.96%	0.407%
96	21.427	3112	3118	3122	rBV2	2887418	4385981	100.00%	8.208%
97	21.468	3122	3125	3133	rVB	504038	649952	14.82%	1.216%
98	23.080	3394	3399	3404	rBV2	474597	1015568	23.15%	1.900%
99	23.644	3489	3495	3500	rBV2	1781201	3279921	74.78%	6.138%
100	23.797	3515	3521	3528	rBV2	1692040	3301841	75.28%	6.179%




Sum of corrected areas: 53438600

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM035997.D
Acq On : 29 Jul 2022 17:53
Operator : CG/JU
Sample : N3790-22
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBUL8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

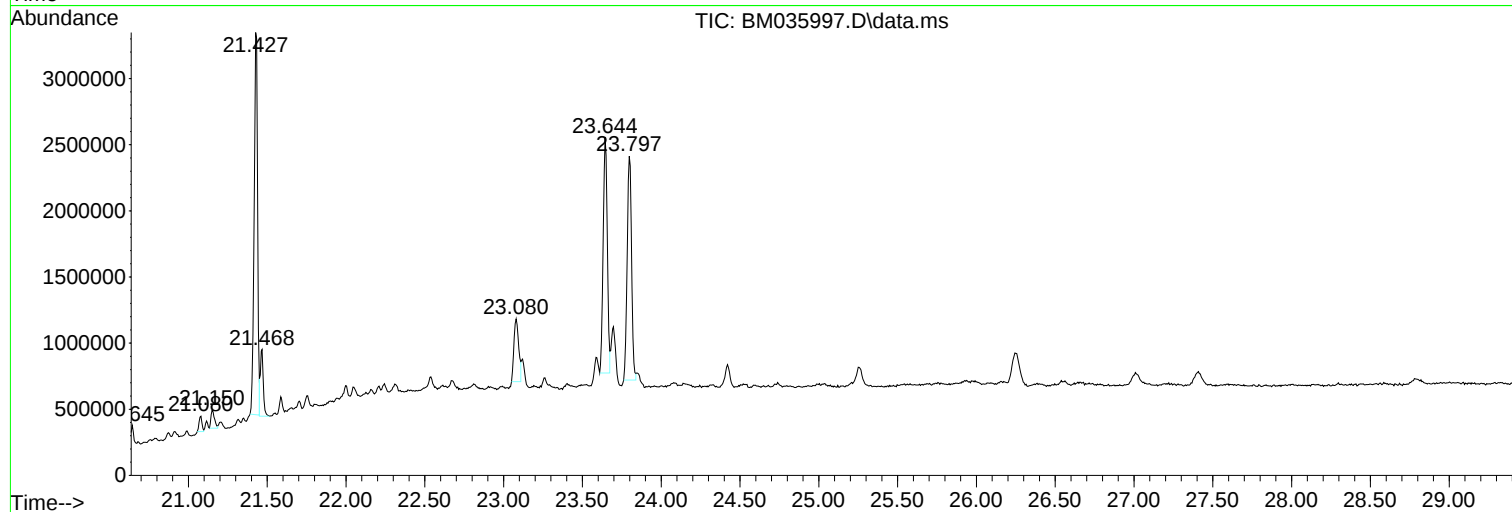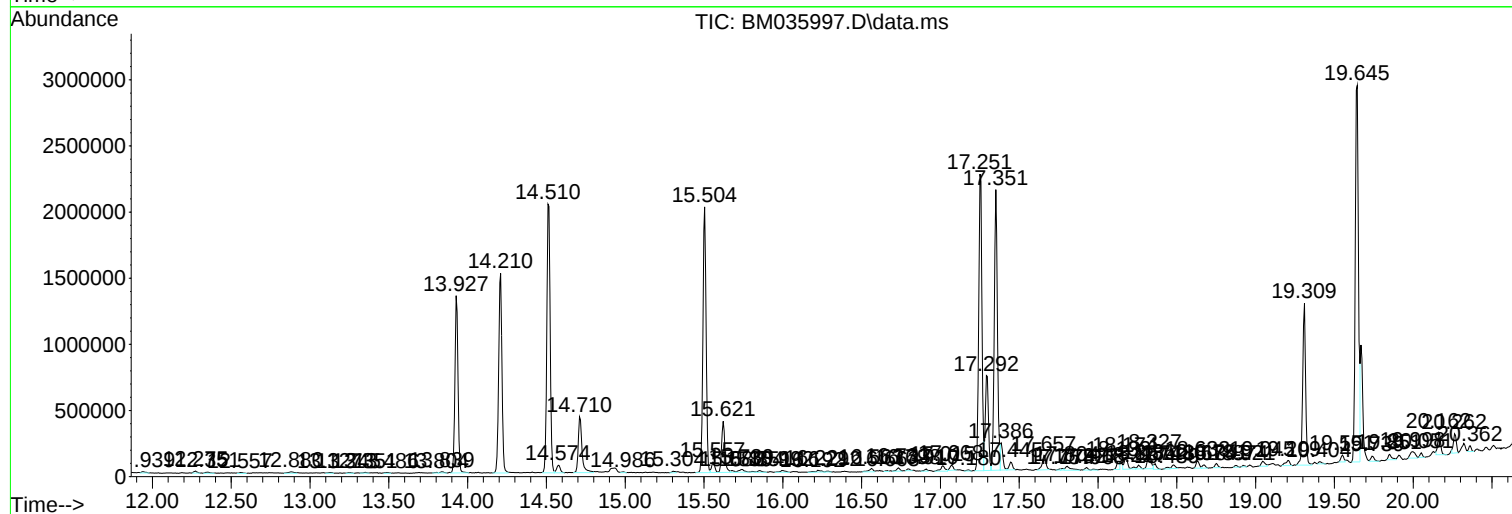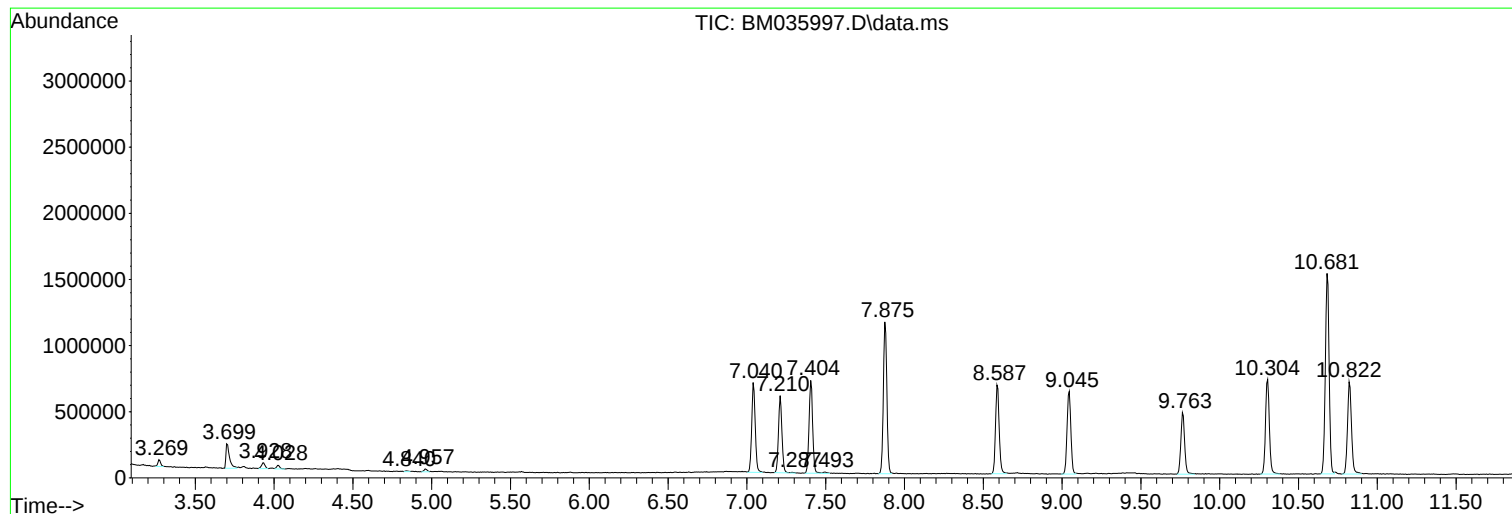

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM035997.D
Acq On : 29 Jul 2022 17:53
Operator : CG/JU
Sample : N3790-22
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBUL8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM035997.D
Acq On : 29 Jul 2022 17:53
Operator : CG/JU
Sample : N3790-22
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBUL8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc