

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
 Data File : BM035998.D
 Acq On : 29 Jul 2022 18:30
 Operator : CG/JU
 Sample : N3890-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YBEA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035998.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	21	26	30	rBV	500819	717372	10.67%	1.138%
2	3.699	101	104	114	rBV	374005	539845	8.03%	0.857%
3	3.934	140	144	149	rVB	34212	51040	0.76%	0.081%
4	4.028	157	160	167	rVB2	26273	35079	0.52%	0.056%
5	4.563	245	251	259	rVB	266503	394870	5.87%	0.627%
6	5.922	478	482	488	rBV8	5872	12632	0.19%	0.020%
7	7.040	666	672	682	rVB	210164	335282	4.98%	0.532%
8	7.210	695	701	713	rVB	1041535	1571551	23.36%	2.493%
9	7.404	728	734	745	rBV	912521	1405383	20.89%	2.230%
10	7.493	747	749	754	rVB5	5618	7067	0.11%	0.011%
11	7.875	806	814	822	rBV	1093719	1697701	25.24%	2.694%
12	8.587	928	935	947	rBV	616609	1000537	14.88%	1.587%
13	9.045	1004	1013	1022	rBV	1130003	1819740	27.05%	2.887%
14	9.210	1037	1041	1045	rVB7	5442	9183	0.14%	0.015%
15	9.763	1128	1135	1145	rBV	780719	1304689	19.40%	2.070%
16	10.304	1219	1227	1237	rBV	1146758	1924815	28.62%	3.054%
17	10.681	1284	1291	1300	rBV	1432985	2362663	35.13%	3.749%
18	10.822	1307	1315	1328	rBV	1144426	1941029	28.86%	3.080%
19	11.098	1356	1362	1367	rVB8	3706	8879	0.13%	0.014%
20	11.339	1400	1403	1406	rBV5	4809	7064	0.11%	0.011%
21	11.886	1491	1496	1498	rBV5	5160	7151	0.11%	0.011%
22	11.945	1501	1506	1515	rVB7	10561	24224	0.36%	0.038%
23	12.269	1556	1561	1570	rVB2	24928	45599	0.68%	0.072%
24	12.480	1593	1597	1602	rBV8	4137	7565	0.11%	0.012%
25	12.886	1662	1666	1669	rVB5	8785	12415	0.18%	0.020%
26	13.133	1702	1708	1710	rBV7	6375	10172	0.15%	0.016%
27	13.345	1739	1744	1748	rVB7	5131	6945	0.10%	0.011%
28	13.486	1761	1768	1774	rBV8	6301	11782	0.18%	0.019%
29	13.927	1836	1843	1855	rBV	2254406	3135420	46.61%	4.975%
30	14.210	1881	1891	1901	rBV	2573659	3756984	55.86%	5.961%
31	14.304	1905	1907	1914	rVB8	4052	6995	0.10%	0.011%
32	14.416	1922	1926	1931	rVB8	4967	7954	0.12%	0.013%
33	14.516	1936	1943	1951	rBV	1885629	2779713	41.33%	4.410%
34	14.716	1971	1977	1992	rBV	160521	298865	4.44%	0.474%
35	14.874	2000	2004	2008	rVB7	4562	6752	0.10%	0.011%
36	14.933	2011	2014	2021	rVB8	7918	13286	0.20%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
 Data File : BM035998.D
 Acq On : 29 Jul 2022 18:30
 Operator : CG/JU
 Sample : N3890-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YBEA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	15.257	2064	2069	2074	rBV2	12753	21580	0.32%	0.034%
38	15.333	2074	2082	2087	rBV2	49614	93875	1.40%	0.149%
39	15.504	2103	2111	2118	rBV	3615863	4950238	73.60%	7.854%
40	15.551	2118	2119	2125	rVB5	7223	6768	0.10%	0.011%
41	15.621	2125	2131	2140	rBV	946731	1276776	18.98%	2.026%
42	15.739	2146	2151	2159	rVB2	36647	62175	0.92%	0.099%
43	16.063	2203	2206	2214	rBV8	5554	9810	0.15%	0.016%
44	16.192	2222	2228	2229	rBV6	6290	10944	0.16%	0.017%
45	16.280	2239	2243	2248	rVB4	10597	15567	0.23%	0.025%
46	16.557	2287	2290	2293	rBV5	7490	11996	0.18%	0.019%
47	16.733	2315	2320	2325	rBV2	27330	40040	0.60%	0.064%
48	16.798	2328	2331	2337	rVB9	6007	7832	0.12%	0.012%
49	17.015	2364	2368	2373	rBV5	25186	43573	0.65%	0.069%
50	17.251	2402	2408	2416	rBV	2120103	2945076	43.78%	4.673%
51	17.351	2418	2425	2437	rVV2	4175543	5765730	85.72%	9.148%
52	17.545	2454	2458	2464	rVB	35945	46409	0.69%	0.074%
53	17.633	2467	2473	2474	rBV5	8111	14115	0.21%	0.022%
54	17.804	2499	2502	2509	rVB3	24694	40555	0.60%	0.064%
55	17.927	2519	2523	2528	rBV2	33711	42759	0.64%	0.068%
56	18.151	2557	2561	2565	rBV5	23753	32425	0.48%	0.051%
57	18.227	2570	2574	2578	rVV	42292	49216	0.73%	0.078%
58	18.751	2659	2663	2669	rBV	26731	38207	0.57%	0.061%
59	19.209	2737	2741	2746	rVB3	45767	66444	0.99%	0.105%
60	19.280	2749	2753	2756	rBV	48132	63652	0.95%	0.101%
61	19.339	2761	2763	2768	rVB4	14963	17300	0.26%	0.027%
62	19.580	2801	2804	2808	rVB5	18335	19974	0.30%	0.032%
63	19.645	2809	2815	2820	rBV	4873058	6598756	98.10%	10.470%
64	20.245	2914	2917	2921	rBV4	30963	42744	0.64%	0.068%
65	20.645	2982	2985	2990	rVB	126300	140794	2.09%	0.223%
66	21.433	3114	3119	3126	rBV	2501535	3206583	47.67%	5.088%
67	23.650	3489	3496	3503	rBV2	3580619	6726234	100.00%	10.672%
68	23.797	3515	3521	3531	rVB2	1698210	3340172	49.66%	5.300%




Sum of corrected areas: 63026562

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM035998.D
Acq On : 29 Jul 2022 18:30
Operator : CG/JU
Sample : N3890-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YBEA3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

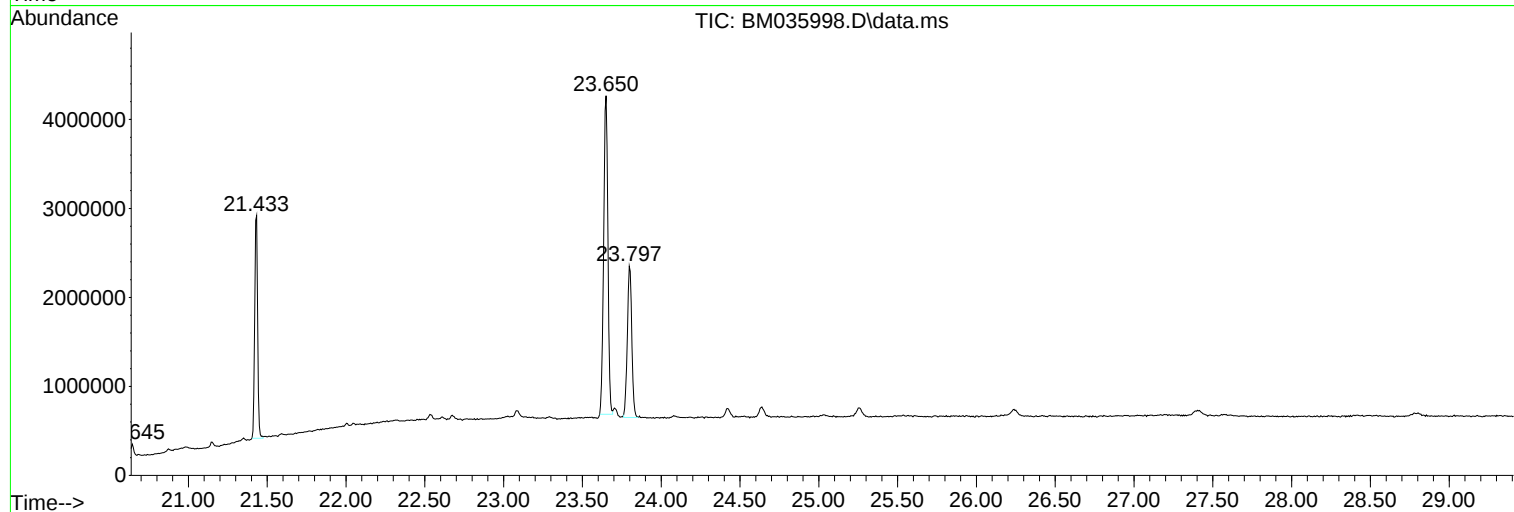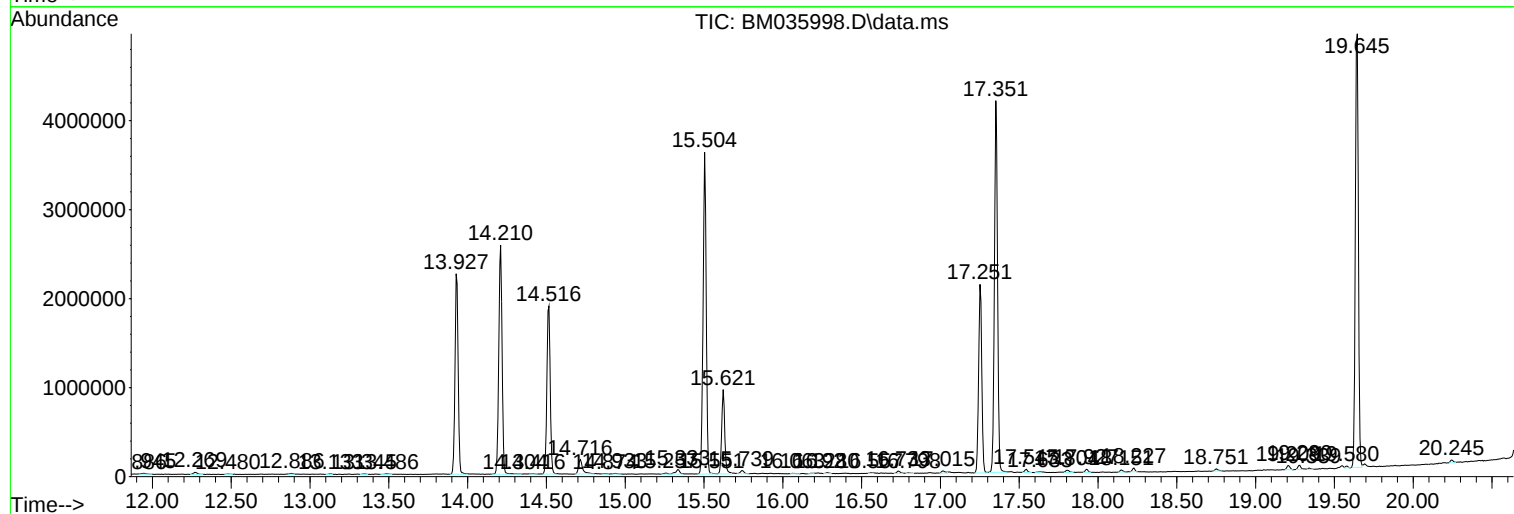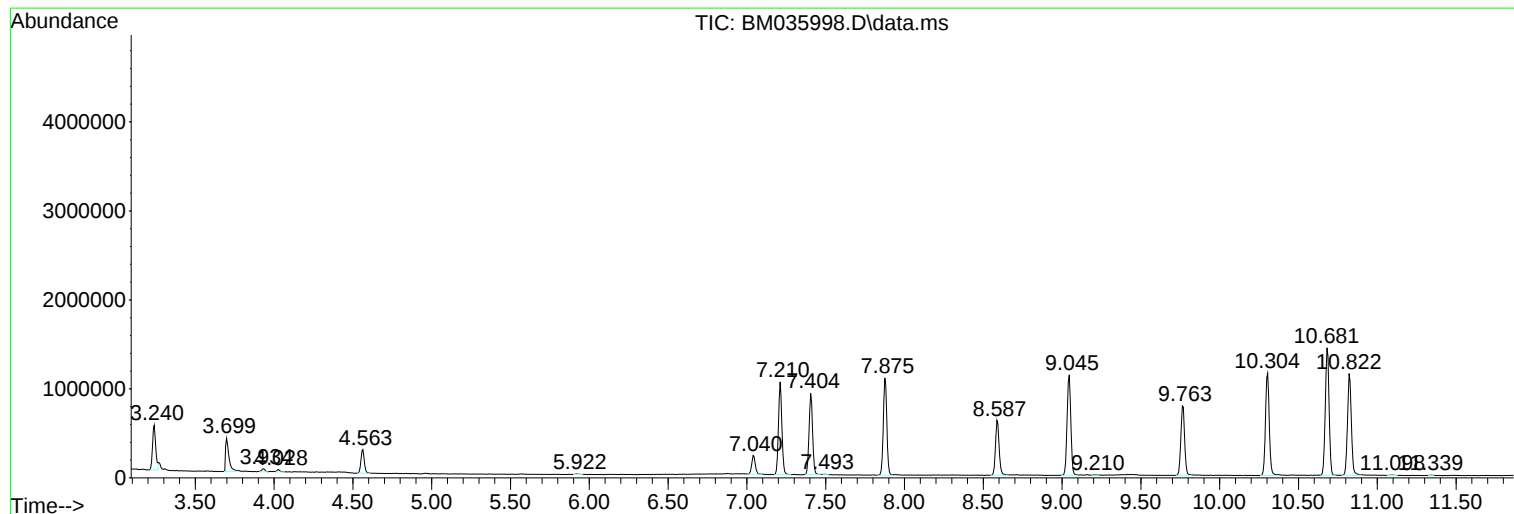

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM035998.D
Acq On : 29 Jul 2022 18:30
Operator : CG/JU
Sample : N3890-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YBEA3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM035998.D
Acq On : 29 Jul 2022 18:30
Operator : CG/JU
Sample : N3890-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YBEA3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc