

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
 Data File : BM036002.D
 Acq On : 29 Jul 2022 20:57
 Operator : CG/JU
 Sample : N3790-21
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBUL7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036002.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	39	rVB	75049	107585	2.07%	0.184%
2	3.699	100	104	116	rBV	319879	491501	9.46%	0.840%
3	3.928	138	143	149	rBV	54660	82105	1.58%	0.140%
4	4.022	156	159	165	rVB	27049	37795	0.73%	0.065%
5	4.957	314	318	324	rBV	27793	44284	0.85%	0.076%
6	5.563	417	421	425	rBV3	8891	13575	0.26%	0.023%
7	6.545	585	588	594	rVB6	8196	12149	0.23%	0.021%
8	7.040	665	672	684	rVB	989766	1519196	29.23%	2.596%
9	7.210	694	701	709	rVV	836296	1286074	24.75%	2.197%
10	7.287	709	714	721	rVB	11996	24881	0.48%	0.043%
11	7.404	726	734	745	rBV	1047712	1592926	30.65%	2.722%
12	7.492	746	749	753	rVB5	10226	13349	0.26%	0.023%
13	7.875	806	814	821	rBV	1060102	1643758	31.63%	2.809%
14	7.940	823	825	833	rVB8	5466	8806	0.17%	0.015%
15	8.587	929	935	944	rBV	967762	1550959	29.84%	2.650%
16	8.710	952	956	962	rVB6	9324	17353	0.33%	0.030%
17	9.039	1004	1012	1022	rBV	905283	1501193	28.89%	2.565%
18	9.151	1029	1031	1036	rVB6	7901	10501	0.20%	0.018%
19	9.392	1069	1072	1076	rBV6	4071	5605	0.11%	0.010%
20	9.451	1078	1082	1088	rVB9	6761	14441	0.28%	0.025%
21	9.763	1128	1135	1147	rBV	701058	1163500	22.39%	1.988%
22	10.298	1218	1226	1238	rBV	1060899	1811615	34.86%	3.095%
23	10.492	1254	1259	1264	rVB9	3921	6613	0.13%	0.011%
24	10.681	1283	1291	1298	rBV	1438223	2356058	45.34%	4.026%
25	10.822	1308	1315	1331	rBV	1073881	1836599	35.34%	3.138%
26	11.492	1422	1429	1430	rBV7	4241	7682	0.15%	0.013%
27	11.875	1488	1494	1497	rBV7	5213	8956	0.17%	0.015%
28	11.939	1500	1505	1514	rVB6	9811	25626	0.49%	0.044%
29	12.180	1542	1546	1547	rBV4	4355	5541	0.11%	0.009%
30	12.269	1556	1561	1568	rVB2	22084	35995	0.69%	0.062%
31	12.339	1570	1573	1578	rVV7	4560	5554	0.11%	0.009%
32	12.551	1608	1609	1616	rVB7	4413	7518	0.14%	0.013%
33	12.686	1629	1632	1635	rBV5	3800	5197	0.10%	0.009%
34	12.880	1657	1665	1671	rBV8	15925	32525	0.63%	0.056%
35	13.127	1703	1707	1713	rVB8	7898	12745	0.25%	0.022%
36	13.257	1723	1729	1731	rBV5	10612	17778	0.34%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
 Data File : BM036002.D
 Acq On : 29 Jul 2022 20:57
 Operator : CG/JU
 Sample : N3790-21
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBUL7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	13.280	1731	1733	1739	rVV6	9343	13990	0.27%	0.024%
38	13.345	1739	1744	1747	rVV6	4252	8340	0.16%	0.014%
39	13.392	1749	1752	1754	rVV3	4671	5405	0.10%	0.009%
40	13.492	1765	1769	1774	rVB8	5579	9138	0.18%	0.016%

41	13.798	1817	1821	1824	rBV6	4877	7649	0.15%	0.013%
42	13.839	1824	1828	1831	rVB6	8835	12633	0.24%	0.022%
43	13.927	1837	1843	1854	rBV	1949955	2627354	50.56%	4.489%
44	14.204	1884	1890	1901	rVB	2266521	3260066	62.73%	5.570%
45	14.357	1912	1916	1920	rVB6	8835	13140	0.25%	0.022%

46	14.416	1920	1926	1928	rBV7	6150	7758	0.15%	0.013%
47	14.510	1935	1942	1949	rBV	2022929	2963388	57.02%	5.064%
48	14.580	1949	1954	1960	rVB7	21017	35139	0.68%	0.060%
49	14.710	1968	1976	1991	rBV	637624	1043567	20.08%	1.783%
50	14.827	1992	1996	2002	rVB3	15006	27751	0.53%	0.047%

51	14.933	2008	2014	2020	rVB4	41730	70677	1.36%	0.121%
52	14.986	2020	2023	2028	rVB6	4872	7437	0.14%	0.013%
53	15.139	2044	2049	2052	rBV7	3303	7297	0.14%	0.012%
54	15.310	2073	2078	2085	rBV5	12562	31347	0.60%	0.054%
55	15.363	2085	2087	2090	rVB4	7293	6867	0.13%	0.012%

56	15.504	2104	2111	2118	rBV	2844495	4096733	78.83%	7.000%
57	15.551	2118	2119	2125	rVB3	13066	17228	0.33%	0.029%
58	15.621	2125	2131	2139	rBV	599627	835066	16.07%	1.427%
59	15.739	2147	2151	2158	rVB2	29059	48860	0.94%	0.083%
60	15.845	2161	2169	2172	rBV9	9887	20429	0.39%	0.035%

61	15.921	2178	2182	2185	rBV6	5841	7186	0.14%	0.012%
62	15.986	2189	2193	2201	rVB7	21564	36614	0.70%	0.063%
63	16.068	2203	2207	2211	rBV7	4649	6832	0.13%	0.012%
64	16.180	2222	2226	2227	rBV4	5620	6007	0.12%	0.010%
65	16.227	2230	2234	2240	rVB8	14360	27497	0.53%	0.047%

66	16.568	2288	2292	2295	rBV6	5973	8113	0.16%	0.014%
67	16.733	2315	2320	2324	rVV3	29539	42145	0.81%	0.072%
68	16.798	2327	2331	2338	rVB3	24144	32871	0.63%	0.056%
69	17.015	2364	2368	2371	rBV4	21578	32642	0.63%	0.056%
70	17.074	2374	2378	2380	rVB5	7265	11685	0.22%	0.020%

71	17.251	2402	2408	2413	rBV	2421186	3288977	63.29%	5.620%
72	17.292	2413	2415	2419	rVV	110398	140985	2.71%	0.241%
73	17.351	2419	2425	2436	rVV	3055389	4229992	81.40%	7.228%
74	17.445	2437	2441	2448	rVB4	47752	69875	1.34%	0.119%
75	17.751	2491	2493	2496	rBV4	5256	6720	0.13%	0.011%

76	17.804	2499	2502	2507	rVB	25291	30405	0.59%	0.052%
----	--------	------	------	------	-----	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
 Data File : BM036002.D
 Acq On : 29 Jul 2022 20:57
 Operator : CG/JU
 Sample : N3790-21
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBUL7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

77	17.927	2519	2523	2528	rVB	77852	94698	1.82%	0.162%
78	18.027	2537	2540	2545	rVB7	8171	11234	0.22%	0.019%
79	18.151	2552	2561	2569	rBV2	89913	181042	3.48%	0.309%
80	18.221	2571	2573	2577	rVB	14747	18032	0.35%	0.031%
81	18.321	2586	2590	2594	rBV3	14242	23960	0.46%	0.041%
82	18.633	2640	2643	2647	rVB5	16775	21909	0.42%	0.037%
83	18.751	2660	2663	2670	rVB3	26321	36345	0.70%	0.062%
84	19.104	2720	2723	2727	rVB5	28531	31781	0.61%	0.054%
85	19.203	2737	2740	2744	rVB3	38370	50843	0.98%	0.087%
86	19.274	2749	2752	2754	rVV	41759	51372	0.99%	0.088%
87	19.303	2754	2757	2766	rVB	157803	226568	4.36%	0.387%
88	19.545	2796	2798	2802	rBV2	24074	29892	0.58%	0.051%
89	19.639	2809	2814	2828	rBV	3709468	5196847	100.00%	8.880%
90	20.645	2981	2985	2988	rBV	138066	154246	2.97%	0.264%
91	21.145	3067	3070	3077	rBV4	150629	225791	4.34%	0.386%
92	21.427	3113	3118	3123	rBV	2765650	3501155	67.37%	5.982%
93	23.644	3488	3495	3501	rBV2	2471774	4757049	91.54%	8.128%
94	23.797	3514	3521	3536	rVB2	1723194	3438316	66.16%	5.875%




Sum of corrected areas: 58524423

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM036002.D
Acq On : 29 Jul 2022 20:57
Operator : CG/JU
Sample : N3790-21
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBUL7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

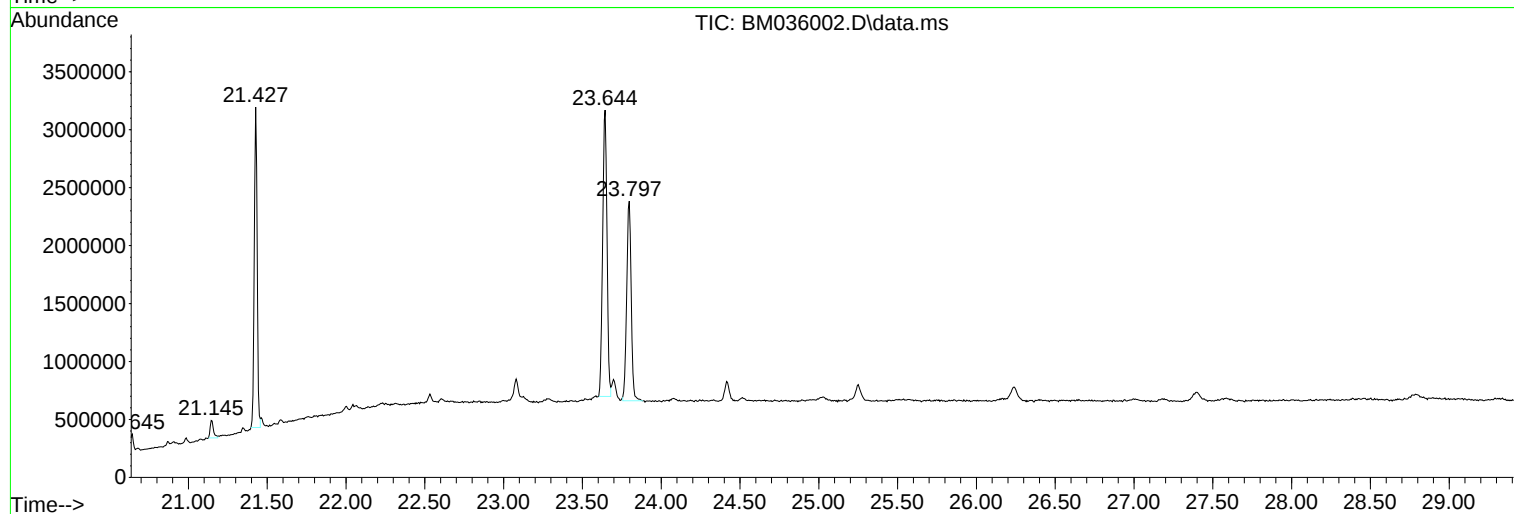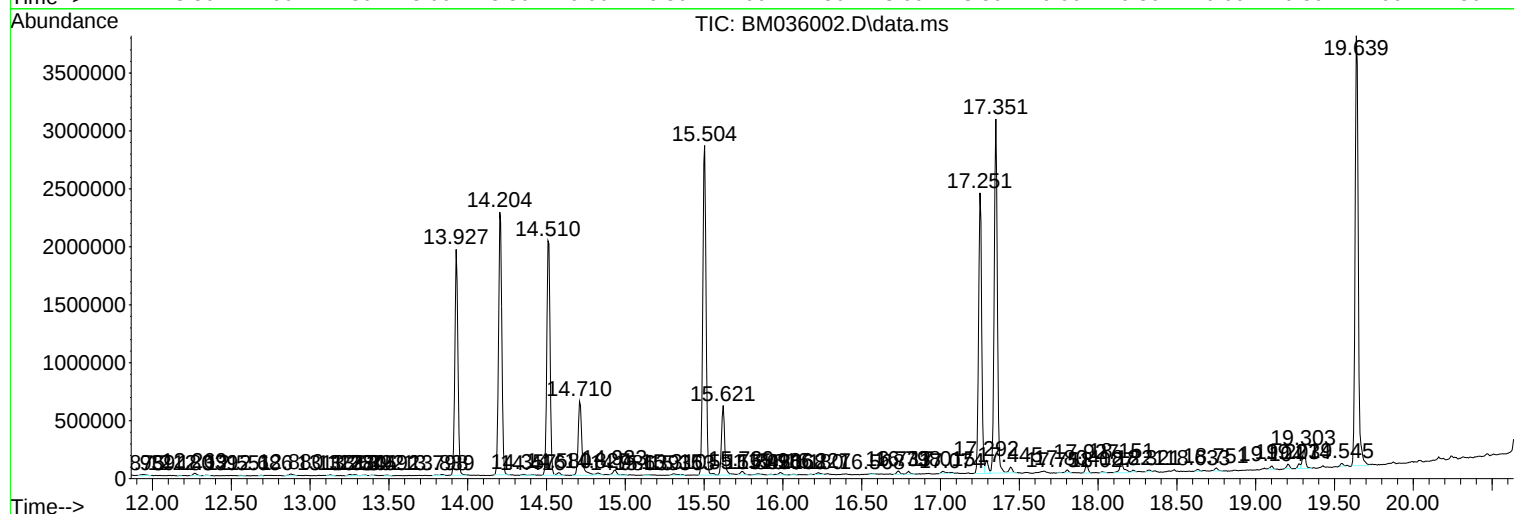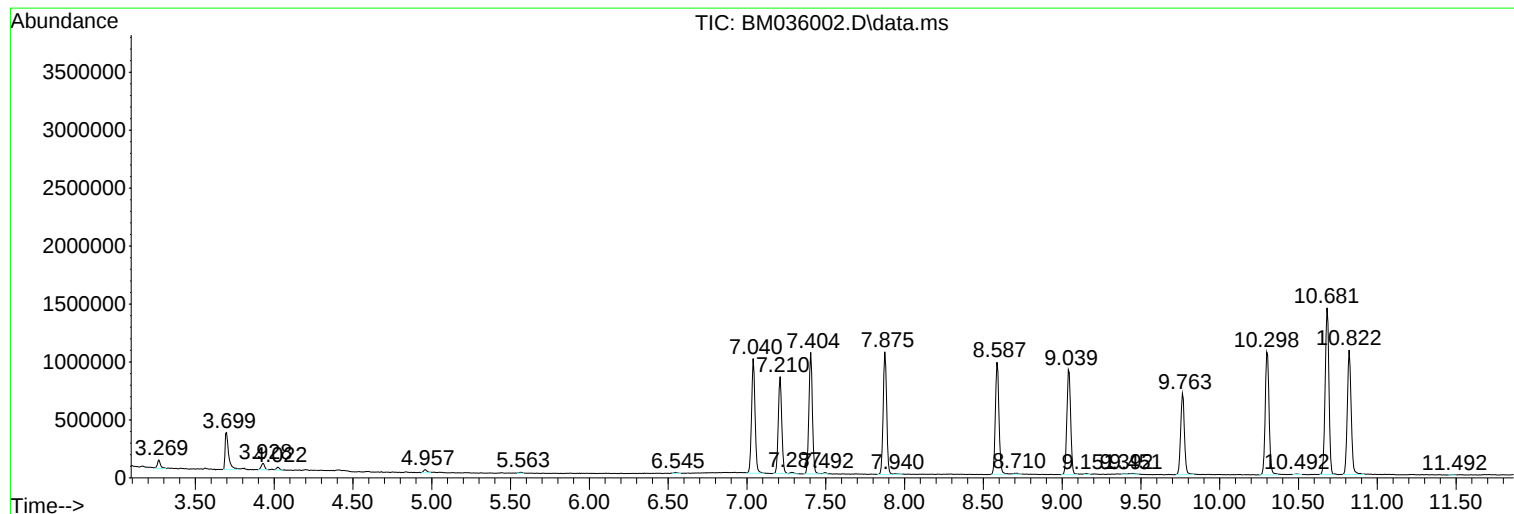

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM036002.D
Acq On : 29 Jul 2022 20:57
Operator : CG/JU
Sample : N3790-21
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBUL7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM036002.D
Acq On : 29 Jul 2022 20:57
Operator : CG/JU
Sample : N3790-21
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBUL7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc