

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM036004.D
Acq On : 29 Jul 2022 22:10
Operator : CG/JU
Sample : N3790-23
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBUM1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Title : SVOA CALIBRATION

Signal : TIC: BM036004.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	36	rVB	67224	81880	1.69%	0.148%
2	3.704	102	105	119	rVB	130697	205489	4.25%	0.370%
3	3.928	139	143	149	rVB	55680	77872	1.61%	0.140%
4	4.022	156	159	163	rVB	22274	28679	0.59%	0.052%
5	4.404	221	224	227	rBV5	9057	14047	0.29%	0.025%
6	4.840	296	298	301	rVB4	6817	7019	0.15%	0.013%
7	4.957	314	318	325	rVB	22394	33852	0.70%	0.061%
8	5.569	419	422	428	rVB6	8661	13222	0.27%	0.024%
9	7.040	665	672	686	rVB	878267	1345735	27.81%	2.426%
10	7.210	695	701	709	rVV	750795	1136443	23.49%	2.049%
11	7.287	712	714	719	rVB2	9971	15535	0.32%	0.028%
12	7.404	726	734	745	rBV	914012	1411331	29.17%	2.545%
13	7.492	747	749	754	rVB6	8787	11634	0.24%	0.021%
14	7.875	807	814	822	rBV	1126404	1703299	35.20%	3.071%
15	7.945	824	826	832	rVB7	5405	7662	0.16%	0.014%
16	8.586	927	935	945	rBV	972927	1562678	32.29%	2.818%
17	8.710	952	956	961	rBV5	8365	12169	0.25%	0.022%
18	9.045	1005	1013	1023	rBV	795903	1331794	27.52%	2.401%
19	9.204	1037	1040	1046	rVB7	6942	8233	0.17%	0.015%
20	9.457	1079	1083	1085	rVV5	7862	10758	0.22%	0.019%
21	9.763	1128	1135	1148	rVV	584890	979811	20.25%	1.767%
22	10.298	1219	1226	1242	rBV	936186	1596255	32.99%	2.878%
23	10.680	1284	1291	1299	rBV	1522387	2472765	51.10%	4.458%
24	10.822	1305	1315	1331	rBV	934045	1627439	33.63%	2.934%
25	10.928	1331	1333	1338	rVB6	4098	5709	0.12%	0.010%
26	11.063	1353	1356	1361	rBV6	4623	8433	0.17%	0.015%
27	11.939	1504	1505	1510	rVB5	7569	9147	0.19%	0.016%
28	12.274	1557	1562	1569	rVB2	17586	32225	0.67%	0.058%
29	12.486	1594	1598	1602	rBV7	4167	6574	0.14%	0.012%
30	12.522	1602	1604	1609	rVV5	5066	5660	0.12%	0.010%
31	12.874	1659	1664	1669	rBV7	8831	17873	0.37%	0.032%
32	13.127	1701	1707	1712	rBV8	9951	14912	0.31%	0.027%
33	13.339	1738	1743	1744	rBV5	4711	6083	0.13%	0.011%
34	13.421	1752	1757	1760	rVB7	4186	6975	0.14%	0.013%
35	13.486	1764	1768	1772	rVB5	4803	7966	0.16%	0.014%
36	13.798	1816	1821	1823	rBV6	6222	9797	0.20%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
 Data File : BM036004.D
 Acq On : 29 Jul 2022 22:10
 Operator : CG/JU
 Sample : N3790-23
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBUM1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	13.839	1826	1828	1833	rVV6	7621	10880	0.22%	0.020%
38	13.927	1836	1843	1859	rVV	1815712	2465768	50.96%	4.446%
39	14.074	1865	1868	1873	rVB7	3042	5561	0.11%	0.010%
40	14.210	1880	1891	1902	rBV	2059451	2999882	62.00%	5.409%
41	14.410	1920	1925	1930	rVB8	7031	9241	0.19%	0.017%
42	14.516	1935	1943	1953	rBV	2117629	3157415	65.25%	5.693%
43	14.710	1969	1976	1991	rBV	524160	862181	17.82%	1.555%
44	14.933	2010	2014	2019	rVB3	41719	55075	1.14%	0.099%
45	15.310	2073	2078	2080	rBV3	13626	18983	0.39%	0.034%
46	15.504	2104	2111	2120	rBV	2784097	3860238	79.78%	6.960%
47	15.621	2124	2131	2144	rVV	429350	627043	12.96%	1.131%
48	15.745	2147	2152	2156	rVB2	27193	40869	0.84%	0.074%
49	15.868	2171	2173	2179	rBV7	5375	7256	0.15%	0.013%
50	15.921	2179	2182	2185	rVB4	6049	6642	0.14%	0.012%
51	16.062	2202	2206	2212	rBV8	9373	18589	0.38%	0.034%
52	16.121	2212	2216	2220	rVV7	3993	6229	0.13%	0.011%
53	16.186	2220	2227	2229	rVV6	7244	9440	0.20%	0.017%
54	16.215	2230	2232	2237	rVV5	10408	18307	0.38%	0.033%
55	16.286	2240	2244	2250	rVV8	11162	15271	0.32%	0.028%
56	16.392	2258	2262	2267	rBV8	6737	14565	0.30%	0.026%
57	16.509	2276	2282	2283	rBV6	4265	7400	0.15%	0.013%
58	16.562	2288	2291	2295	rBV6	8771	12331	0.25%	0.022%
59	16.657	2304	2307	2313	rVB8	7739	10703	0.22%	0.019%
60	16.733	2315	2320	2325	rBV	26857	41159	0.85%	0.074%
61	16.798	2327	2331	2335	rBV3	18158	25803	0.53%	0.047%
62	17.015	2364	2368	2371	rBV4	22758	31531	0.65%	0.057%
63	17.174	2392	2395	2401	rVB7	16649	20608	0.43%	0.037%
64	17.251	2401	2408	2416	rBV	2638607	3551884	73.40%	6.404%
65	17.351	2418	2425	2435	rVV	2964488	4050138	83.70%	7.302%
66	17.445	2437	2441	2446	rVB3	45588	68680	1.42%	0.124%
67	17.545	2455	2458	2460	rBV3	8031	7734	0.16%	0.014%
68	17.633	2471	2473	2480	rVB8	7379	12843	0.27%	0.023%
69	17.804	2497	2502	2506	rBV2	22446	33766	0.70%	0.061%
70	17.927	2519	2523	2532	rVB2	49595	62025	1.28%	0.112%
71	18.021	2536	2539	2543	rVV5	11221	19060	0.39%	0.034%
72	18.145	2556	2560	2565	rBV	80106	110570	2.29%	0.199%
73	18.221	2570	2573	2579	rVV2	17960	25624	0.53%	0.046%
74	18.445	2609	2611	2612	rBV2	8369	6814	0.14%	0.012%
75	18.480	2614	2617	2621	rVB5	16269	26054	0.54%	0.047%
76	18.751	2659	2663	2671	rVB2	24380	36818	0.76%	0.066%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
 Data File : BM036004.D
 Acq On : 29 Jul 2022 22:10
 Operator : CG/JU
 Sample : N3790-23
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBUM1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

77	19.203	2737	2740	2747	rVB	38499	54741	1.13%	0.099%
78	19.274	2749	2752	2755	rBV	37428	50976	1.05%	0.092%
79	19.303	2755	2757	2761	rVB4	18348	19057	0.39%	0.034%
80	19.545	2795	2798	2801	rBV3	23999	28919	0.60%	0.052%
81	19.639	2808	2814	2821	rBV	3595371	4838817	100.00%	8.724%
82	20.645	2982	2985	2989	rVB	113904	119466	2.47%	0.215%
83	21.144	3067	3070	3077	rBV3	157957	213196	4.41%	0.384%
84	21.427	3113	3118	3129	rBV	2884598	3735478	77.20%	6.735%
85	23.644	3488	3495	3501	rBV2	2408999	4527320	93.56%	8.163%
86	23.797	3514	3521	3530	rVB2	1834356	3676951	75.99%	6.630%




Sum of corrected areas: 55462856

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM036004.D
Acq On : 29 Jul 2022 22:10
Operator : CG/JU
Sample : N3790-23
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBUM1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

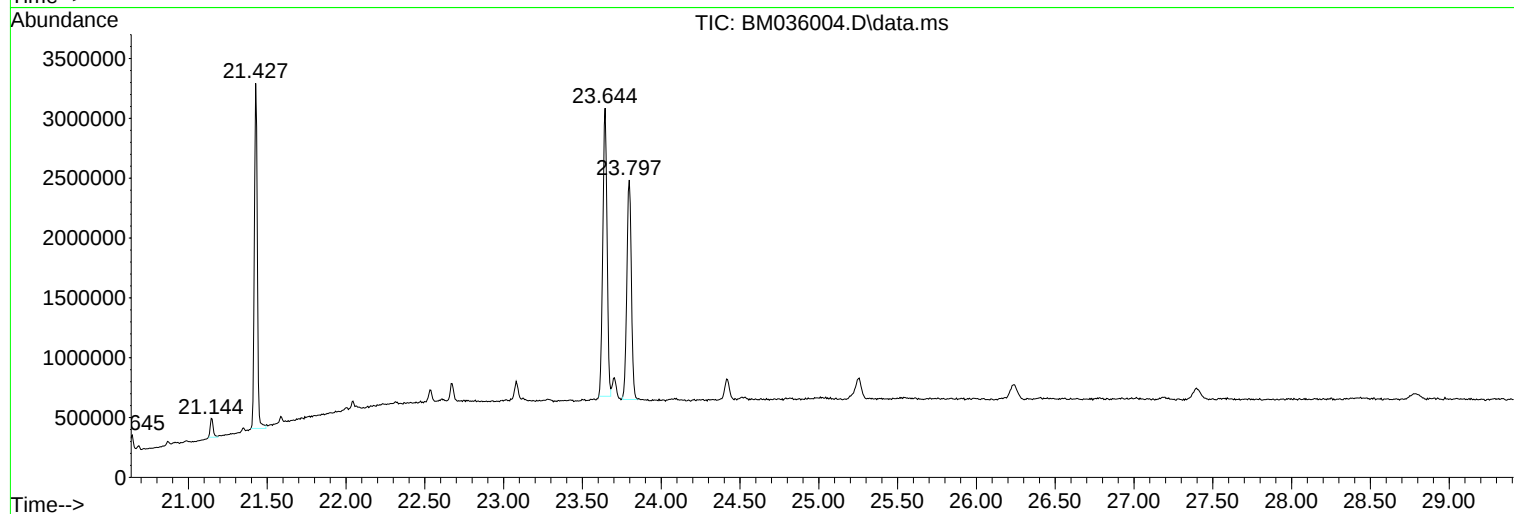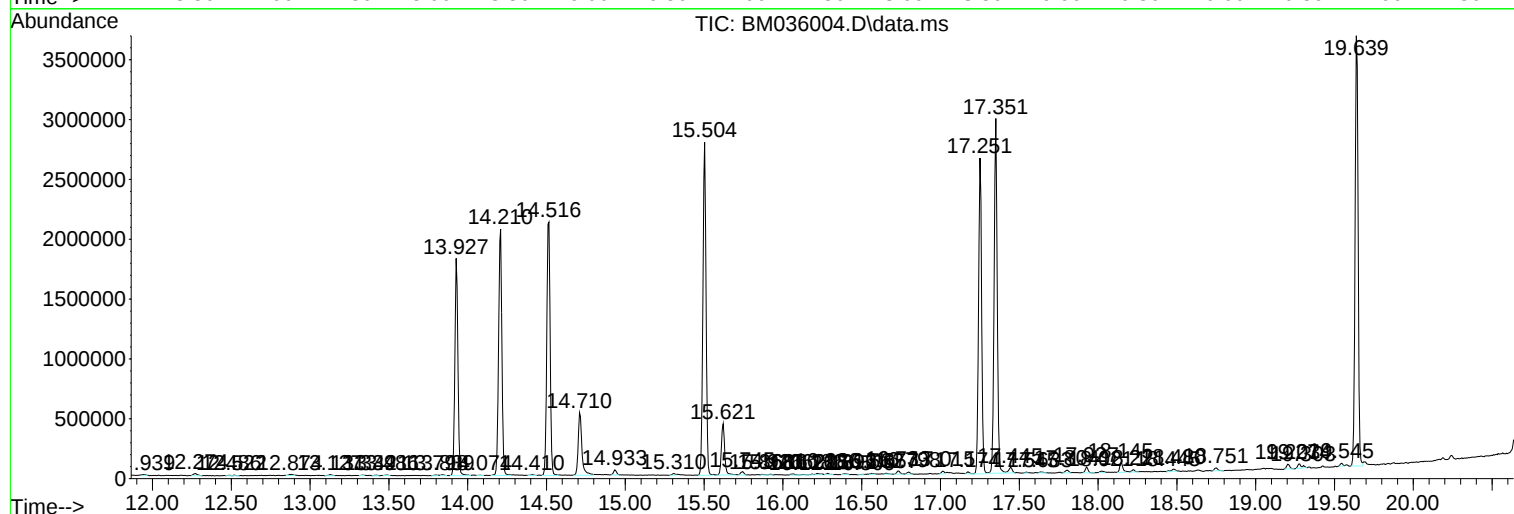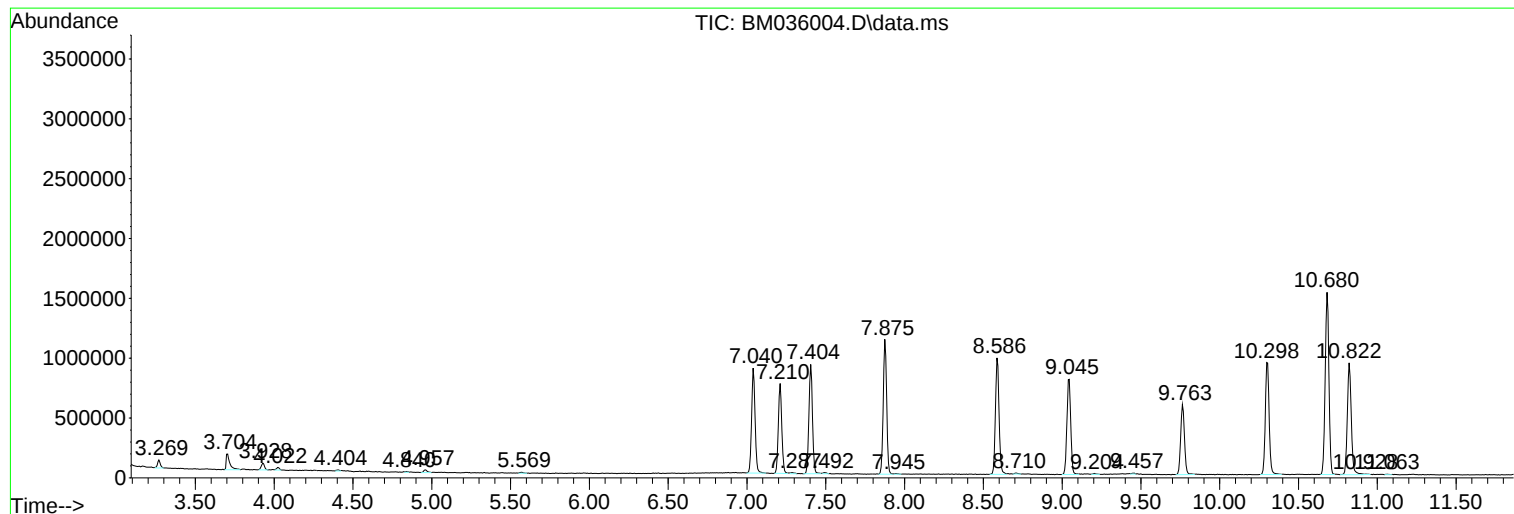

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM036004.D
Acq On : 29 Jul 2022 22:10
Operator : CG/JU
Sample : N3790-23
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBUM1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM036004.D
Acq On : 29 Jul 2022 22:10
Operator : CG/JU
Sample : N3790-23
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBUM1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc